



US 20200240977A1

(19) **United States**

(12) **Patent Application Publication**  
**Ingber et al.**

(10) **Pub. No.: US 2020/0240977 A1**

(43) **Pub. Date: Jul. 30, 2020**

(54) **SYSTEM FOR CONDUCTING THE IDENTIFICATION OF BACTERIA IN URINE**

(71) Applicant: **POCARED Diagnostics LTD.**,  
Rehovot (IL)

(72) Inventors: **Gal Ingber**, Oranit (IL); **William G. Atterbury**, Columbus, OH (US); **Russell H. Barnes**, Columbus, OH (US); **Douglas E. Boyd**, Columbus, OH (US); **Joseph D. Dennis**, Granview Heights, OH (US); **Jonathan Gurfinkel**, Omer (IL); **Dave Holley**, Lancaster, OH (US); **Steven E. Huckaby**, Blacklick, OH (US); **Thomas A. Klausung**, Powell, OH (US); **John S. Laudo**, Columbus, OH (US); **Kevin Sadeski**, Canal Winchester, OH (US); **Jason A. Schaefer**, Coral Springs, FL (US); **K. Bryan Scott**, Westerville, OH (US); **Carol Stillman**, Powell, OH (US); **Sherwood Talbert**, Columbus, OH (US); **John Tallarico**, Powell, OH (US)

(21) Appl. No.: **16/842,061**

(22) Filed: **Apr. 7, 2020**

**Related U.S. Application Data**

(60) Continuation of application No. 15/425,253, filed on Feb. 6, 2017, now Pat. No. 10,656,140, which is a division of application No. 14/330,450, filed on Jul. 14, 2014, now Pat. No. 9,606,105, which is a continuation of application No. 12/682,402, filed on Sep. 15, 2010, now Pat. No. 8,808,649, filed as application No. PCT/US2008/079533 on Oct. 10, 2008.

(60) Provisional application No. 60/978,810, filed on Oct. 10, 2007, provisional application No. 60/978,820, filed on Oct. 10, 2007, provisional application No. 60/978,856, filed on Oct. 10, 2007, provisional application No. 60/978,862, filed on Oct. 10, 2007.


**Publication Classification**

(51) **Int. Cl.**  
*G01N 33/493* (2006.01)  
*C12Q 1/04* (2006.01)  
*G01N 21/03* (2006.01)  
*G01N 35/02* (2006.01)  
*G01N 35/04* (2006.01)

(52) **U.S. Cl.**  
CPC ..... *G01N 33/493* (2013.01); *C12Q 1/04* (2013.01); *G01N 2021/6482* (2013.01); *G01N 35/025* (2013.01); *G01N 35/04* (2013.01); *G01N 21/0303* (2013.01)

(57) **ABSTRACT**

A system for conducting the identification and quantification of micro-organisms, e.g., bacteria in urine samples which includes: 1) several disposable cartridges for holding four disposable components including a centrifuge tube, a pipette tip having a 1 ml volume, a second pipette tip having a 0.5 ml volume, and an optical cup or cuvette; 2) a sample processor for receiving the disposable cartridges and processing the urine samples including transferring the processed urine sample to the optical cups; and 3) an optical analyzer for receiving the disposable cartridges and configured to analyze the type and quantity of micro-organisms in the urine sample. The disposable cartridges with their components including the optical cups or cuvettes are used in the sample processor, and the optical cups or cuvettes containing the processed urine samples are used in the optical analyzer for identifying and quantifying the type of micro-organism existing in the processed urine samples.

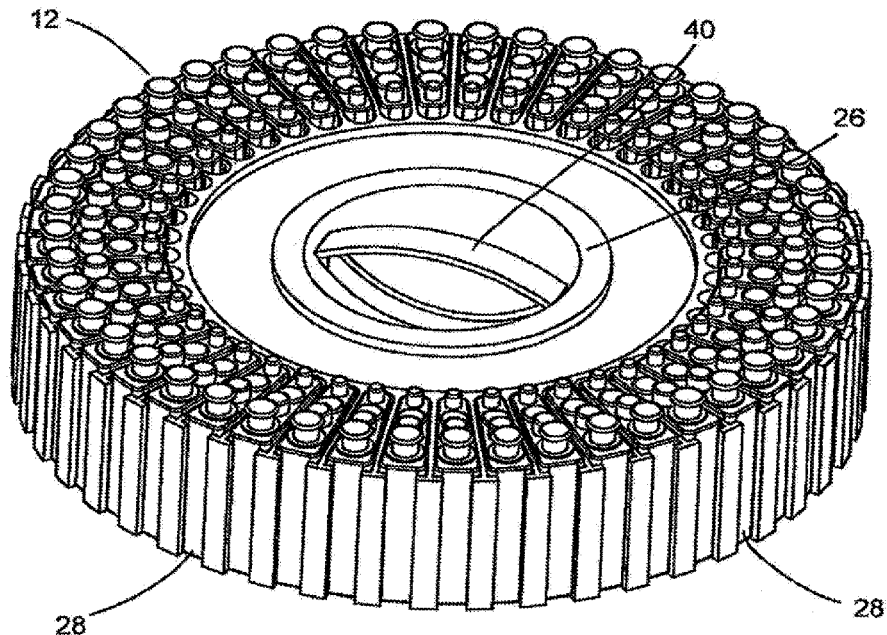

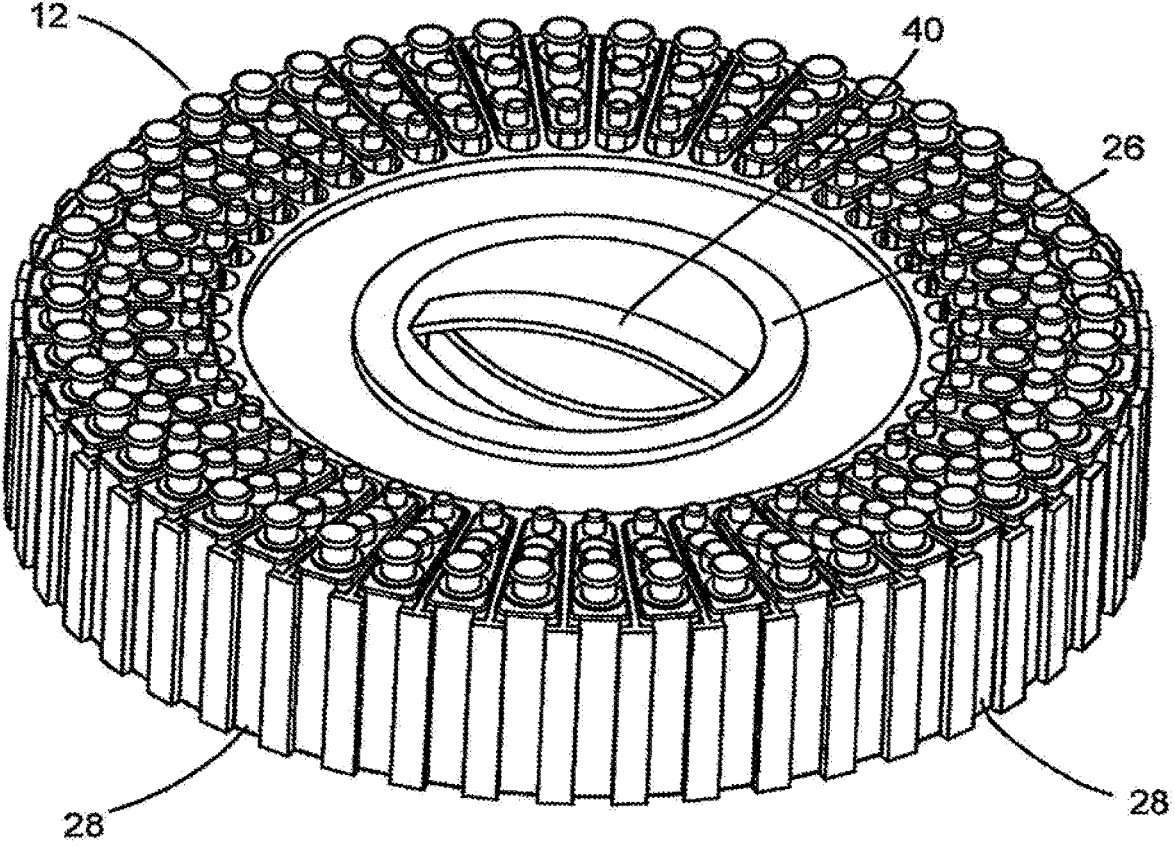


FIG. 1A

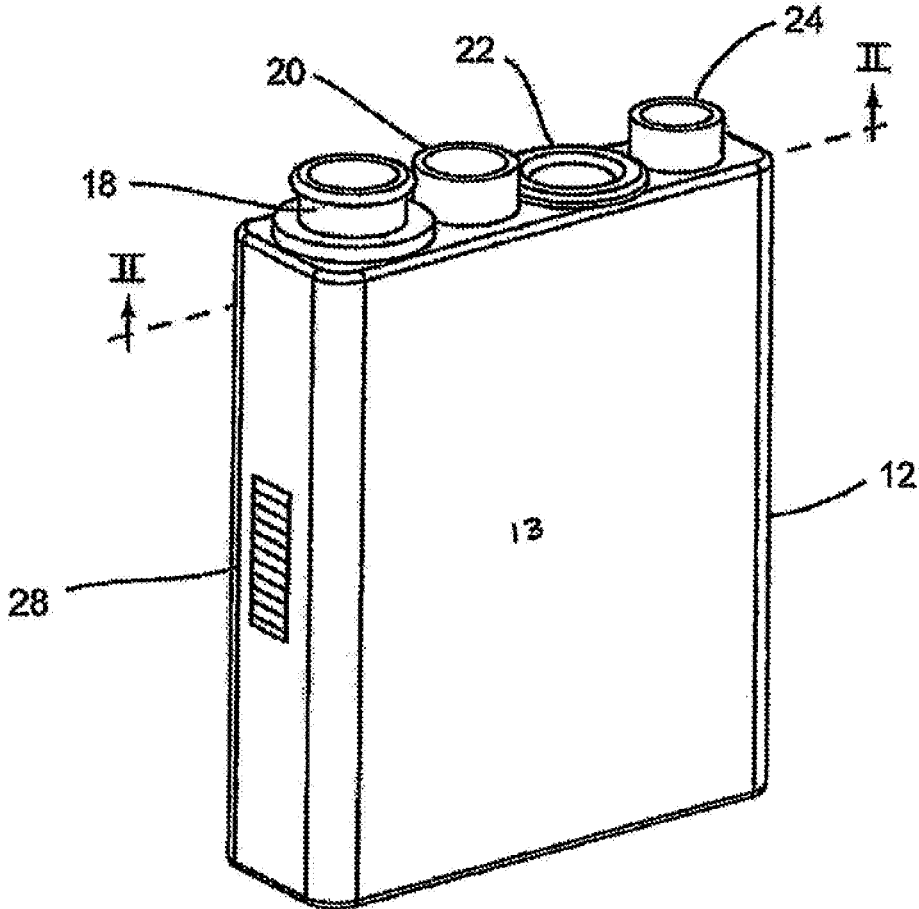


FIG. 1B

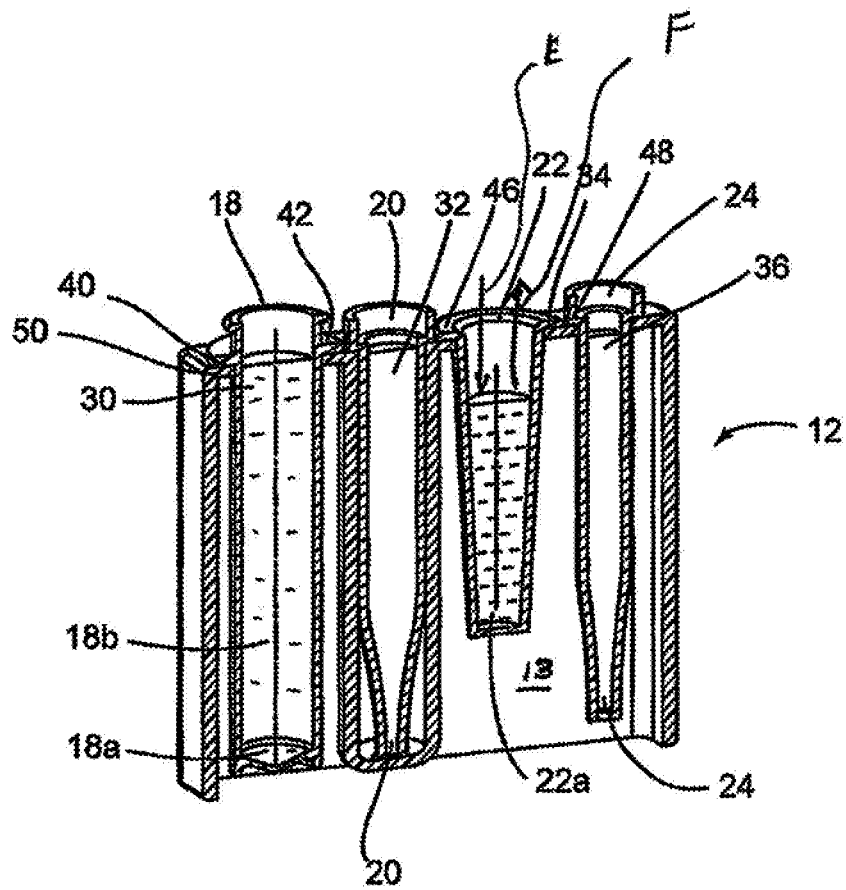


FIG. 2

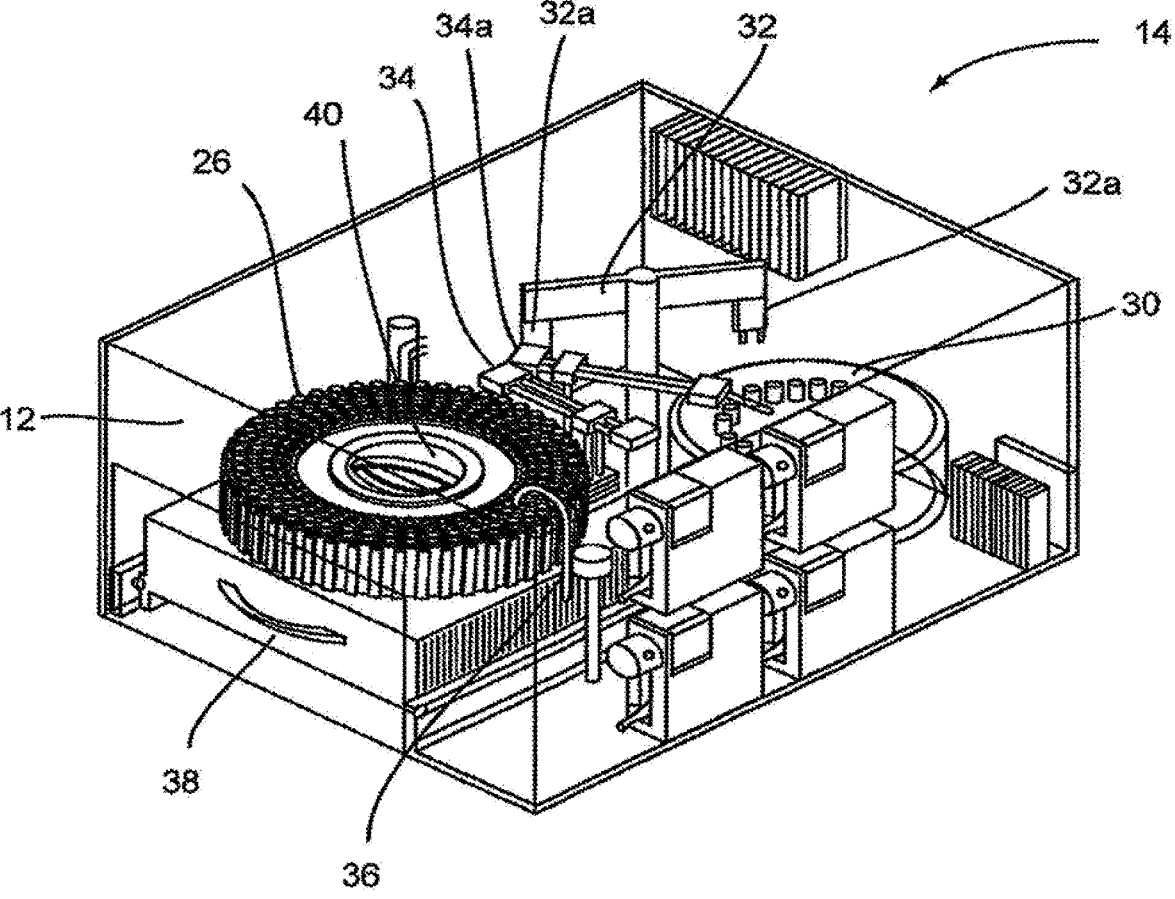


FIG. 3A

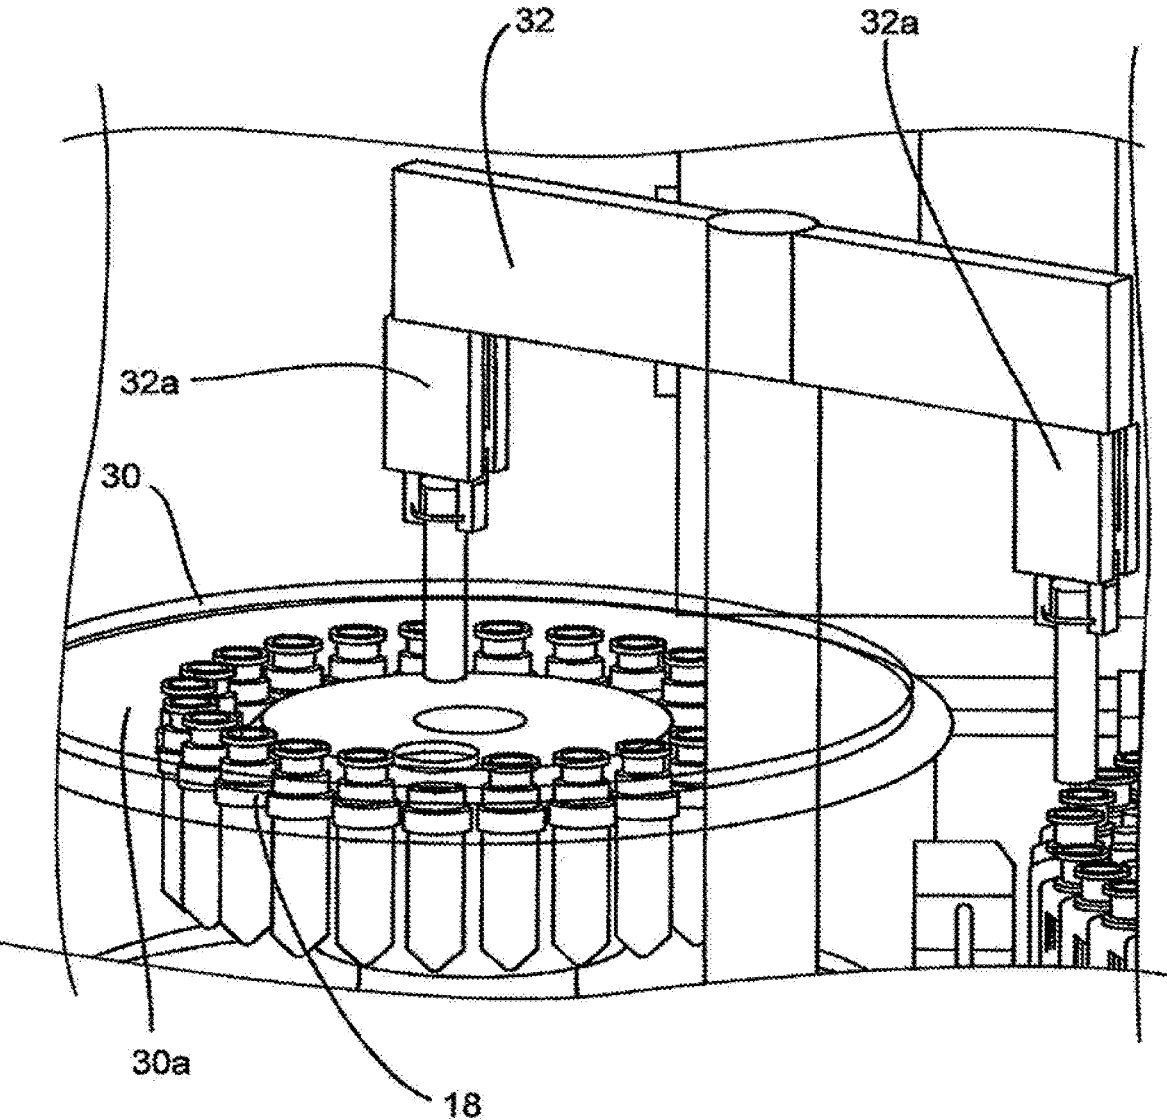


FIG. 3B

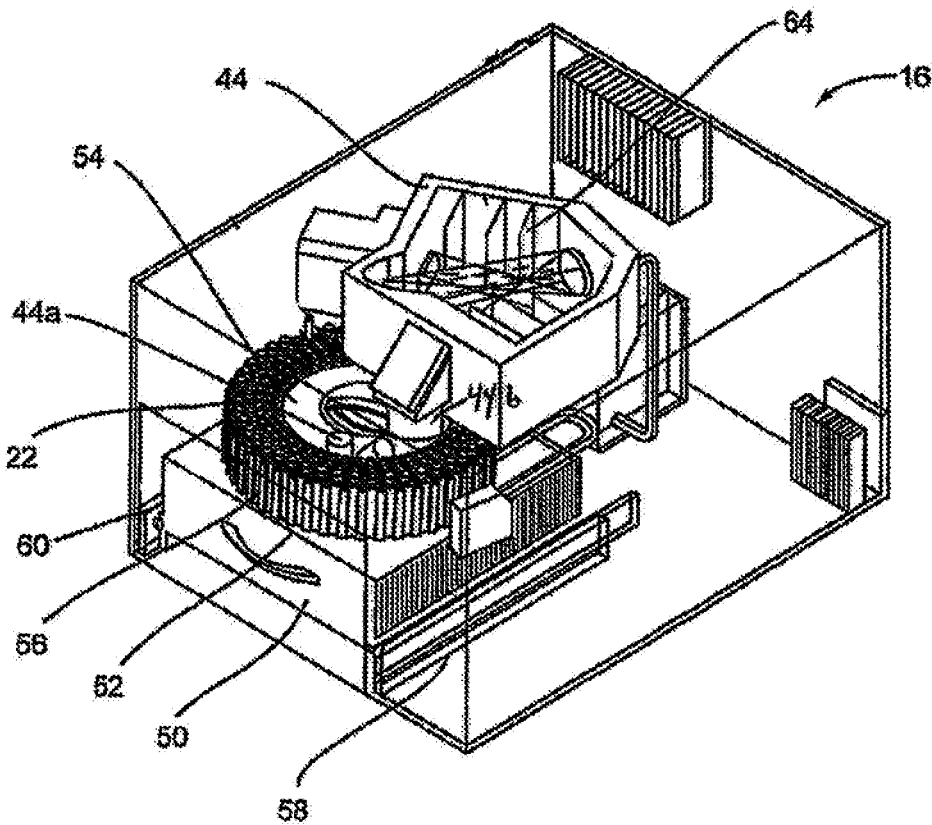


FIG. 4A

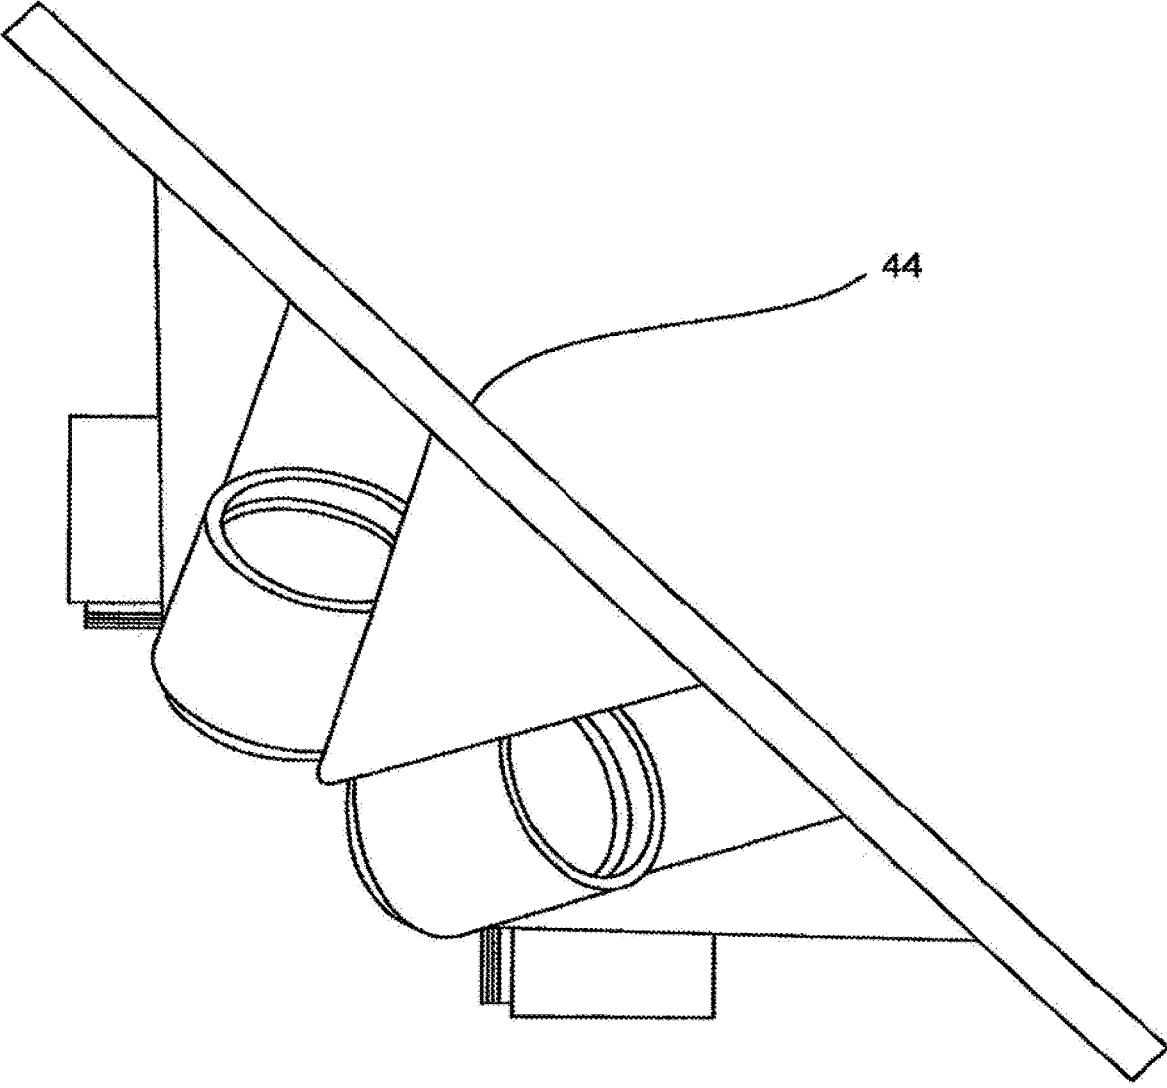


FIG. 4B



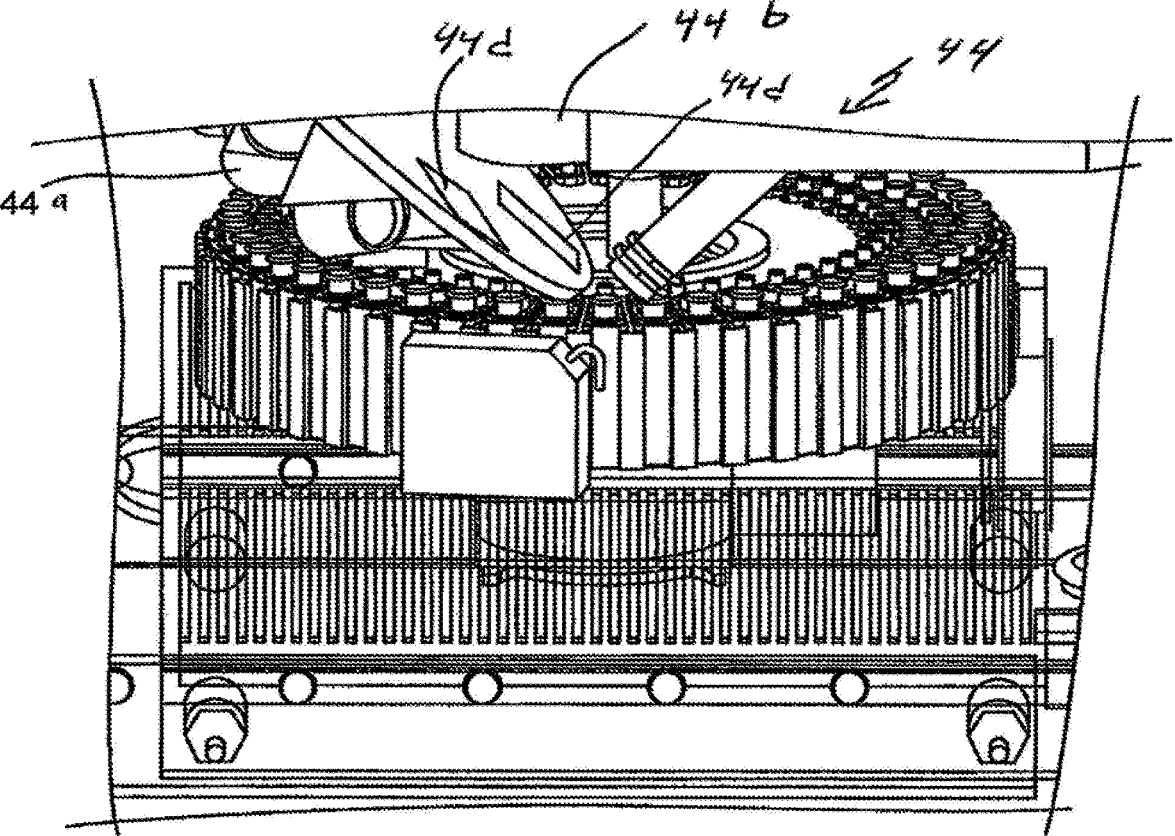


FIG. 4C

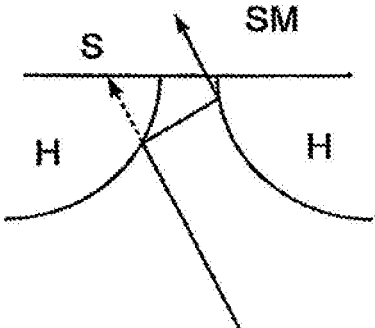


FIG. 5

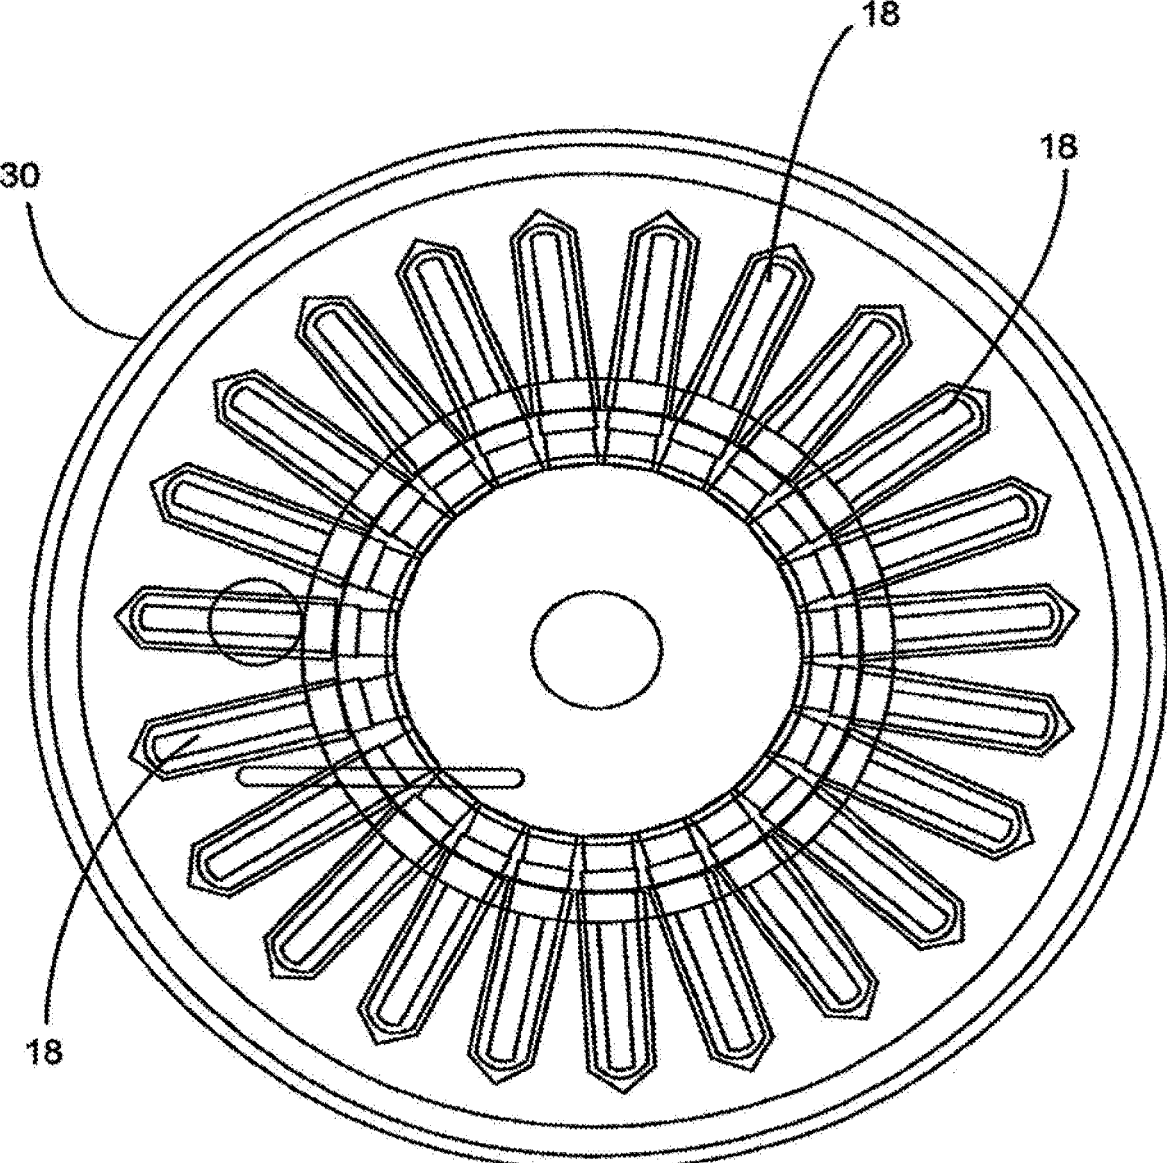


FIG. 6

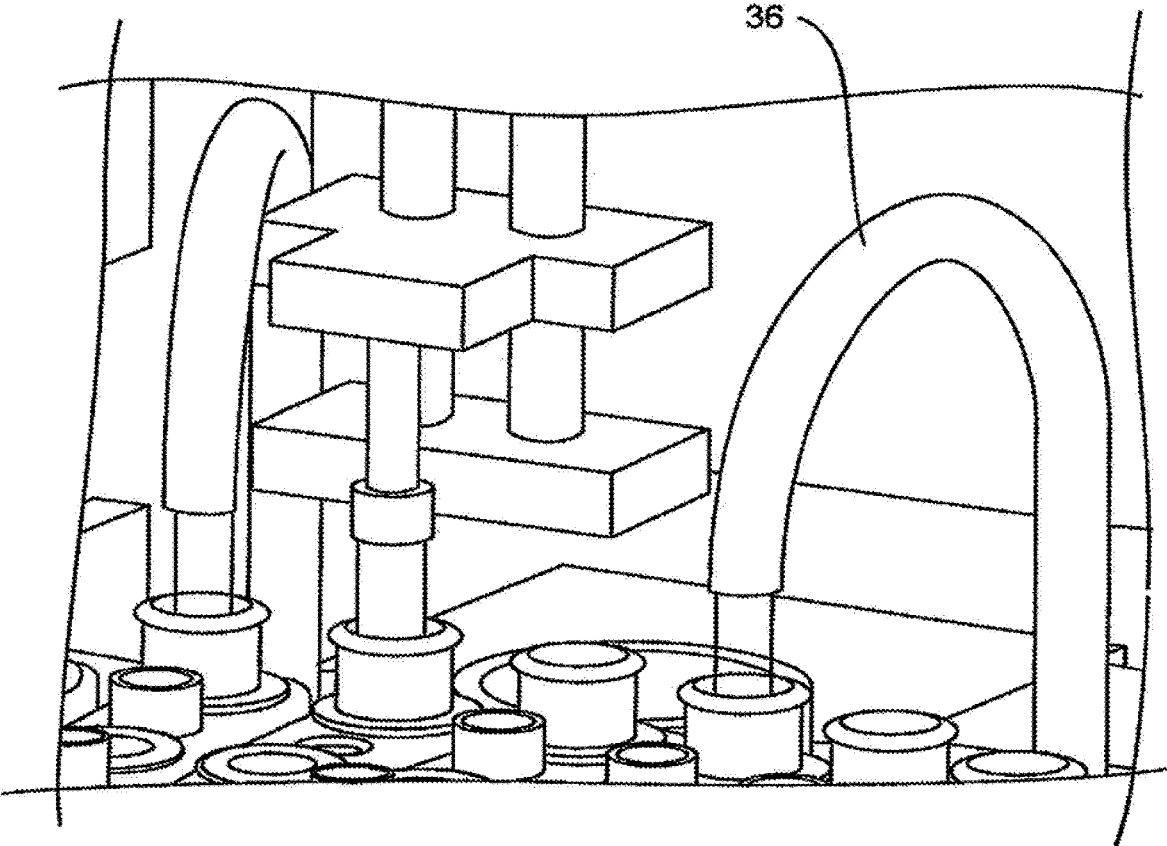


FIG. 7

## SYSTEM FOR CONDUCTING THE IDENTIFICATION OF BACTERIA IN URINE

### CROSS REFERENCE TO RELATED APPLICATIONS

[0001] The present application claims priority as a divisional application of U.S. patent application Ser. No. 14/330,450 entitled "System for Conducting the Identification of Bacteria in Urine" filed Jul. 14, 2014, which claims priority to U.S. patent application Ser. No. 12/682,402 entitled "System For Conducting The Identification Of Bacteria In Urine" filed Apr. 9, 2010, which is the United States national phase of International Patent Application No. PCT/US2008/079533 entitled "System For Conducting The Identification Of Bacteria In Urine" filed Oct. 10, 2008, which claims priority to U.S. Provisional Application Nos. 60/978,810, 60/978,820, 60/978,856 and 60/978,862, all filed on Oct. 10, 2007, which are herein incorporated by reference in their entirety.

### BACKGROUND OF THE INVENTION

#### Field of the Invention

[0002] The present invention relates to a system for conducting the identification and quantification of micro-organisms, e.g., bacteria in urine samples. More particularly, the invention relates to a system for identifying bacteria in urine samples which includes: 1) a disposable cartridge or holder for holding disposable components including a centrifuge tube, two pipette tips with a different volume capacity, and an optical cup or cuvette; 2) a sample processor for processing or preparing the urine samples; and 3) an optical analyzer for analyzing the processed urine samples. The disposable cartridge with its four components is used in the sample processor and the optical cup or cuvette in particular is used in the optical analyzer.

#### Description of Related Art

[0003] In general, current-day practice for identifying micro-organisms, e.g., bacteria in urine samples involves a complex, lengthy and expensive process for identifying and specifying micro-organisms in microbiology labs. In the current process, the samples are accepted into the lab. These specimens are then sorted and labeled and then they are inoculated onto blood agar medium using sterilized loop. The specimens are then inserted into a dedicated incubator for a 24-hour period. A day later, the lab technicians screen the specimens for positive and negative cultures. In general, most of the cultures are negative and they are manually reported. The organisms for the positive cultures are isolated and suspended in a biochemical fluid. This involves suspension, dilution, vortexing and turbidity measurements resulting in biochemical waste products. The cultures are then subjected to a species identification and antibiotics susceptibility testing exposing the suspensions to multiple reagents. After another 6 to 24-hour incubation period, the findings are interpreted and reported by lab technicians. This entire process generally takes 11 steps and 50 hours to obtain specimen results and the process is labor intensive.

[0004] Commonly owned U.S. Publication No. US 2007/0037135 A1, the contents of which are herein incorporated by reference, discloses a system for identifying and quantification of a biological sample suspended in a liquid.

Paragraph [0038] of this publication states that sample cuvettes are used. These cuvettes are said to be well known in the art and are typically square or rectangular in shape (having a well area to contain the sample) and are made of a transparent material such as glass or a polymeric material.

[0005] There is a need, therefore, particularly for species identification of the above lab procedure to provide a more efficient, and less time consuming process which requires less labor.

### SUMMARY OF THE INVENTION

[0006] The system of the invention streamlines this current system for obtaining specimen results. The system is environmentally friendly, enables a rapid diagnosis, results are consistent, no reagents are needed and there is a multi-functional diagnosis. Urine samples are contained within disposable cartridges which hold four disposable components, i.e., a centrifuge, two pipette tips with a different volume and an optical cuvette. The cartridges are bar coded and tied in with the patient's ID. The cartridges are inserted in a magazine which is then inserted into a sample processor which processes the specimens. The prepared specimens are transferred into the optical cuvettes and then the magazine is inserted into an optical analyzer which analyses the specimens. The optical analyzer analyses and generates the complete results enabling ultimate treatment of the bacteria. The system does not require a sophisticated operator and gives rapid results. The system increases efficiency, improves workload, saves time and money and is easy to operate. The sample preparation can be performed in parallel with the specimen analysis process and from 1 to 50 specimens can be analyzed simultaneously.

[0007] The system includes a plurality of disposable cartridges for holding a plurality of disposable components including a centrifuge tube, a first pipette tip with a 1 ml volume; an optical urine sample cuvette, and a second pipette tip with a 0.5 ml volume; a sample processor for receiving the plurality of disposable cartridges and configured to process and prepare the urine sample of each disposable cartridge and to transfer the urine samples into the respective optical cuvette of each of the disposable cartridges; and an optical analyzer for receiving the cartridge with the optical cuvettes containing the processed urine samples and analyzing and generating the specimen results. The entire process of processing the urine specimens in the sample processor and analyzing them in the optical analyzer takes about 20 minutes for a single specimen and up to 2 hours for 50 specimens.

[0008] The disposable cartridge and the disposable components increase efficiency, improve workload and save time and money since the components necessary for the preparation or processing of the urine samples are conveniently located in one place, i.e., in a cartridge. Additionally, less manpower or manual handling of the components is required for the processing/analyzing of the urine samples. There is also the added convenience in that the cartridge and its components are disposable. That is, these items do not need to be sterilized for the next urine specimen identification process and contamination of the work area and/or surrounding environment is minimized.

[0009] The sample processor of the invention streamlines the current practice for processing urine samples for analysis. The sample processor of the invention is automated, fully compact, self-contained and does not require any

reagents. Urine samples are injected into centrifuge tubes which are carried in removable cartridges. The specimens are bar coded and tied with the cartridges which are also bar coded. The cartridges are mounted in a magazine which is then inserted into the sample processor which processes the specimens in preparation for analysis. The sample processor does not require a sophisticated operator and rapidly processes the samples or specimens. The sample processor increases efficiency, improves workload, saves time and money and is easy to operate. The processing of several samples can be performed in about 20 minutes for a single specimen and up to 1 hour for about 50 specimens.

**[0010]** The optical analyzer contains an optics system, a thermal control and a drawer which has a rotatable table for receiving, supporting and rotating a magazine containing a plurality of disposable cartridges with optical cups or cuvettes which contain the urine samples to be analyzed. The optical analyzer also contains a bar code reader for inventorying the urine samples and a level sensor that verifies that each optical cup or cuvette contains the correct volume of processed urine sample. When the drawer with the magazine is inserted into the optical analyzer, the drive mechanism for the rotatable table supporting the magazine rotates and registers the magazine relative to the bar code reader and then rotates and registers the magazine relative to the optics system. The optics system includes an excitation module unit, an optical collection unit and a spectrometer. The temperature of each cup or cuvette is decreased to a temperature which will slow the metabolism of the bacteria in the urine samples while increasing the fluorescence signal. A thermal control cools a large thermal mass which is located on the rotatable table underneath the magazine containing the disposable cartridges with urine sample cups or cuvettes. An infrared temperature sensor detects and monitors the temperature of each urine sample.

**[0011]** A related method for identifying the type of micro-organism and quantifying it in a urine sample includes the steps of obtaining a urine sample; passing the urine sample through a ten micron filter; obtaining a 2 ml sample of the filtered urine and placing it into a centrifuge tube; obtaining a 1,000,000:1 dilution of the dissolved materials in the urine retaining bacteria in the urine sample by centrifuging the 2 ml sample at about a 12,000 g-force, decanting about 95% of the fluid in the centrifuge tube, replacing the decanted solution with a saline solution, and repeating these steps about five times; transferring the final solution into an optical cup or cuvette; and subjecting the optical cup or cuvette to an optical analysis having optics which include exciting the urine sample with at least five different wavelengths, collecting and detecting the fluorescent emissions; and directing the fluorescent emissions into a spectrometer.

**[0012]** These and other objects and advantages of the invention will be made apparent from the following description taken together with the drawings.

#### BRIEF DESCRIPTION OF THE DRAWINGS

**[0013]** FIG. 1A is a top perspective view of a magazine having a plurality of disposable cartridges.

**[0014]** FIG. 1B is a top perspective view of a disposable cartridge used in the magazine shown in FIG. 1A.

**[0015]** FIG. 2 is a front sectional view illustrating the components of the disposable cartridge of FIG. 1 in phantom.

**[0016]** FIG. 3A is a perspective view of a sample processor illustrating in phantom the several components of the sample processor of the system of the invention.

**[0017]** FIG. 3B is an additional perspective view of a sample processor illustrating in phantom the several components of the sample processor of the system of the invention.

**[0018]** FIG. 4A is a perspective view of an optical analyzer illustrating in phantom the several components of the optical analyzer of the system of the invention.

**[0019]** FIG. 4B is a perspective view of an optics system illustrating in phantom the several components of the optics of the system of the invention.

**[0020]** FIG. 4C is an additional perspective view of an optical analyzer illustrating in phantom the several components of the optical analyzer of the system of the invention.

**[0021]** FIG. 5 is a schematic illustrating mirrored convex "horn" that may be provided at the entrance of a slit of a spectrometer.

**[0022]** FIG. 6 is a perspective view of a centrifuge illustrating in phantom the several components of the centrifuge of the system of the invention.

**[0023]** FIG. 7 is an additional perspective view of a sample processor illustrating in phantom the several components of the sample processor of the system of the invention.

#### DETAILED DESCRIPTION OF THE INVENTION

**[0024]** The present invention will be described with reference to the accompanying drawings where like reference numbers correspond to like elements.

**[0025]** Referring to FIGS. 1-4, the system for conducting the identification of bacteria in urine samples includes a disposable cartridge 12 (FIGS. 1 and 2); a sample processor 14 (FIGS. 3A, 3B, 6 and 7); and an optical analyzer 16 (FIGS. 4A, 4B, and 4C). As shown in FIGS. 1 and 2, cartridge 12 contains four disposable components, which are a centrifuge tube 18, a first pipette tip 20 having a 1 ml volume, an optical cup or cuvette 22, and a second pipette tip 24 having a 0.5 ml volume. It is to be understood that the presently described inventive system is appropriate for the identification of bacteria in any fluid and is not limited to bacteria samples contained in urine.

**[0026]** The centrifuge tube 18 is a container that has an elongated body 18b with a tapered end indicated at 18a. In general, the centrifuge tube 18 initially contains the urine sample and the first pipette tip 20 may be used to dilute the urine-dissolved constituents, and the second pipette tip 24 may be used to transfer the diluted urine sample into the optical cup or cuvette 22 for optical analysis. The disposable cartridge 12 and its disposable components 18, 20, 22, and 24 may be made of a plastic material which is easily molded and inexpensive to manufacture.

**[0027]** Still referring to FIG. 2, the disposable components 18, 20, 22, and 24 are each contained within separate locations 30, 32, 34, and 36, respectively of the disposable cartridge 12. As is shown, the bottom of compartment 32 which receives and carries the first pipette tip 20 is closed so that any drip from the first pipette tip 20 will not contaminate the surface below the disposable cartridge 12. Each component 18, 20, 22, and 24 is suspended within its respective location 30, 32, 34, and 36 via a lip 40, 42, 46, and 48,

respectively attached to each component **18**, **20**, **22**, and **24** which is supported by the top surface **50** of disposable cartridge **12**.

[0028] Referring to FIGS. **2** and **4A**, an optical cup or cuvette **22** may be used in the optical analyzer **16** of FIG. **4A**. Preferably, the urine samples are prepared with a saline solution since saline solutions minimize background fluorescence while maintaining the integrity of the bacteria which particularly is important when using optics in the urine analysis process. The optical cup or cuvette **22** will include a reflective coating to assist in the optical analysis. The optical cup or cuvette **22** may be made of an ABS plastic material, glass or a metallic material, e.g., aluminum, and then coated with or layered with the reflective material. Alternatively, in the manufacturing of the optical cup or cuvette **22**, the layer of reflective material may be incorporated onto the plastic, glass or metallic material. As best shown in FIG. **2**, the optical cup or cuvette **22** includes a tapered end indicated at **22a** in order to assist with the optical analysis. It is anticipated that the UV light source in the optical analyzer **16** (FIGS. **4A**, **4B** and **4C**) be directed down the middle of the cup or cuvette **22** for the optical analysis of the urine specimen in the cup or cuvette **22**.

[0029] Several disposable cartridges **12** each containing the four disposable components **18**, **20**, **22**, and **24** are then inserted into a magazine **26** shown at the top of FIG. **1**, which is then loaded into the sample processor **14** as shown in FIG. **3**. Magazine **26** contains several disposable cartridges **12** some of which are numbered, each cartridge **12** has a unique bar code as indicated at **28** in FIG. **1** that is paired with the specimen of a patient. Alternatively, the magazine **26** can then be inserted into a device for the optical analysis of the urine samples. Preferably, the same magazine **26** used in obtaining processed urine samples in a sample processor is used in the device for the optical analysis of the processed urine samples.

[0030] The sample processor **14** of FIGS. **3A** and **3B** contains a centrifuge **30**, a rotatable gripper mechanism **32** which picks up the centrifuge tube **18** (FIG. **1**) of each disposable cartridge **12** and inserts the centrifuge tube **18** into the centrifuge **30**; two movable fluid transfer arms **34**, **34a** which are used to dilute the dissolved material in the urine samples via the pipette tip **20** (FIGS. **1** and **2**) and to transfer the diluted sample to the optical cup or cuvette **22** (FIG. **2**) via the pipette tip **24**; and a syringe pump dispenser fluid system **36** for delivering water to the samples for dilution purposes. The sample processor **14** also includes a drawer **38** which has a rotatable table **40** which receives, supports, and rotates the magazine **26** when the drawer **38** is inserted into the sample processor **14**. The drawer **38** contains a magazine drive mechanism (not shown) which rotates the magazine **26**.

[0031] In general, centrifuge tube **18** contains about 2 ml sample of filtered urine which is placed into the centrifuge tube by the user. This sample may then be sufficiently diluted with a saline solution or water by centrifuging the sample followed by using the first pipette tip **20** with the 1.0 ml volume to decant the supernates in two decant cycles followed by refilling of the centrifuge tube **18** with a saline or water. The second pipette tip **24** having the 0.5 ml volume may then be used to draw out about 500  $\mu$ l of fluid from centrifuge tube **18** and then to dispense this 500  $\mu$ l of fluid into the respective optical cup or cuvette **22** of the designated patient. This second pipette tip **24** can then be inserted

into the first pipette tip **20** and both pipette tips **20**, **24** can be disposed of properly. It is believed that one pipette tip may be used to dilute and draw out instead of two pipette tips. This process may be done manually or may be done automatically.

[0032] The loading and unloading of the magazine **26** is accomplished with the several disposable cartridges **12** mounted on the rotatable table **40** (FIG. **1** and FIG. **2**). The manual drawer contains a magazine drive mechanism (not shown). Once the magazine **26** is inserted into the sample processor **14**, the drive mechanism (not shown) for rotatable table **40** rotates the magazine **26**; the bar code reader (element **58** in FIG. **4A**) inventories the samples, a level sensor (not shown) verifies that samples were dosed properly; and a second sensor (not shown) verifies that all of the necessary disposable components **18**, **20**, **22**, and **24** (FIG. **2**) are contained in each disposable cartridge **12**.

[0033] The transfer of the centrifuge tube **18** (FIG. **2**) into the centrifuge **30** (FIGS. **3A** and **3B**) will now be described. A centrifuge lid **30a** of the centrifuge **30** is oriented to allow the rotatable gripper mechanism unit **32** to access and load the centrifuge **30**. The drive mechanism of the rotatable table **40** is configured to align the centrifuge tube **18** of each disposable cartridge **12** into position relative to the rotatable unit **32**. The gripper **32a** of rotatable gripper mechanism **32** selects the centrifuge tube **18** for transfer from the magazine **26** and into the centrifuge **30**. The centrifuge rotor (not shown) is configured to align a vacant centrifuge holder of centrifuge **30** in the load position. The gripper **32a** referred to as a "Theta Z gripper" is a radial member that rotates and has a downward and upward movement for picking up and setting a centrifuge tube **18** into a vacant centrifuge holder of centrifuge **30**. The lid of centrifuge **30** is closed after all of the centrifuge tubes **18** are placed into the centrifuge **30**.

[0034] Centrifuge **30** (FIG. **6**) is automatically operated to spin the centrifuge tubes **18** at about a 12,000 g-force for about 2 minutes. The centrifuge **30** includes tube holders that are configured to rotate each of the centrifuge tubes **18** about ninety degrees upon rotation of the centrifuge **30**. The centrifuge allows for precise positioning and position tracking so that correct tubes are returned to cartridges in the magazine after centrifugation. This action results in the solid formation of the bacteria present in the urine sample at the bottom of the centrifuge tube **18**.

[0035] There are two fluid transfer arms **34**, **34a** (FIGS. **3A** and **3B**) for removing the supernates from two samples of two disposable cartridges **12** at a time. After the two fluid transfer arms **34**, **34a** (FIGS. **3A** and **3B**) obtain the pipette tip **20** (FIG. **2**) with a 1 ml volume, each of the fluid transfer arms **34** and **34a** (FIGS. **3A** and **3B**) makes two consecutive trips to the centrifuge tube **18**, each time drawing fluid from the tube **18** and dispensing this fluid into a waste port (not shown) of sample processor **14** before returning the pipette tip **20** to its location on the disposable cartridge that is being sampled and before continuing with the next sample in the disposable cartridge **12** that is rotated to be registered in the sampling location of sample processor **14**.

[0036] The syringe pump dispenser fluid system **36**, is illustrated in FIG. **7**, for delivering water or saline to the samples for dilution purposes. The waste fluid which had been decanted from a centrifuge tube **18** as described in the preceding paragraph is replaced with clean process fluid via system **36**. Two syringe pumps dispense this clean process fluid into the centrifuge tube **18** from which the waste fluid

had been removed in the previous step. During the final refill step, a smaller amount of clean fluid is used in order to get the bacteria level in the cartridge tube 18 to the required concentration.

[0037] After the sample in centrifuge tube 18 has been sufficiently diluted with the clean fluid, one of the two fluid transfer arms 34, 34a (FIGS. 3A and 3B) transfers the processed sample in centrifuge tube 18 to the optical cup or cuvette 22 of its respective disposable cartridge 12. One of the fluid transfer arms 34, 34a grasps the pipette tip 24 having the 0.5 ml volume, which until now has not been used in this process. This pipette tip 24 with the smaller volume is used to draw out about 500  $\mu$ l of fluid from centrifuge tube 18 and is used to dispense this fluid into the respective optical cup or cuvette 22 of the designated patient. This pipette tip 24 with the smaller volume is then inserted into the pipette tip 20 with the larger volume via the fluid transfer arm 34 or 34a for disposal of both pipette tips 20, 24.

[0038] The metering/decanting, metering/refilling, and metering/fluid transferring process described herein above is to obtain preferably, approximately a 1,000,000:1 dilution of the dissolved materials retaining bacteria in the urine sample in centrifuge tube 18. This can be achieved by 1) centrifuging, through means known to those skilled in the art, the urine sample at a 12,000 g-force; 2) decanting about 95% of the fluid by using the first pipette tip 20; 3) replacing the decanted solution of 2) with a saline solution; and 4) repeating steps 1), 2), and 3) at least five times by using the first pipette 20. The final processed urine sample in centrifuge tube 18 can then be decanted via the second pipette 24 into the optical cup or cuvette 22.

[0039] The final processed urine sample in optical cup or cuvette 22 can then be used in an optical analysis for determining the micro-organism's identity and/or quantity in the urine sample in optical cup or cuvette 22. This information can be obtained by using the system as disclosed in the aforesaid U.S. Publication No. 2007/0037135 A1.

[0040] Each of the steps described above for one centrifuge tube 18 is done in the sample processor 14 for each of the disposable cartridges 12 in magazine 26. It is to be appreciated that the waste fluid of each disposable cartridge 12 is disposed into a receptacle (not shown) in sample processor 14 or is plumbed directly into a drain. The waste disposables, i.e., the disposable cartridge 12 and disposable components 18, 20, 22, and 24 remain on the magazine 26 for manual removal when the magazine 26 is unloaded in preparation for the next operation of the sample processor 14 for processing the next batch of urine samples.

[0041] The following steps are involved in processing the urine samples in preparation for analysis via the optical analyzer 16 of FIGS. 4A, 4B, and 4C. In general, a sample of urine is obtained in a test tube. This sample is passed through a ten micron filter from which a 2 ml sample is obtained and placed into the centrifuge tube 18. The desired diluted sample, i.e., 1,000,000:1 dilution of dissolved materials while retaining bacteria in the urine sample is obtained by centrifuging this 2 ml sample at about a 12,000 g-force; and decanting 95% of the fluid. This latter step is repeated five times wherein the decanted solution is replaced each time with a saline solution. A saline solution is selected for this process in that it minimizes background fluorescence

which comes into play when the processed urine sample is inserted into the optical analyzer 16 while maintaining the bacteria integrity.

[0042] The optical analyzer 16 of FIGS. 4A, 4B, and 4C will now be described. With reference to FIG. 4A, the optical analyzer 16 includes an optics system 44 (shown in greater detail in FIGS. 4B and 4C), a thermal control unit (not shown), a drawer 50 which has a rotatable table 52 which receives, supports, and rotates a magazine 54 containing a plurality of holders 56 for receiving the disposable cartridges 12 in which cups or cuvettes 22 contain the processed urine samples which are to be analyzed, and a bar code reader 58 (FIG. 4A).

[0043] As can be appreciated, a cartridge 12 that has the cups or cuvettes 22 containing the processed urine sample for optical analysis are placed into the holders 56 of the magazine 54. FIG. 4A illustrates the magazine 54 mounted on the rotatable table 52 being loaded into the optical analyzer 16. Drawer 50 is pulled out manually for the loading and unloading of magazine 54. Drawer 50 contains the thermal control unit (not shown) and a drive mechanism (not shown). Alignment features on the magazine 54 and drawer 50 allow the operator to orient the magazine 54 properly on the drive mechanism and the thermal control unit when the magazine 54 is loaded onto the rotatable table 52. Once the drawer 50 and magazine 54 are manually inserted into the optical analyzer 16, the drive mechanism rotates the magazine 54 at which time a bar code reader station 58 (FIG. 4A) inventories the samples. A level sensor (not shown) verifies that each optical cup or cuvette 22 contains the correct sample volume. An operator can access the optical analyzer 16 when a user interface indicates that all the samples in the cups or cuvettes 22 have been analyzed and drawer 50 is prevented from being opened when any of the components of optical analyzer 16 are moving or when the UV light sources of the optics system 44 are on.

[0044] FIG. 4A illustrates the magazine 54 on rotatable table 52 while being positioned within optical analyzer 16. The optical analyzer 16 further includes a mechanical locking system (not shown) which positions the drawer 50 accurately with respect to the optics system 44. The drive mechanism is configured to automatically rotate the magazine 54 to position each cartridge 12 into the bar code reader station 58 and into precise alignment with the optics system 44. A second mechanical locking system (not shown) is used to secure each cup or cuvette 22 in its proper positioning relative to the optics system 44 for optical analysis.

[0045] FIG. 4A illustrates the thermal control for the optical cups or cuvettes 22. Preferably, the temperature of each cup or cuvette 22 is decreased to a temperature which will slow the metabolism of the bacteria while increasing the fluorescence signal. The thermal control unit 46 which is a thermal electric cooler (TEC) cools a large thermal mass 60 which is located on the rotatable table 52 underneath the magazine 54. The thermal mass 60 (FIG. 4A) is in direct contact with the optical cups or cuvettes 22, and an infrared temperature sensor (not shown) detects and monitors the temperature of each sample prior to the sample being rotated and positioned within the optics system 44.

[0046] The optics system 44 of the optical analyzer 16 will now be described. The optics system is shown in greater detail in FIG. 4B. The optics system 44 contains three separate units, that is, an excitation unit 44(a), an optical collection unit 44(b) and a spectrometer. Excitation will be



provided by a ultra-violet (UV) light source, which preferably will be LED (light emitting diode). A series of five LED modules provide an excitation unit 44(a) will sequentially provide excitation signals to each sample cup or cuvette 22 at five different excitation wavelengths which will be applied to each sample cup or cuvette 22 in the same order. The excitation time will be approximately 14 seconds per wavelength. The excitation emissions are directed via lenses and filters 44(d) to be directed an upper surface of the sample in the cuvette 22 as shown in FIG. 2. In order to narrow or control the shape of each excitation wavelength, narrow bandwidth filters will be used. These filters will direct in a downwardly direction the excitation wavelengths E to the sample cups or cuvettes 22 and the fluorescent emissions F will be reflected back in an upwardly direction to the optical collection unit from the same position of the cassette. The fluorescent emissions can be separated and directed via a filter arrangement. FIG. 4C illustrates the positioning of the optics system 44. As described previously, mechanical locking features position the drive mechanism such that the sample cup or cuvette 22 is aligned precisely. This precise alignment allows for the reflection of the fluorescent emission to the optics system 44 allowing for measurement of fluorescence. Optical elements (not shown) are utilized to gather and direct the fluorescent emissions into the spectrophotometer for measurement.

[0047] In addition, the optical collection unit includes optical elements to gather and direct the fluorescent emissions of the samples in the cups or cuvettes 22 into the spectrometer.

[0048] The optics system 44 may include a Czerny-Turner spectrometer with a CCD (charged couple device) Photon Detector, whereby fluorescent photons are reflected by several mirrors before contacting the CCD device. The emitted fluorescence will be monitored on the CCD device by integrating for a period of time. It is also envisioned that the Czerny-Turner spectrometer be modified with additional cylindrical lenses adjacent the entrance slit and the CCD device in order to improve photon usage efficiency. Additionally, as schematically illustrated in FIG. 5, mirrored convex "horn" H may be provided at the entrance of the slit S of the spectrometer SM to direct additional photons through the slit S.

[0049] Referring to FIG. 4A, the optics system 44 will include a light-tight enclosure or housing 64 in order to minimize light entering the optics system 44, and the camera of the CCD device will include a thermal electric cooler (TEC) (not shown) for transferring heat from the camera chip to the enclosure or housing 64 of the optics system 44.

[0050] Both the sample processor 14 and the optical analyzer 16 will have a HEPA air-filtering system for ventilation purposes in filtering the air entering and exiting the sample processor 14 and the optical analyzer 16. The sample processor 14 and the optical analyzer 16 will also have a slight positive pressure during operation. However, this pressure will decrease to atmospheric pressure when the user is allowed to open the door. Power to both the sample processor 14 and the optical analyzer 16 will be supplied from a separate rack mounted power supply module.

[0051] It is further envisioned that the LED intensity will be monitored to correlate the emitted fluorescence with the intensity of the excitation fluorescence. In particular, the information obtained by the optical analyzer 16 may be used to generate graphs similar to FIGS. 5 through 9 of U.S.

Publication No. 2007/0037135 A1, described in greater detail below. The graphs represent for the concentration of the bacteria in the sample cups or cuvettes 22, the fluorescence intensity, the emission wavelengths and the excitation wavelengths.

[0052] As discussed hereinabove, the optical analyzer 16 provides results that are then used to identify the type of bacteria in the urine samples. This can be done by coupling the optical analyzer 16 to a computer module (not shown) and feeding in the acquired information of the optical analyzer 16, such as the fluorescence emission, into the computer module. The computer module may perform multivariate analysis on the fluorescence excitation-emission matrices of the urine samples to identify and quantify the urine samples in a manner similar to that disclosed in the above U.S. Publication No. US 2007/0037135 A1. Here, the system includes a fluorescence excitation module which includes an excitation light source, a sample interface module for positioning the sample to receive the light source, a fluorescence emission module and a detection device. The computer module described above is coupled to the fluorescence module. The multivariate analysis may comprise extended partial least squared analysis for identification and quantification of the urine samples.

[0053] It is still further envisioned that a "homogenitor tube" will be used to mix the different LED packages output into a uniform UV light source. A typical "homogenitor tube" for use in the invention will be similar to that known to those skilled in the art.

[0054] The present invention has been described with reference to the preferred embodiments. Obvious modifications and alterations will occur to others upon reading and understanding the preceding detailed description. It is intended that the invention be construed as including all such modifications and alterations.

1-16. (canceled)

17. A method for processing a fluid sample in preparation for the identification and quantification of micro-organisms in the fluid sample, the steps comprising:

- a) obtaining a fluid sample;
- b) passing the fluid sample through a filter;
- c) obtaining a sample of the filtered fluid sample and placing it into a centrifuge tube;
- d) obtaining a dilution of the dissolved material in the fluid sample while retaining bacteria in the fluid sample by performing the following steps:
  - 1) centrifuging the sample of step c);
  - 2) decanting a portion of the fluid in the centrifuge tube of step 1);
  - 3) replacing the decanted solution of step 2) with a saline solution; and
- e) transferring the final solution of step 4) into an optical cup or cuvette for analysis.

18. The method of claim 17, wherein the fluid sample is urine.

19. The method of claim 17, wherein step d) results in about a 1,000,000:1 dilution.

20. The method of claim 17, wherein the sample of step (d)(1) is centrifuged at about 12,000 g-forces.

21. The method of claim 17, wherein about 95% of the fluid from step (d)(2) is decanted.

**22.** The method of claim **17**, wherein after step d(3), further comprising a step of repeating steps (1), (2) and (3) and then transferring the final solution into an optical cup or cuvette for analysis.

**23.** The method of claim **17**, wherein after step (d)(3), further comprising a step of repeating steps (1), (2) and (3) for a plurality of times and then transferring the final solution into an optical cup or cuvette for analysis.

**24.** The method of claim **23**, wherein the plurality of times is at least five times.

**25-37.** (canceled)

**38.** A method for identifying the type and quantity of micro-organisms in a fluid sample, the steps comprising:

- a) obtaining a fluid sample;
- b) passing the fluid sample through a filter;
- c) obtaining a sample of the filtered fluid and placing it into a centrifuge tube;
- d) obtaining a dilution of the dissolved material in the urine sample while retaining bacteria in the urine sample by performing the following steps:
  - 1) centrifuging the sample of step c);
  - 2) decanting a portion of the fluid in the centrifuge tube of step 1);
  - 3) replacing the decanted solution of step 2) with a saline solution; and
- e) transferring the final solution of step 4) into an optical cups or cuvette; and
- f) subjecting the optical cup or cuvette to an optical analysis having optics which include exciting the fluid sample with a plurality of different wavelengths, collecting and detecting the fluorescent emissions; and directing the fluorescent emissions into a spectrometer.

**39.** The method of claim **38**, wherein step d) results in about a 1,000,000:1 dilution.

**40.** The method of claim **38**, wherein the sample of step (d)(1) is centrifuged at about 12,000 g-forces.

**41.** The method of claim **38**, wherein about 95% of the fluid from step (d)(2) is decanted.

**42.** The method of claim **38**, wherein after step d(3), further comprising a step of repeating steps (1), (2) and (3) and then transferring the final solution into an optical cup or cuvette for analysis.

**43.** The method of claim **38** wherein after step (d)(3), further comprising a step of repeating steps (1), (2) and (3)

for a plurality of times and then transferring the final solution into an optical cup or cuvette for analysis.

**44.** The method of claim **43** wherein the plurality of times is at least five times.

**45.** A method for identifying the type and quantity of micro-organisms in a fluid sample, the steps comprising:

- a) obtaining a fluid sample;
- b) passing the fluid sample through a filter;
- c) obtaining a sample of the filtered fluid and placing it into a removable tube; and
- d) transferring the sample of the filtered fluid into an optical cup or cuvette, said optical cup or cuvette comprising a container having an open portion and a sidewall that is continuously tapered along their length to a truncated conical end and a reflective surface; and
- e) subjecting the optical cup or cuvette to an optical analysis having optics which include exciting the fluid sample with a plurality of different wavelengths, collecting and detecting the fluorescent emissions, and directing the fluorescent emissions into a spectrometer, wherein during the optical analysis, a light is directed down a middle portion of the container through the open portion of the container and into the fluid sample, wherein the sidewall is continuously tapered along its length to a truncated conical end configured to assist with the optical analysis and the reflective surface of the container reflects fluorescent emissions back in an upwardly direction out of the fluid sample and through the open portion of the container to an optics system for the optical analysis.

**46.** The method of claim **45**, wherein the container includes a lip for suspending the container from a top surface of a cartridge.

**47.** The method of claim **46**, wherein the cartridge includes a body and the container is located within an opening in the cartridge body.

**48.** The method of **45**, wherein the container has a flat bottom surface.

**49.** The method of claim **45**, wherein the reflective surface is a coated onto the container or is a separately formed layer of material.

**50.** The optical cup or cuvette of claim **45**, wherein the reflective surface is an inner reflective surface of the container or is incorporated onto the container material.

\* \* \* \* \*