



(19) **United States**

(12) **Patent Application Publication**
Melanson et al.

(10) **Pub. No.: US 2020/0253615 A1**

(43) **Pub. Date: Aug. 13, 2020**

(54) **DEVICES AND METHODS FOR EXCLUDING THE LEFT ATRIAL APPENDAGE**

Publication Classification

(71) Applicant: **Conformal Medical, Inc.**, Merrimack, NH (US)

(51) **Int. Cl.**
A61B 17/12 (2006.01)

(72) Inventors: **David A. Melanson**, Hudson, NH (US); **Andy H. Levine**, Newton Highlands, MA (US); **James H. Loper**, Wales, MA (US); **Michael T. Radford**, Nashua, NH (US); **Carol Devellian**, Topsfield, MA (US); **Aaron V. Kaplan**, Norwich, VT (US); **Ronald B. Lampport**, Pelham, NH (US)

(52) **U.S. Cl.**
CPC *A61B 17/12122* (2013.01); *A61B 2017/00579* (2013.01)

(21) Appl. No.: **16/794,023**

(57) **ABSTRACT**


(22) Filed: **Feb. 18, 2020**

Systems, devices and methods for occluding the left atrial appendage (LAA). The device excludes the LAA from blood flow. The implantable device is delivered via transcatheter delivery into the LAA and secured within the LAA. The implant comprises an expandable and compliant frame and an expandable and conformable tubular foam body. A delivery and tether retraction system includes a handle for controlling a pusher and tether. The pusher may be moved a distance away from the implant without changing the orientation of the implant, while the tether is still attached to the implant. Severing the tether and proximally retracting a control on the hand piece by a distance causes the severed end to advance distally by at least about twice that distance. A loader includes a conical portion with guides and a reservoir for submerging the foam prior to loading and delivery.

Related U.S. Application Data

(63) Continuation of application No. 16/782,871, filed on Feb. 5, 2020.

(60) Provisional application No. 62/803,289, filed on Feb. 8, 2019.

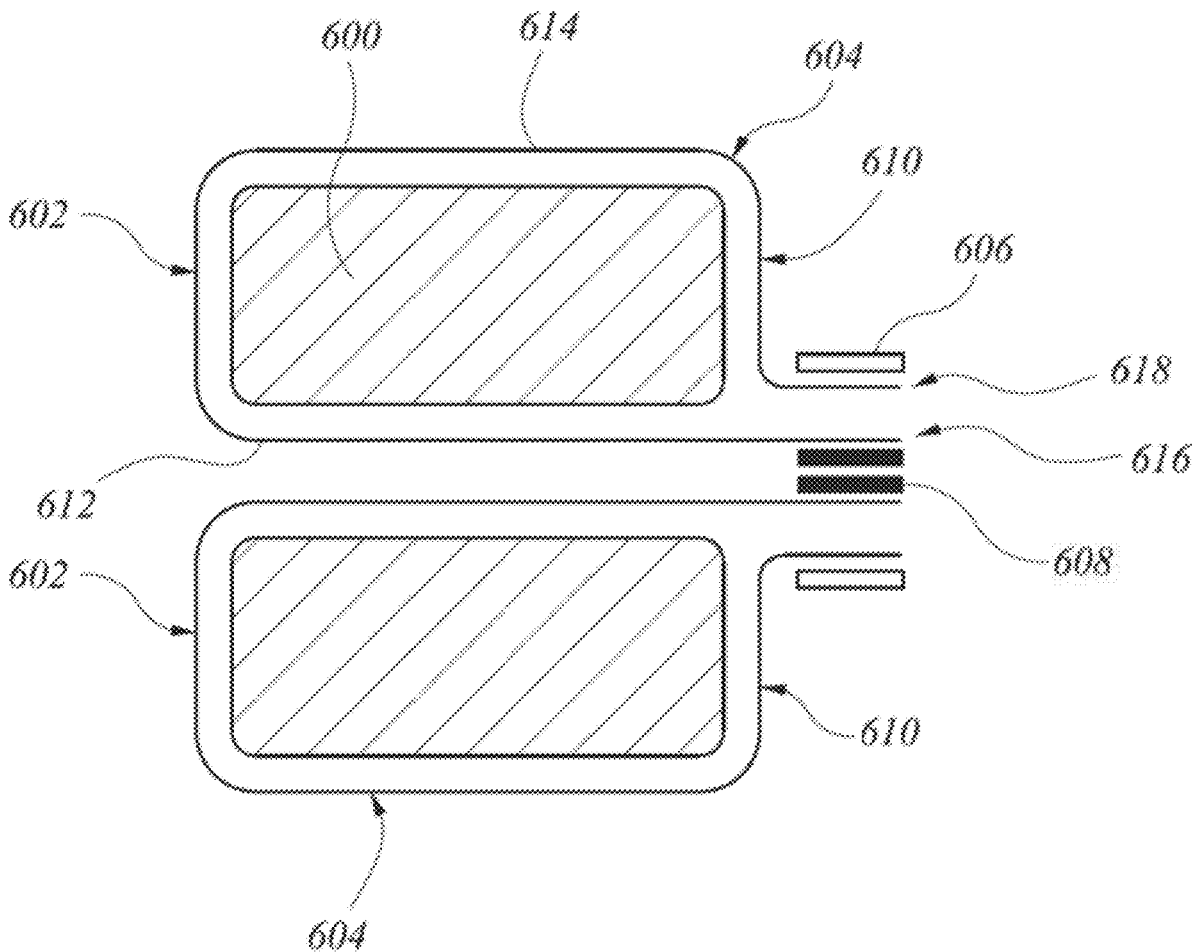

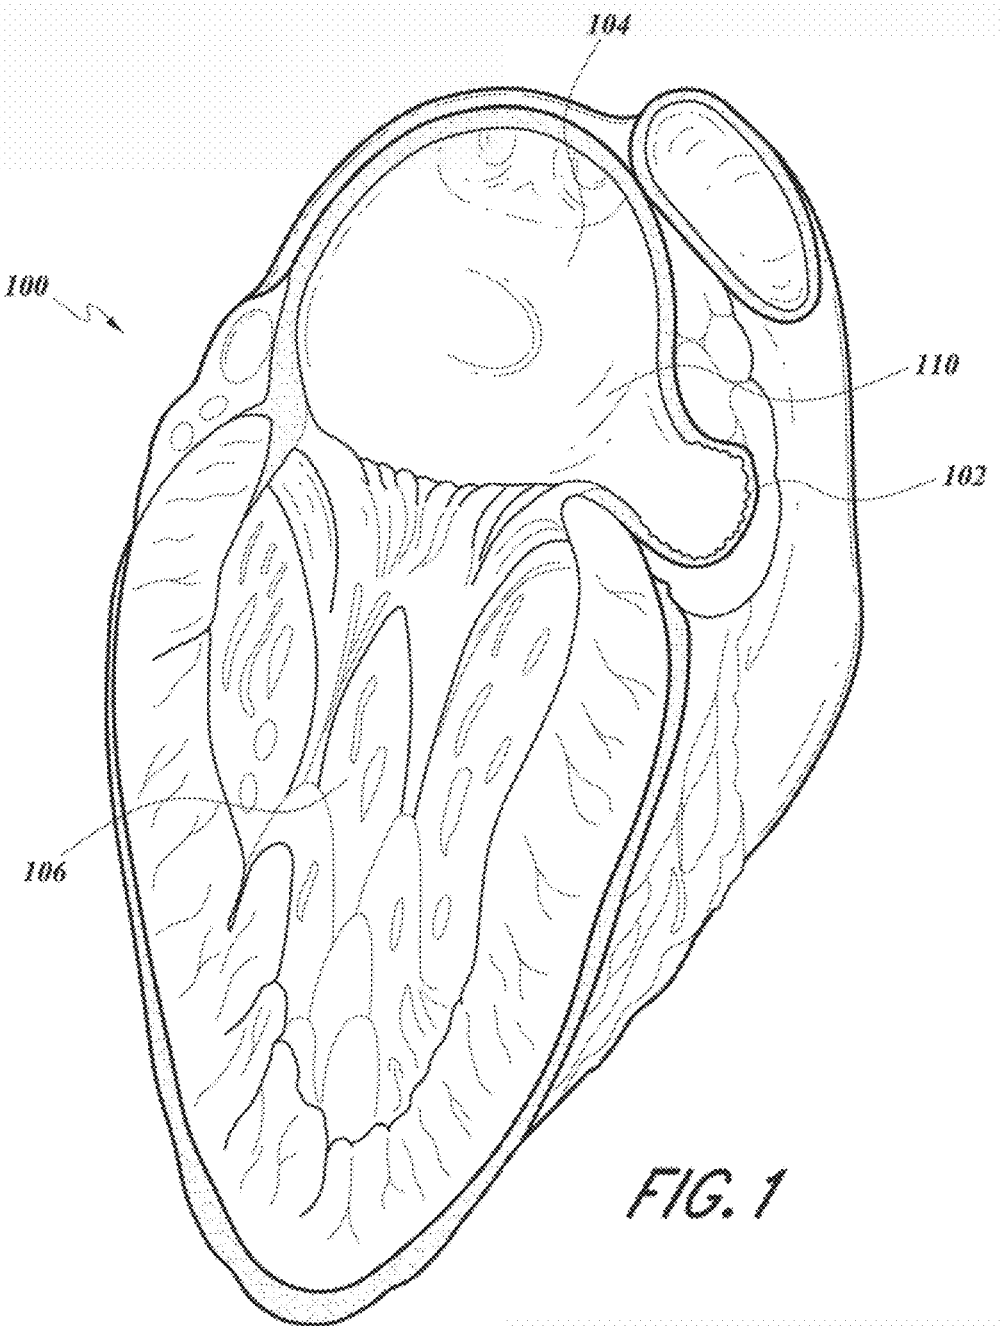


FIG. 1

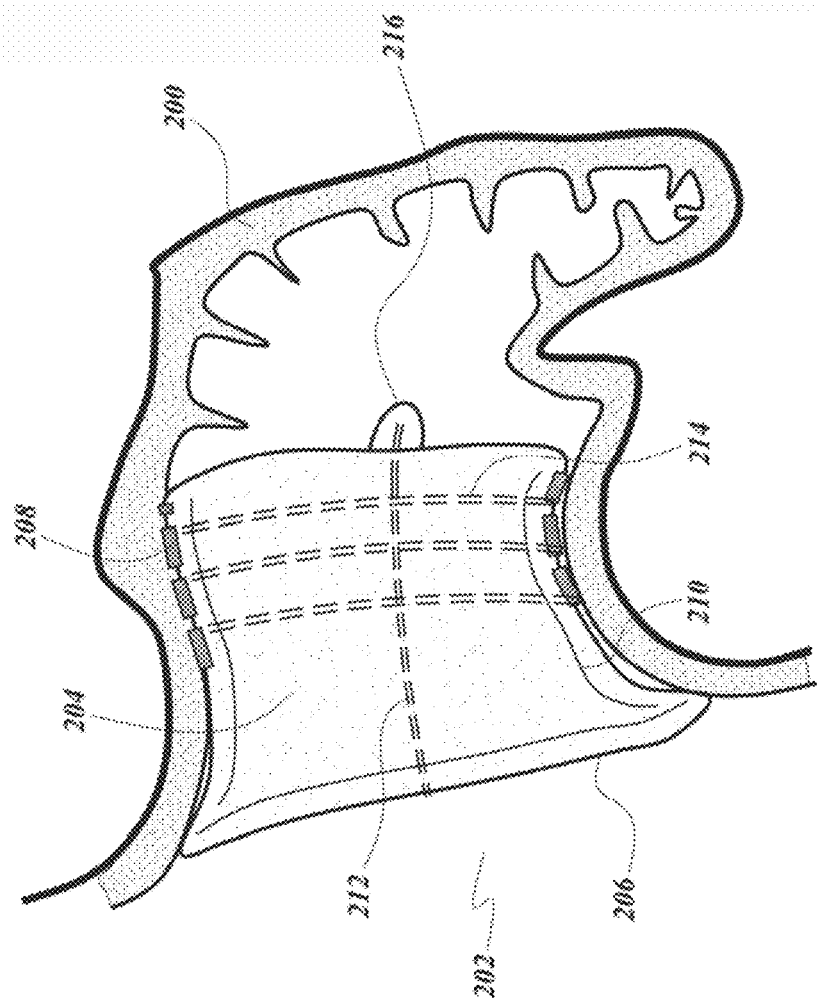
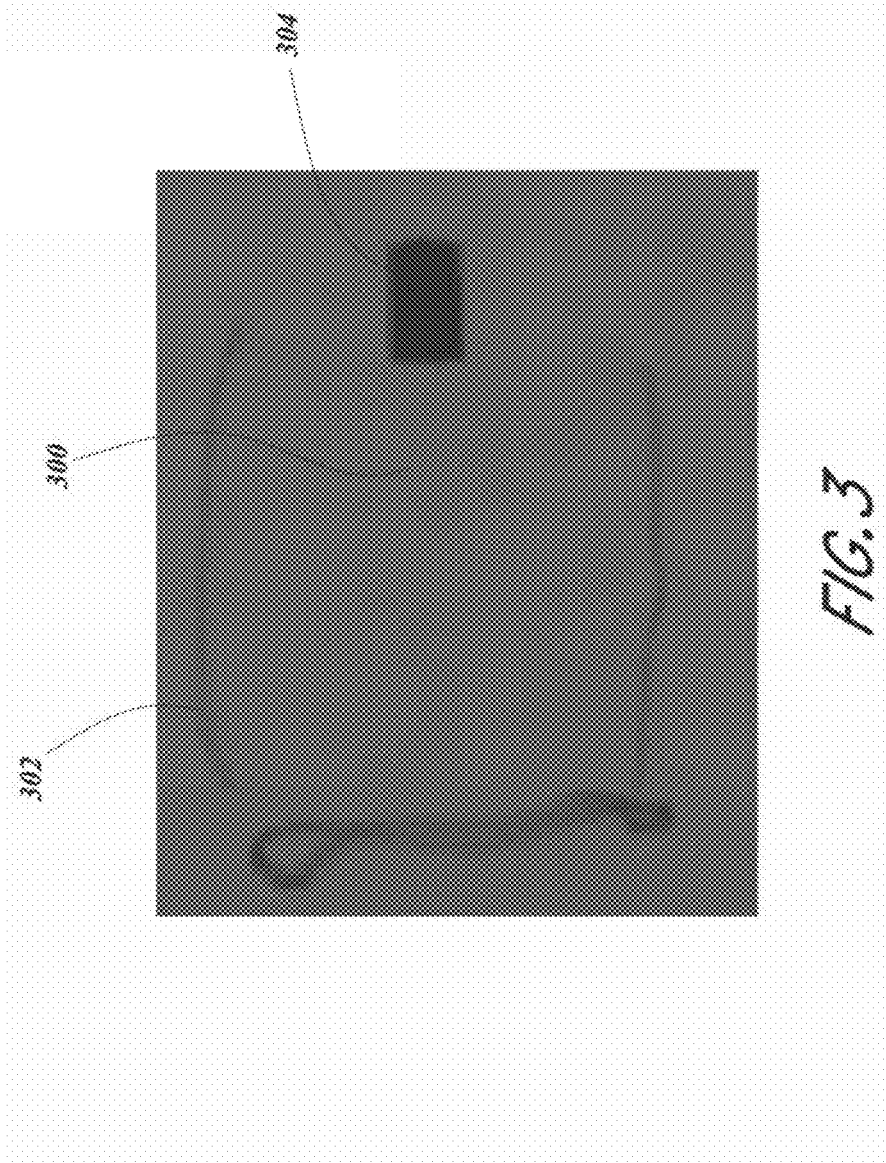


FIG. 2



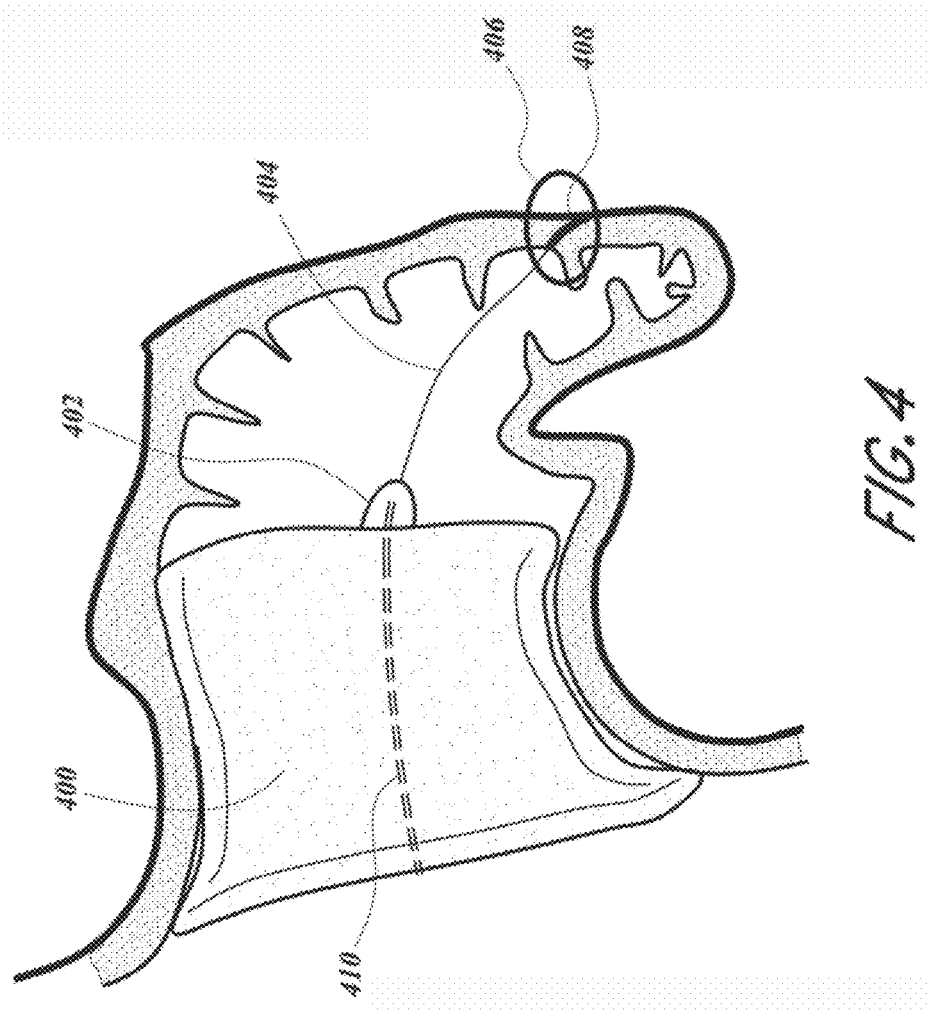
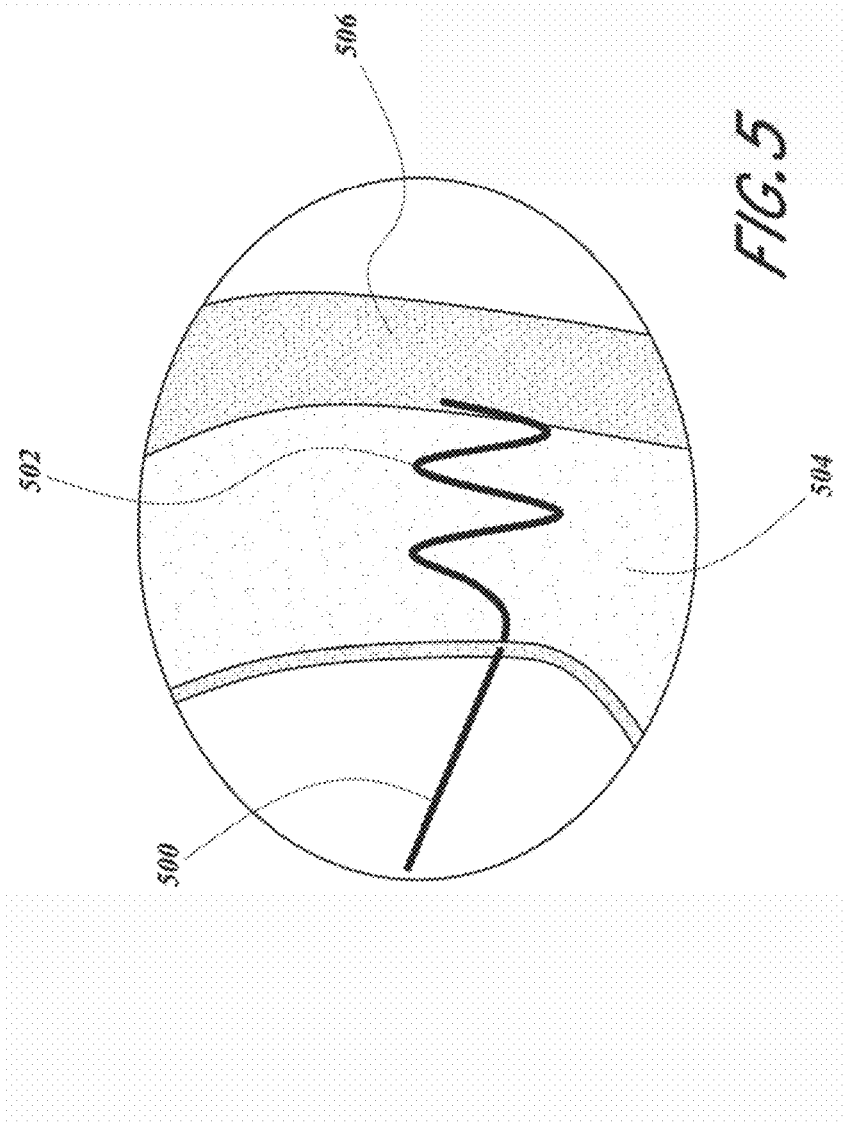


FIG. 4



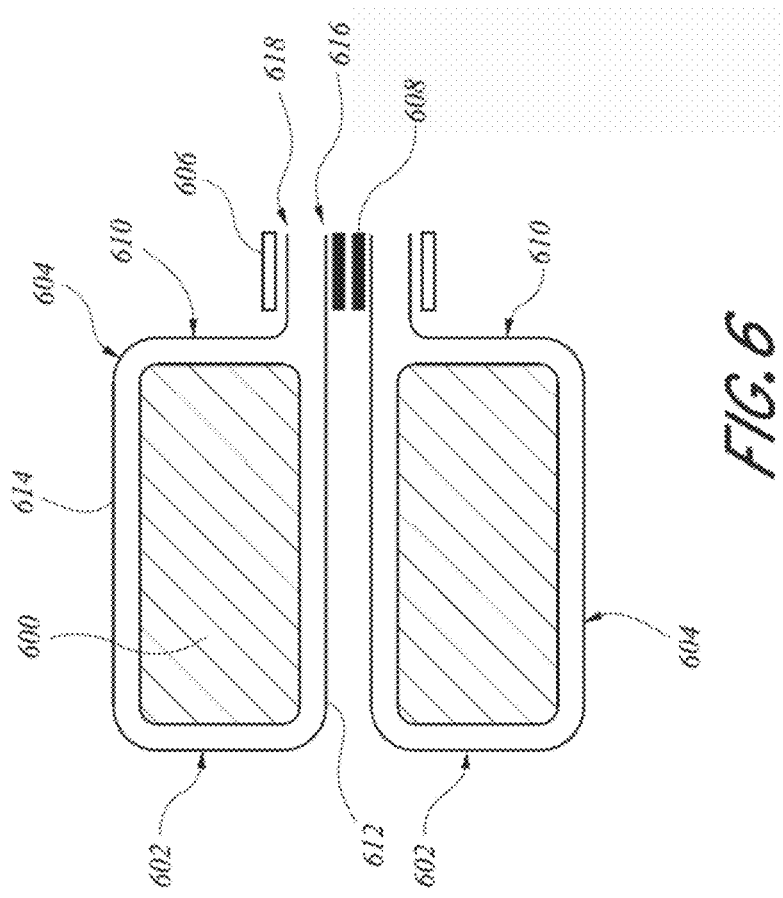


FIG. 6

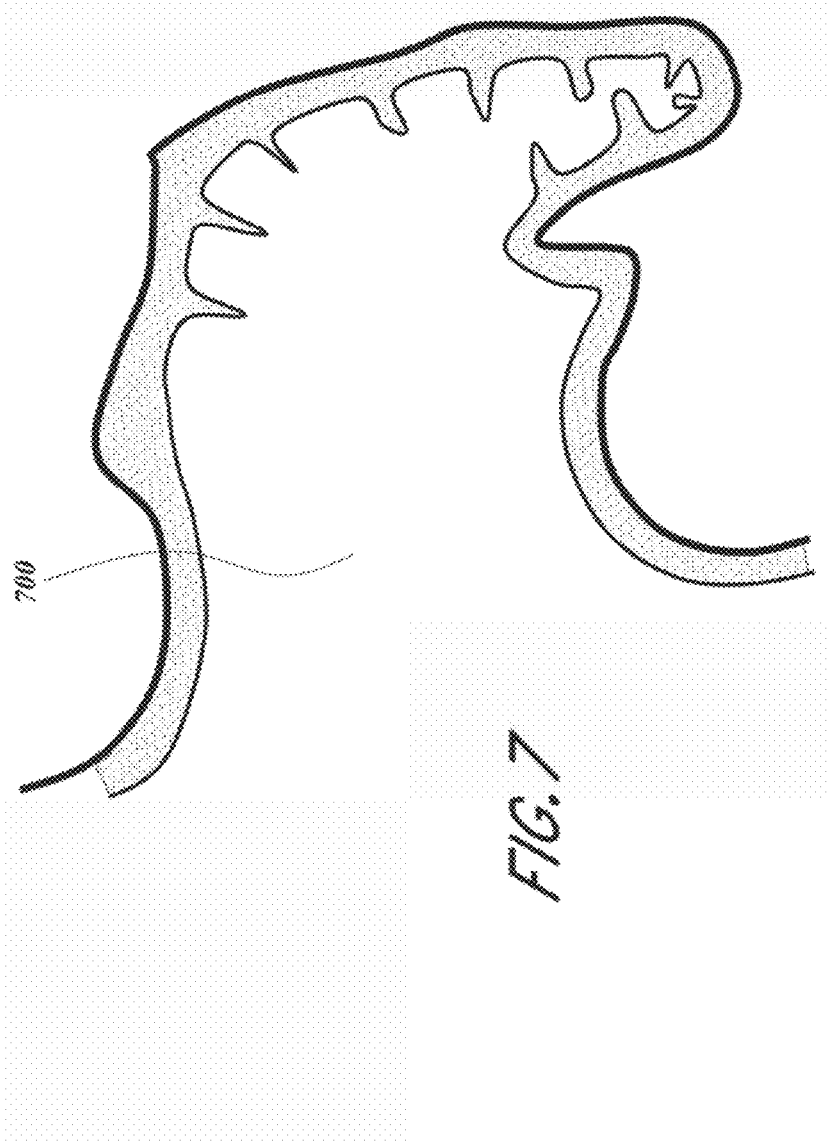
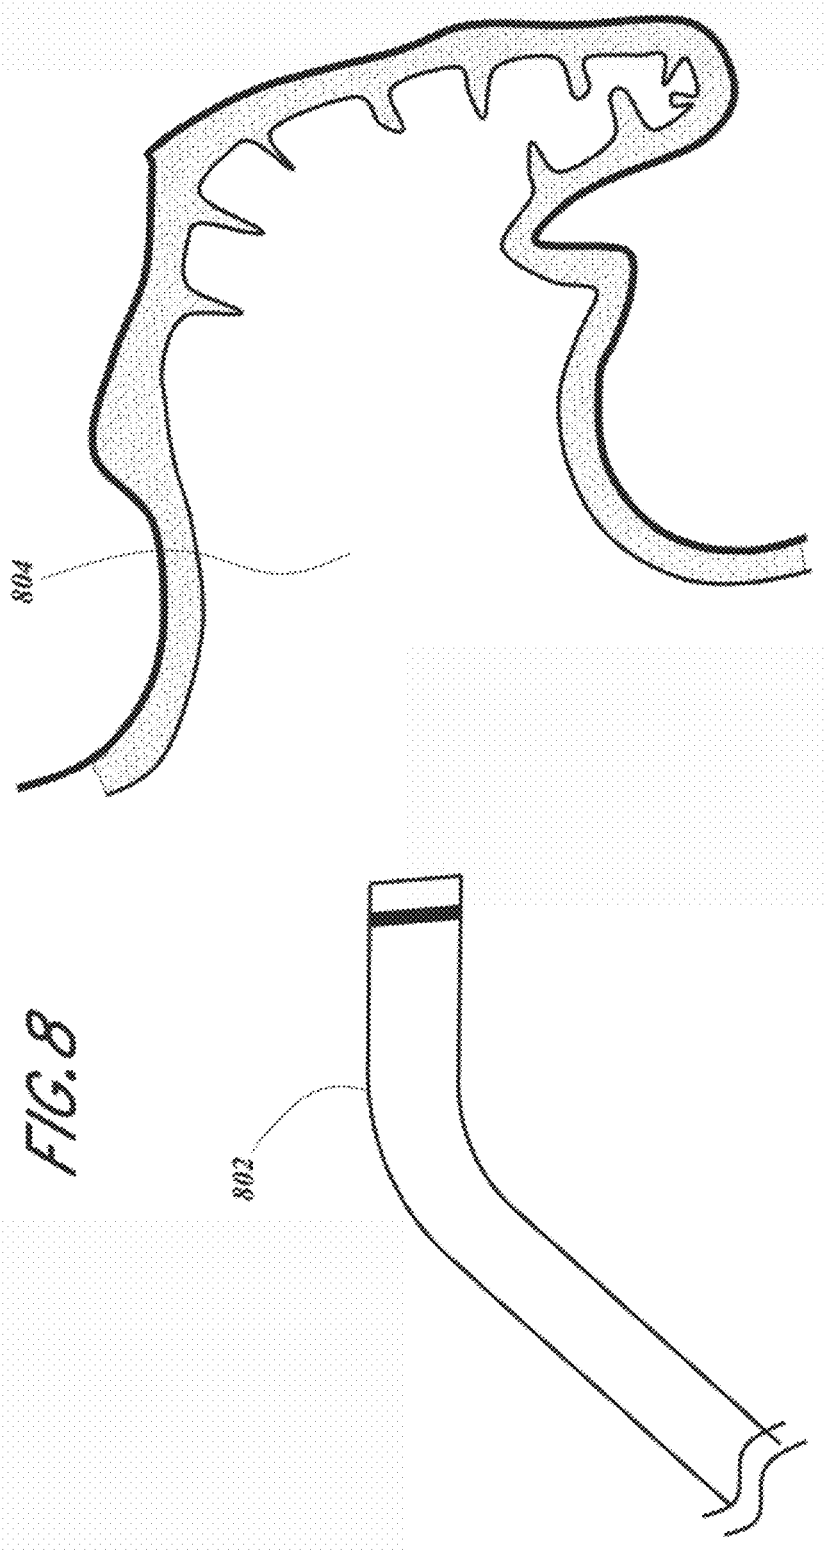


FIG. 7



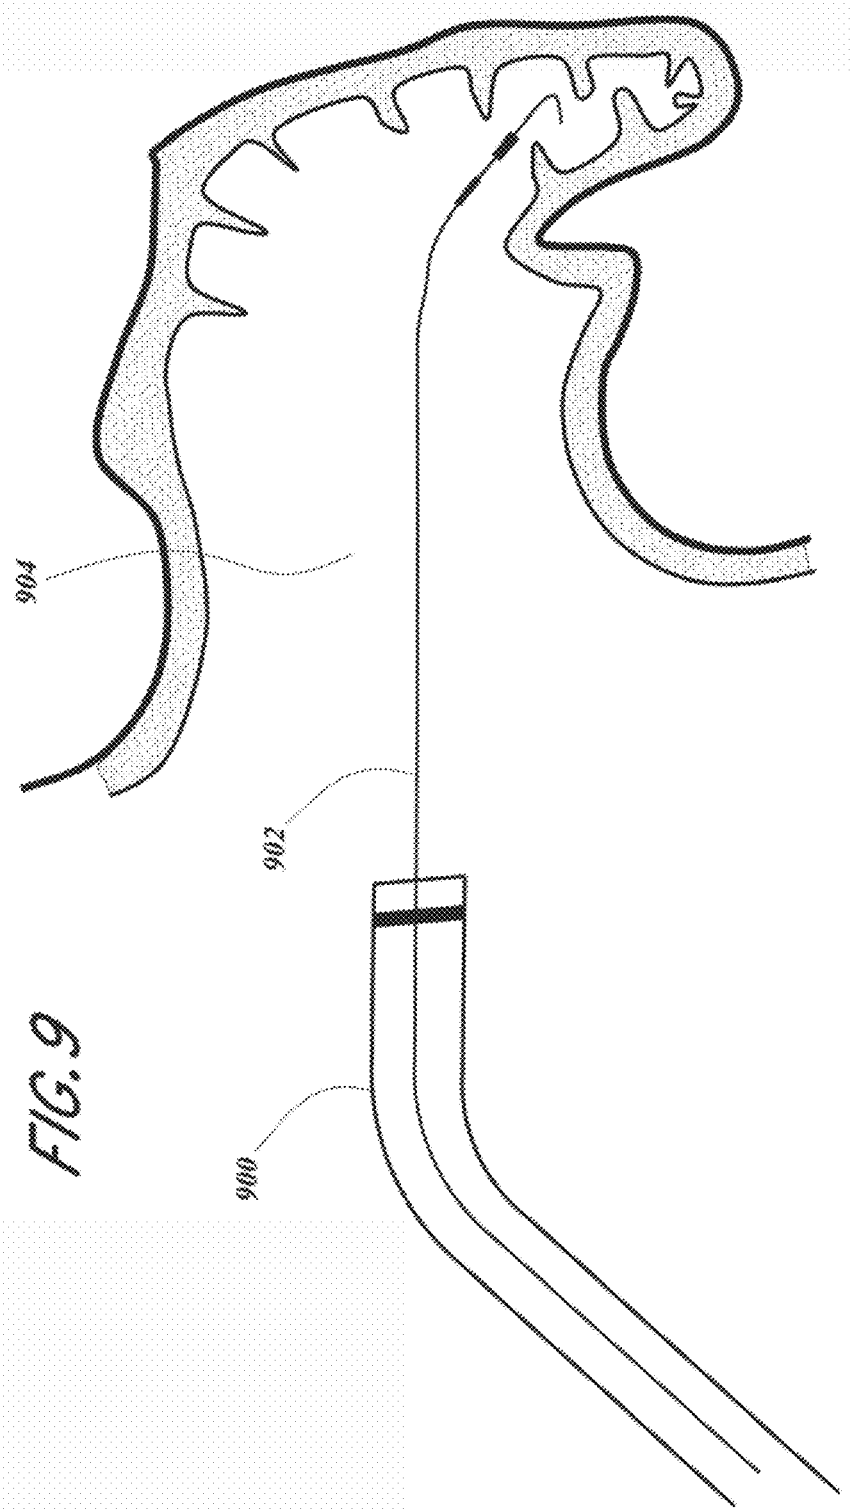


FIG. 9

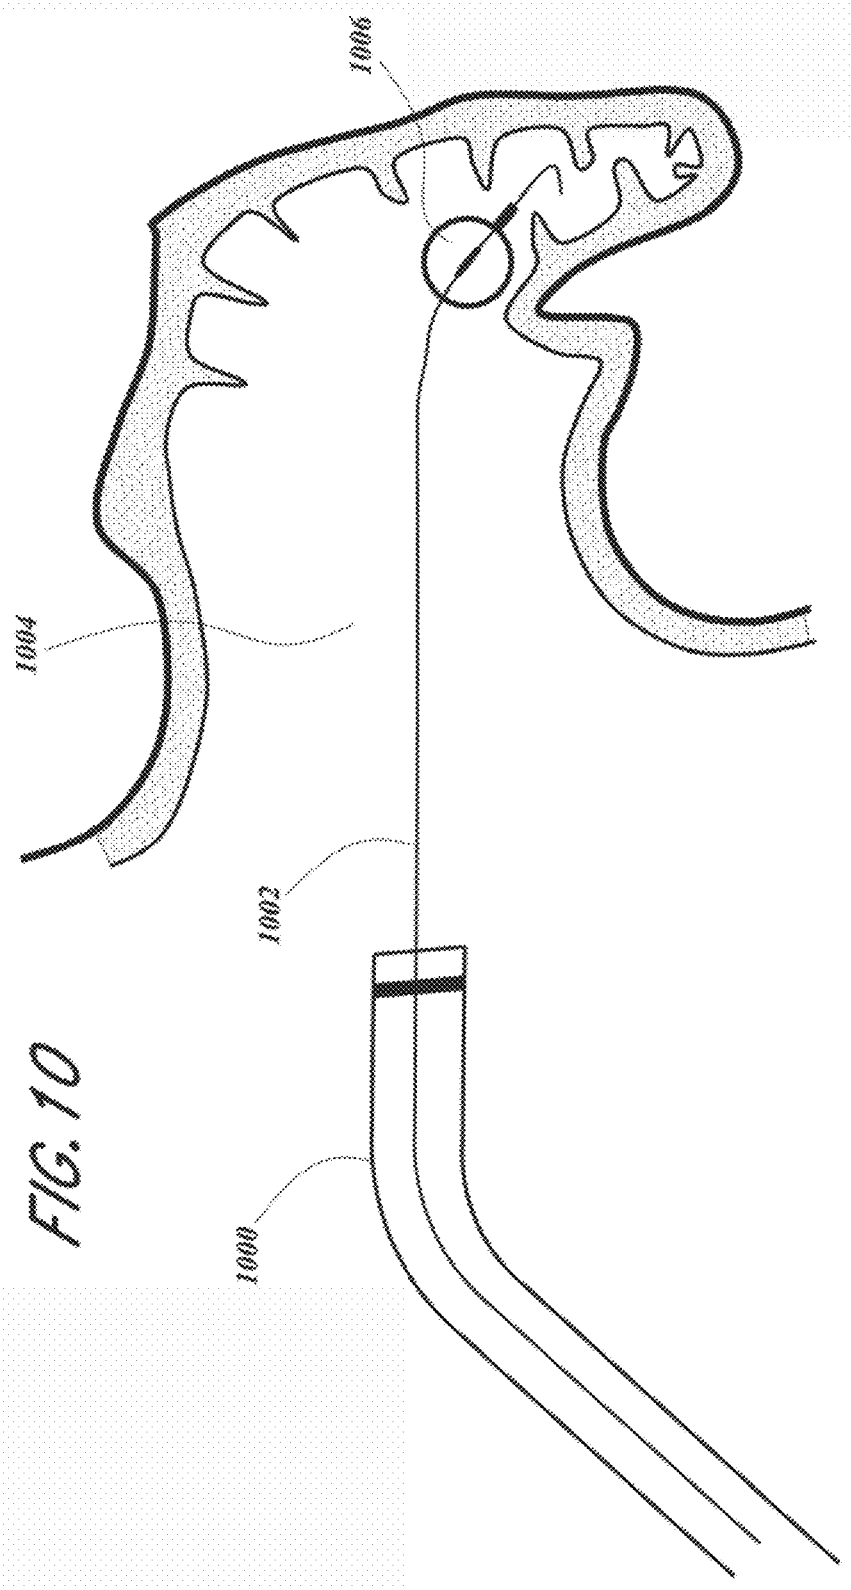


FIG. 10

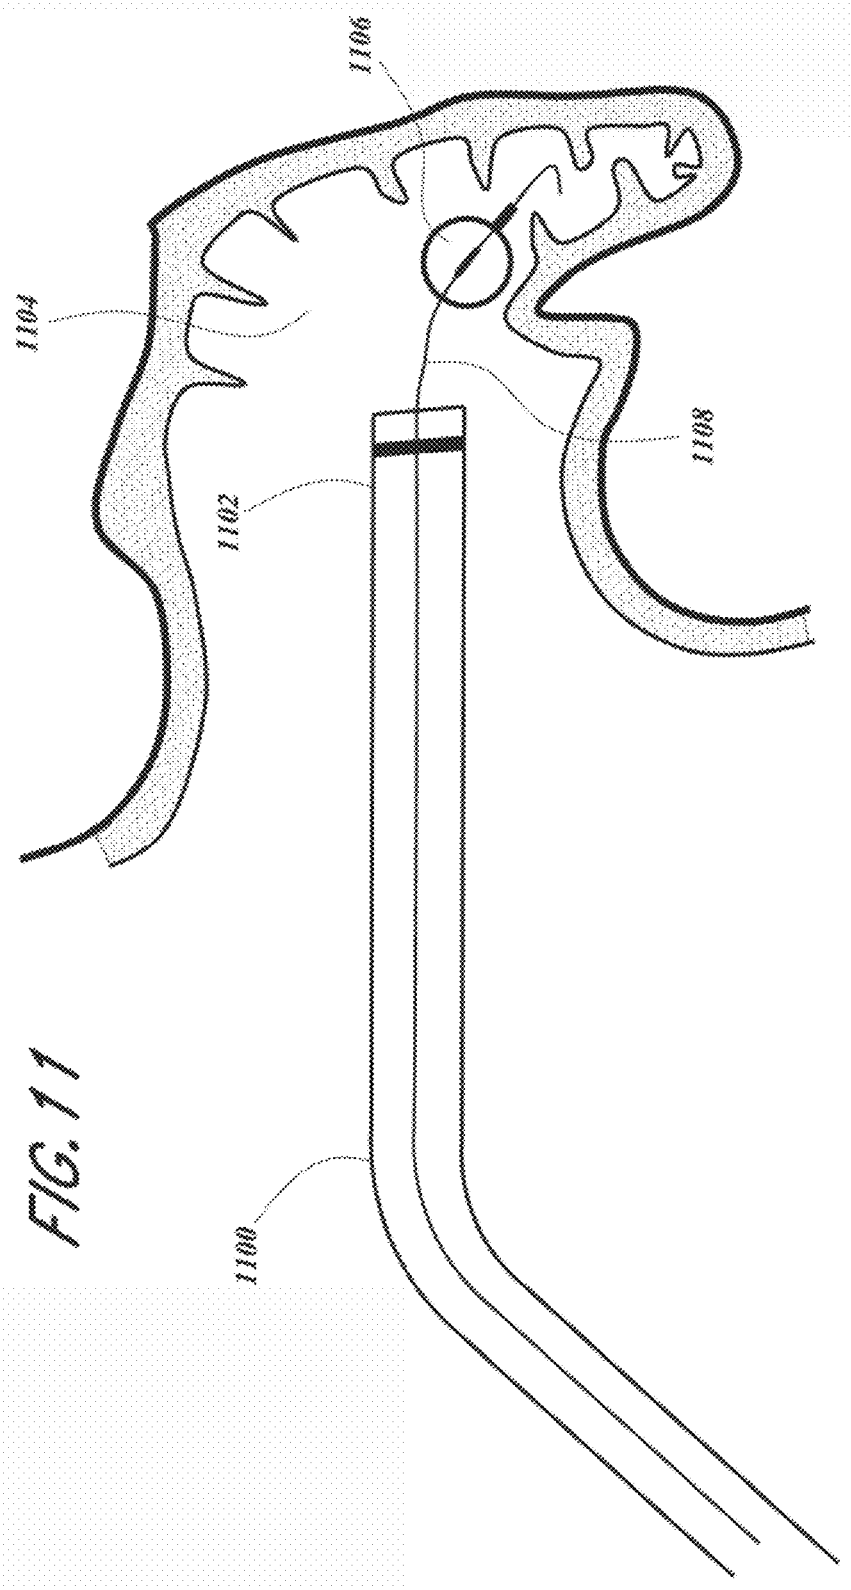
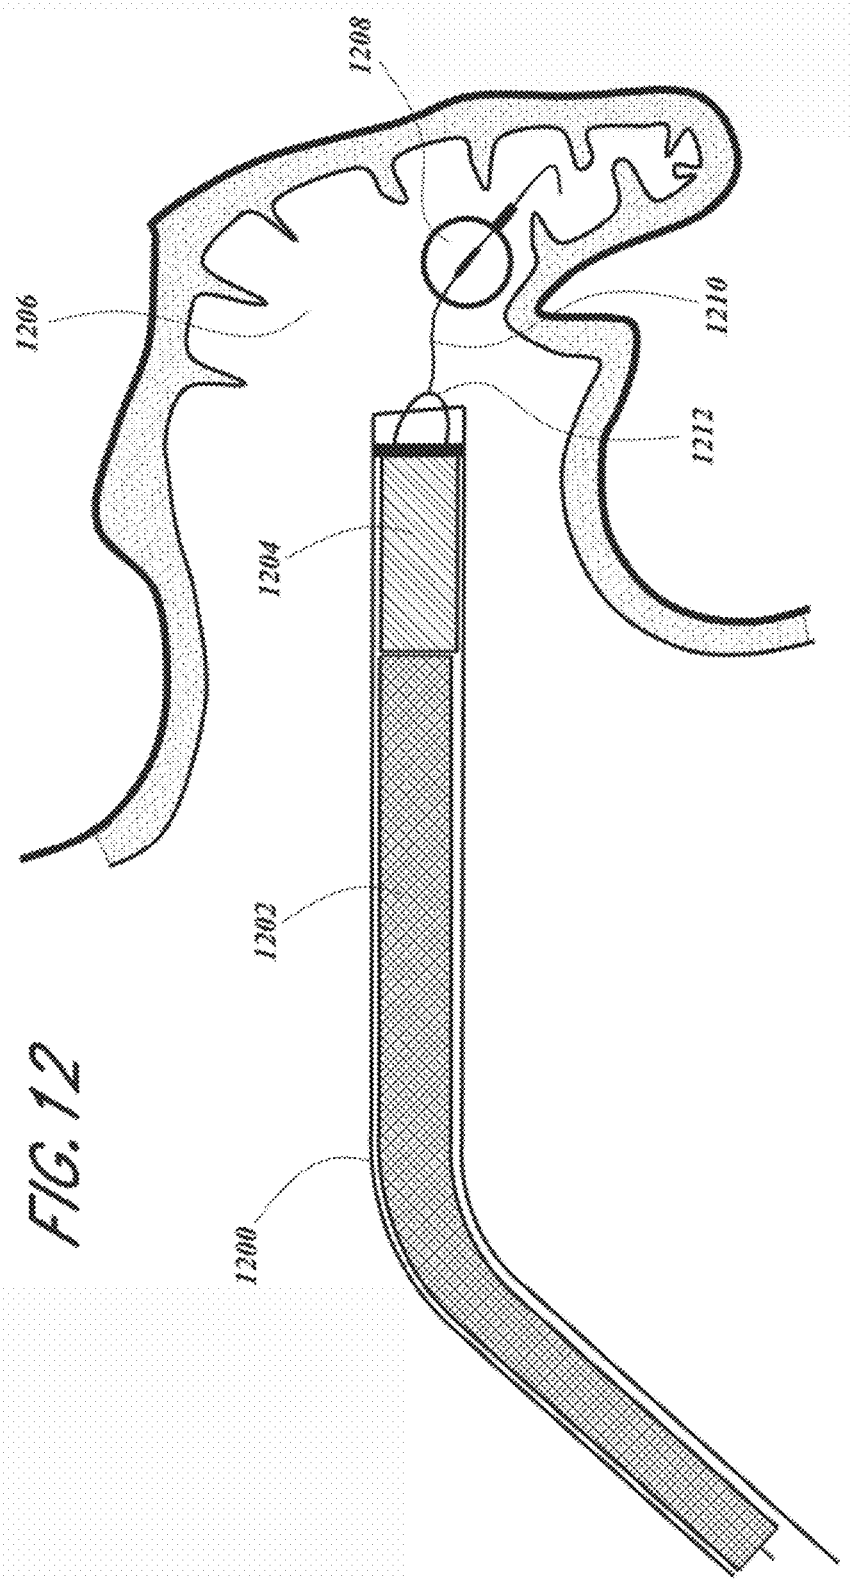


FIG. 11



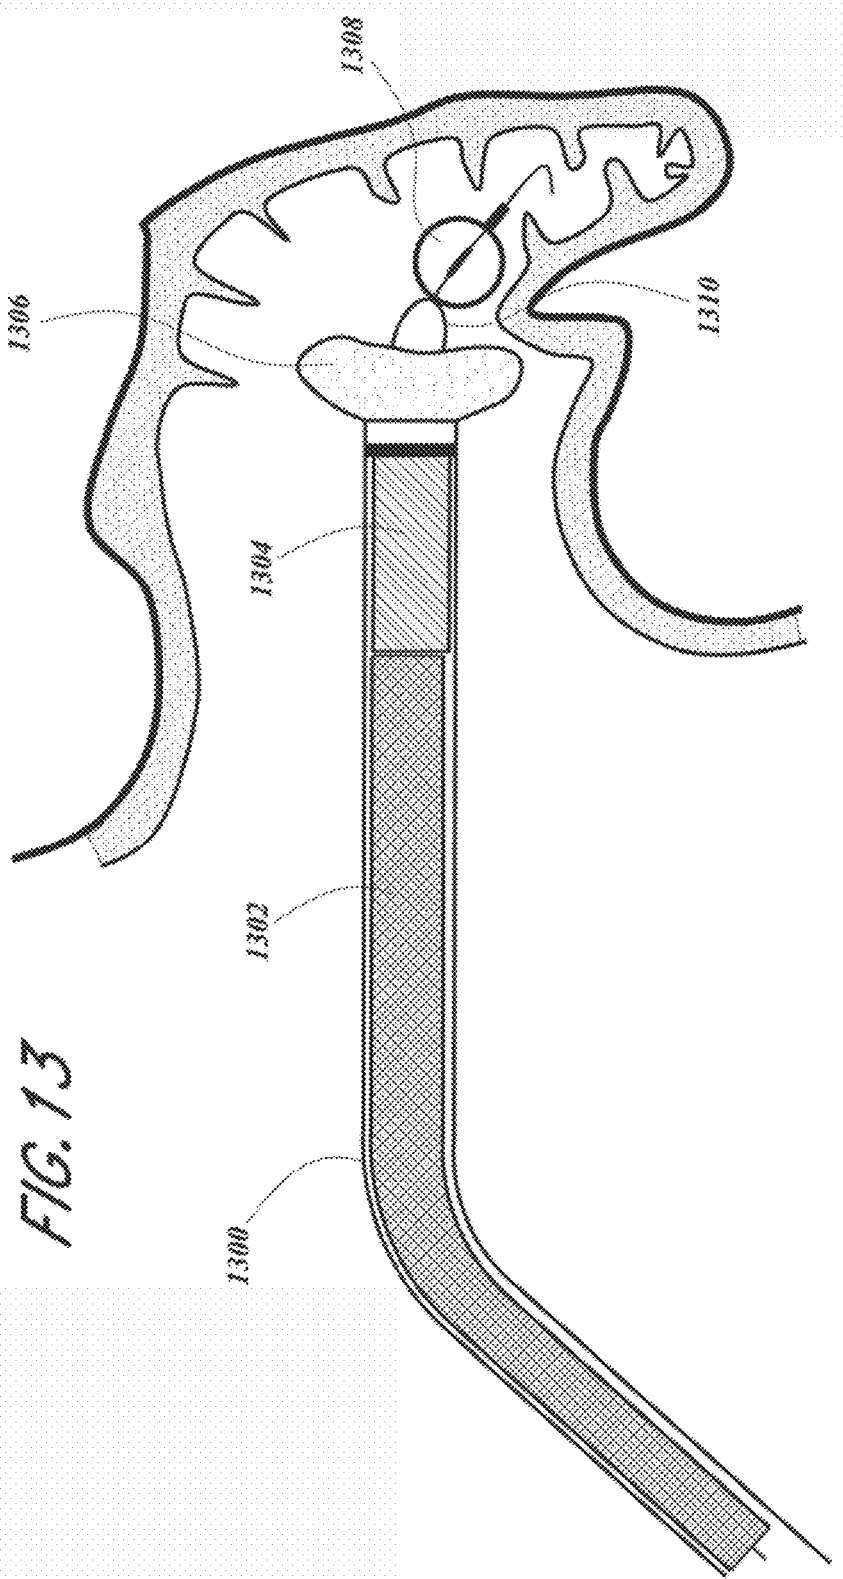


FIG. 13

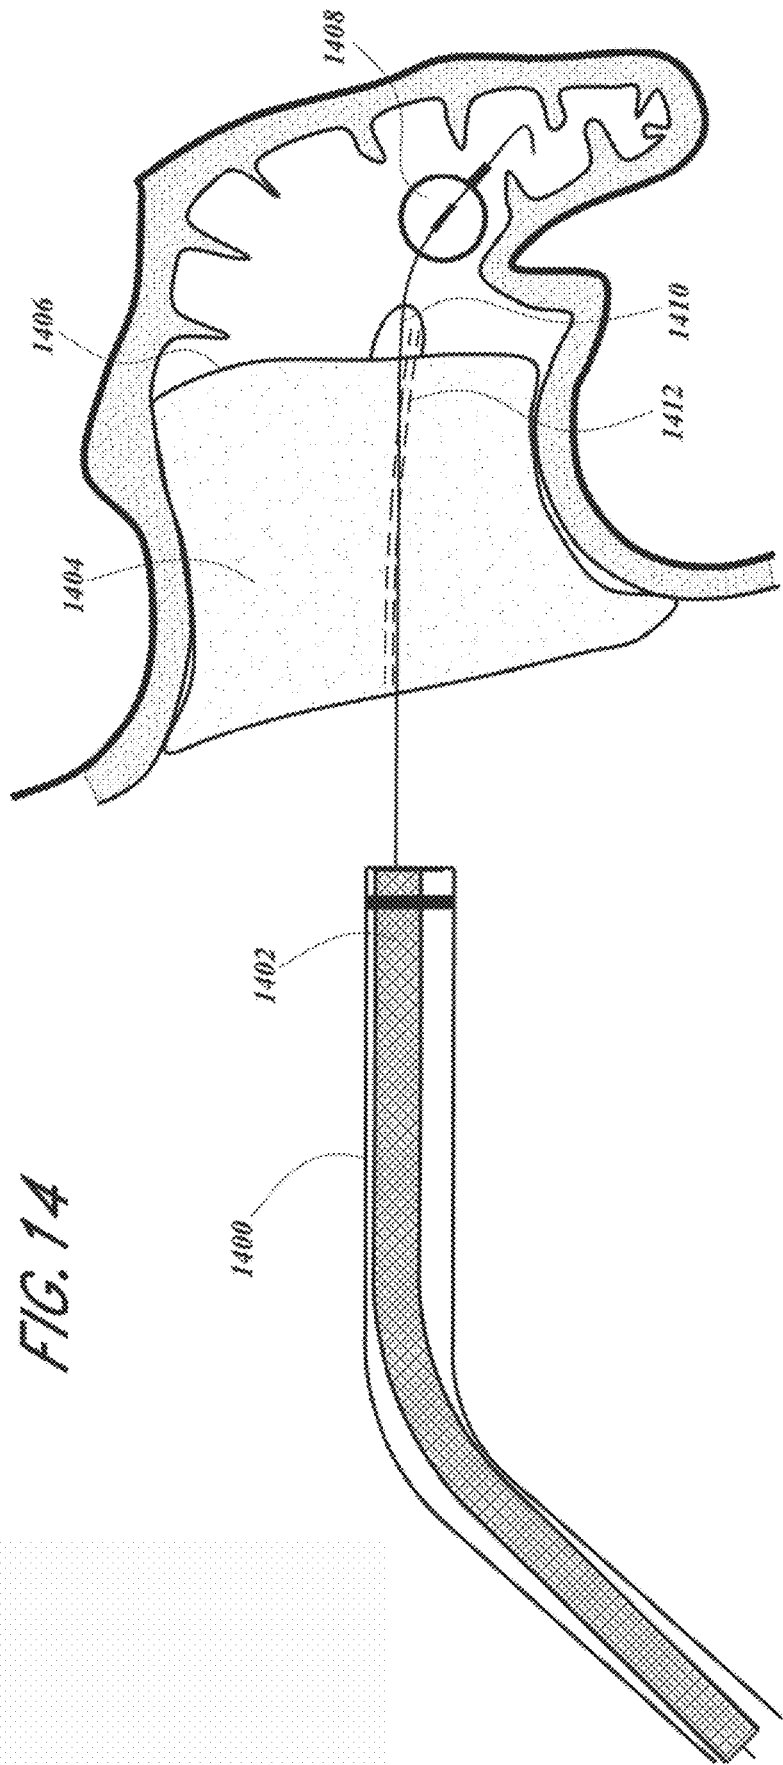
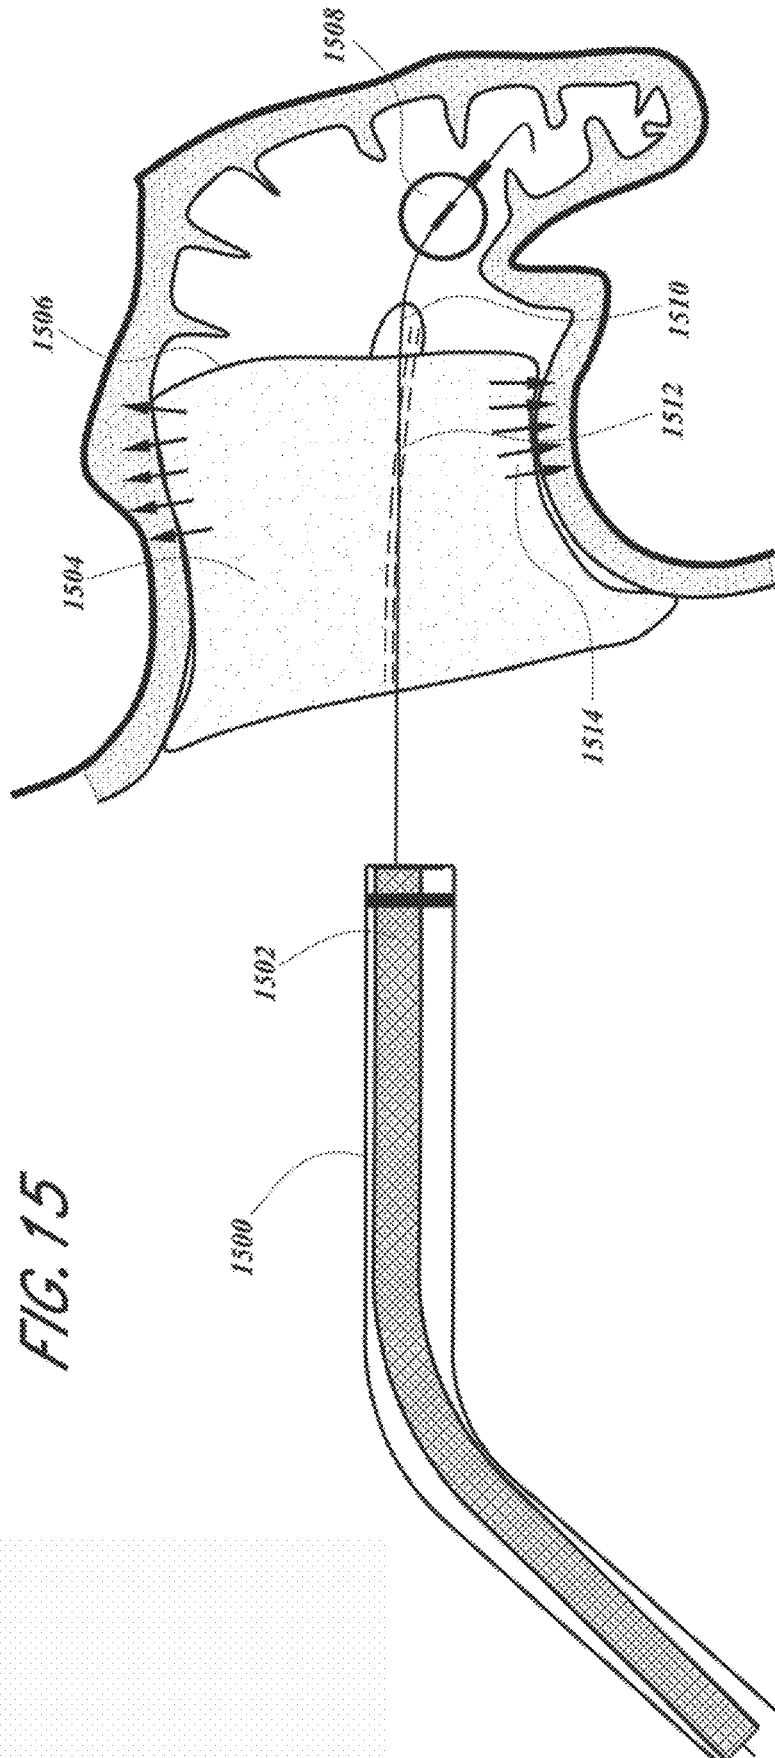


FIG. 14



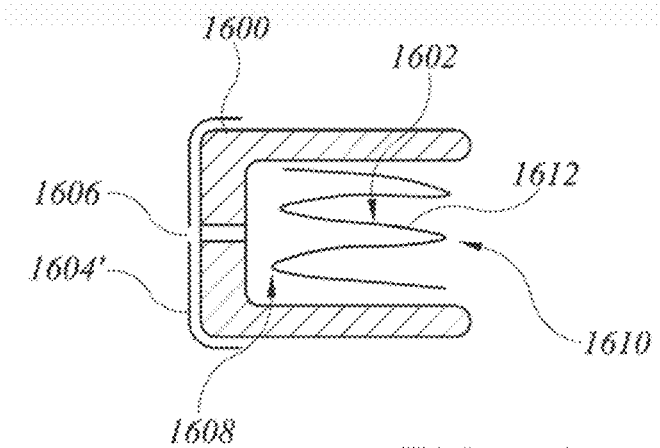


FIG. 16

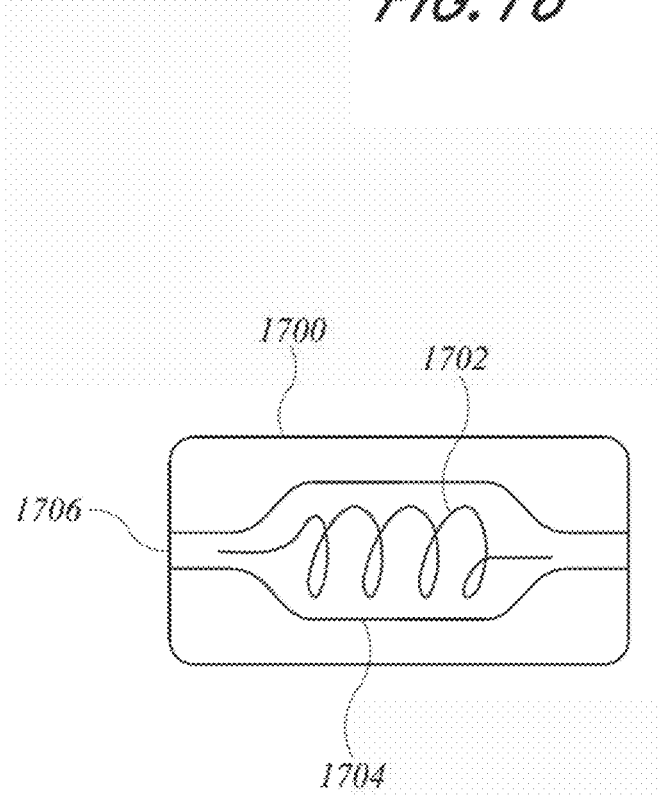


FIG. 17

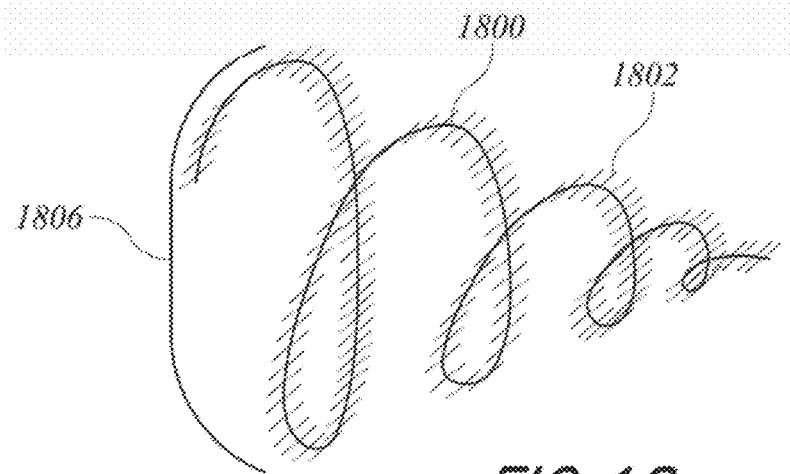


FIG. 18

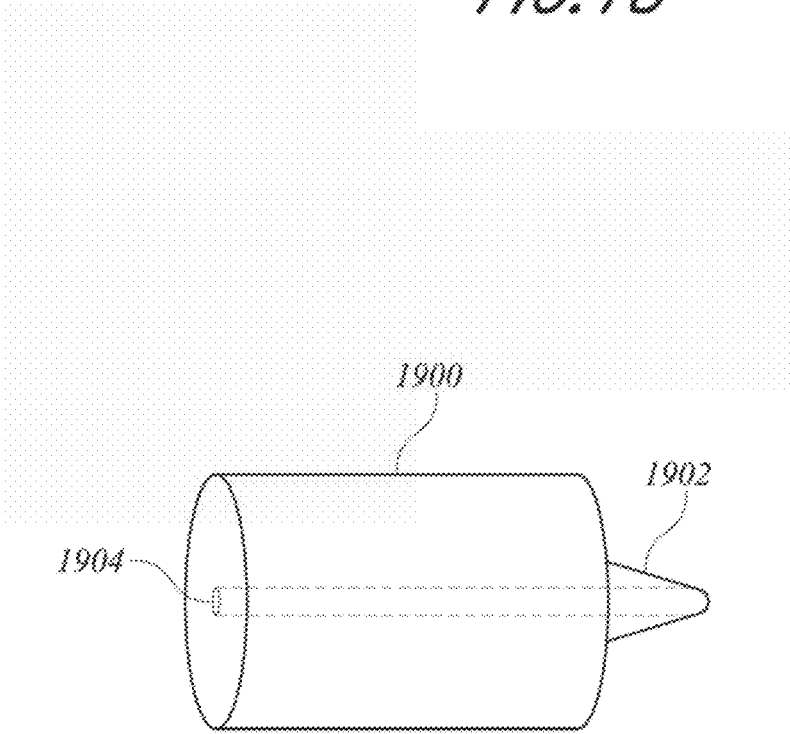


FIG. 19

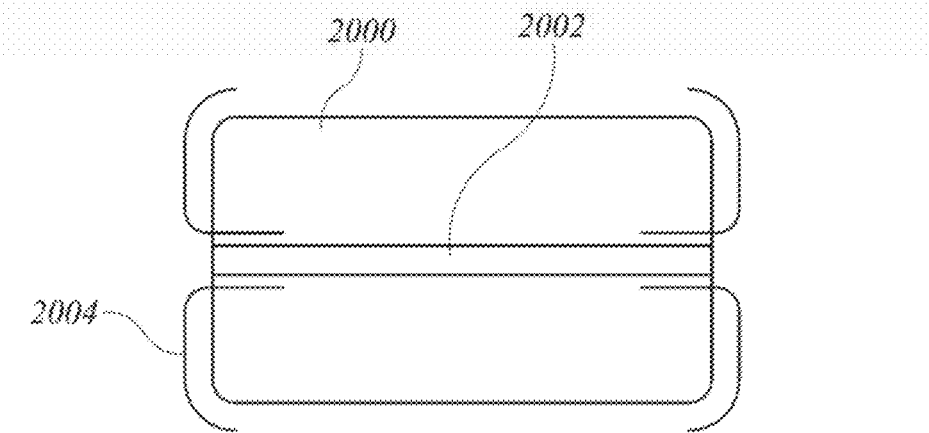


FIG. 20

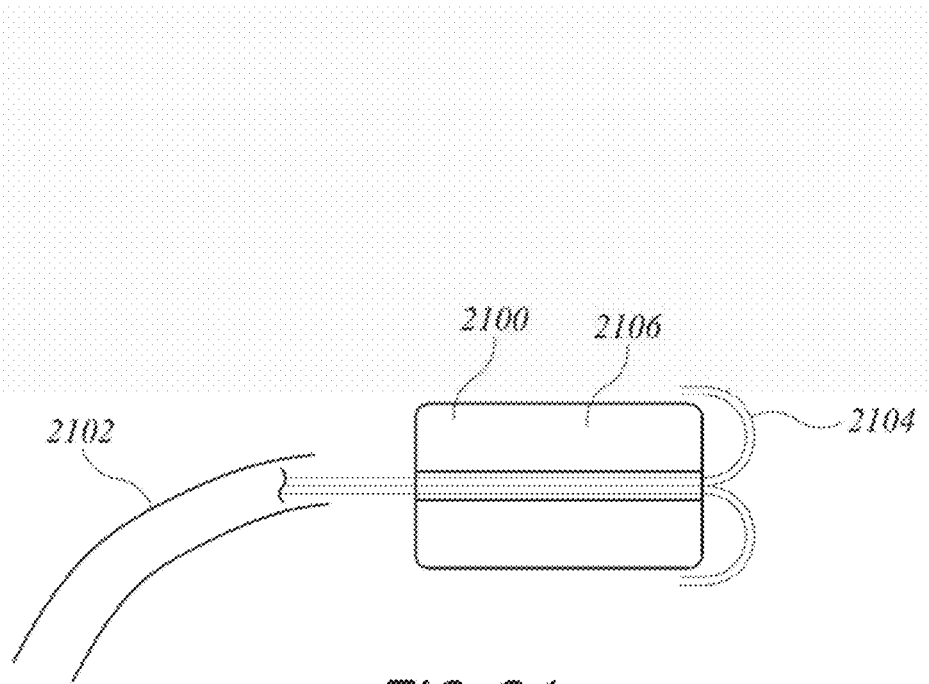


FIG. 21

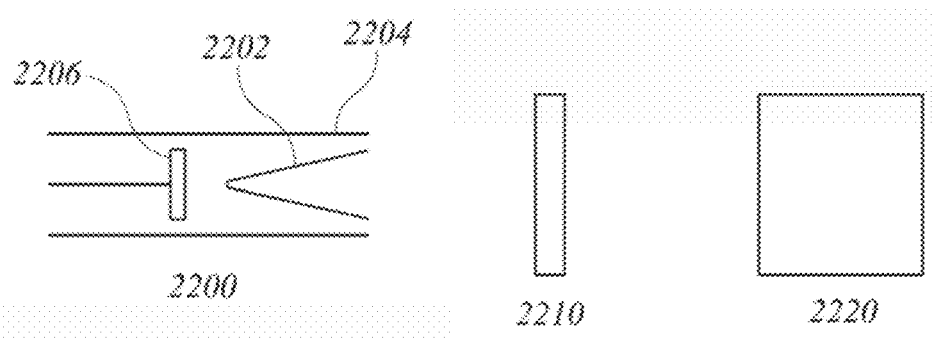


FIG. 22

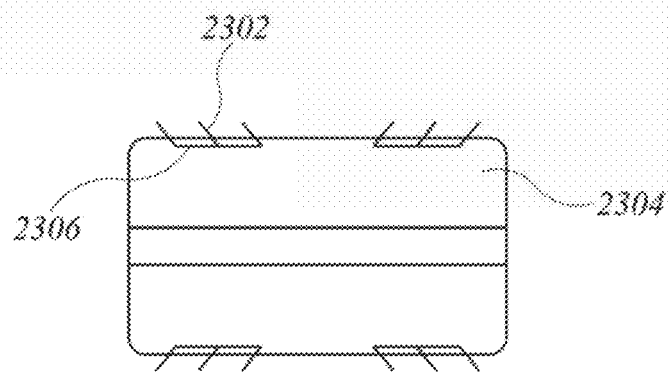
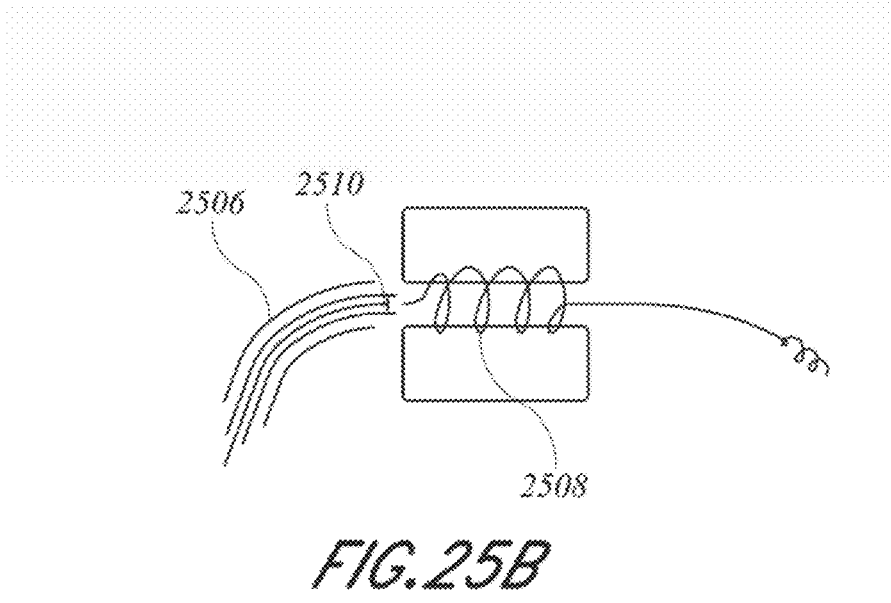
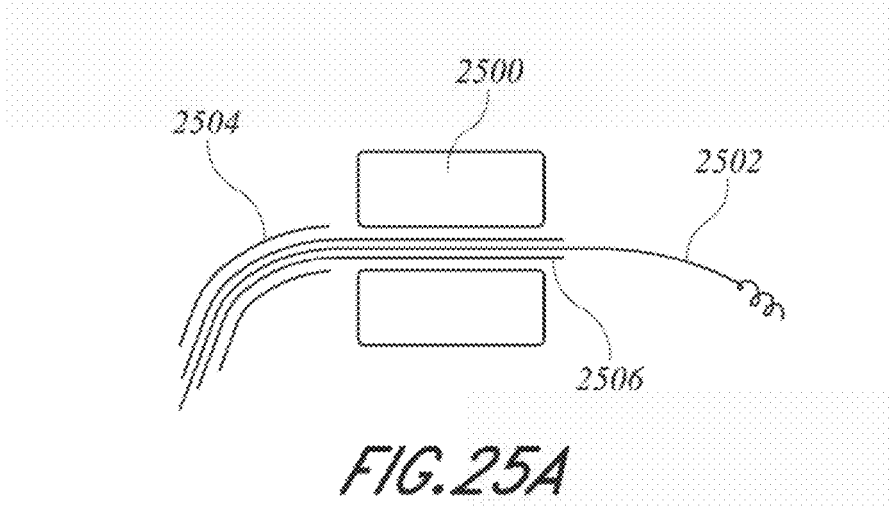
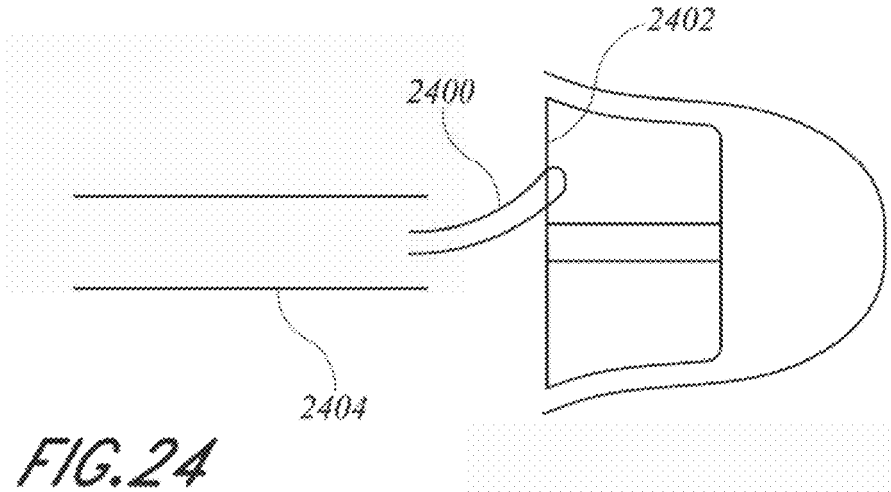


FIG. 23



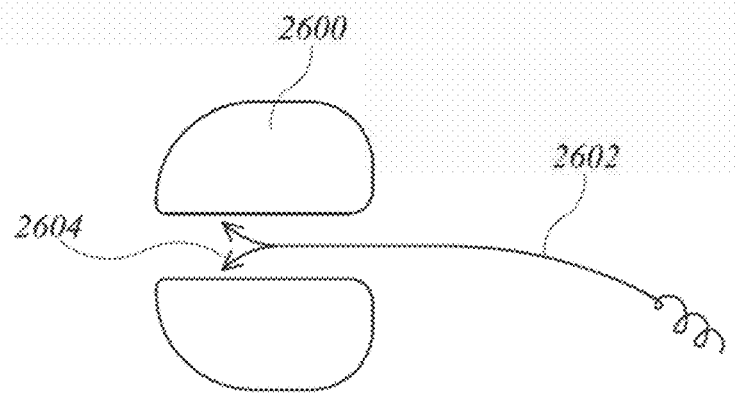


FIG. 26


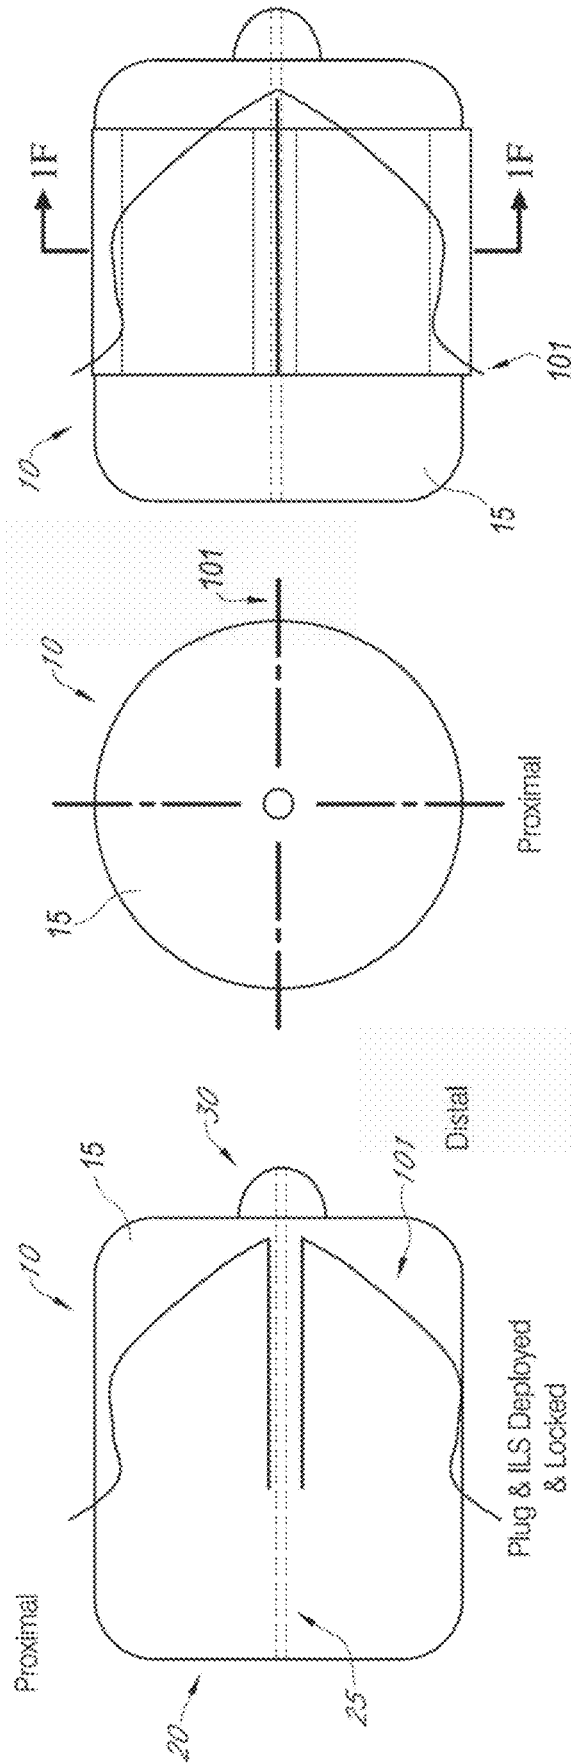


FIG. 27C


FIG. 27B

FIG. 27A

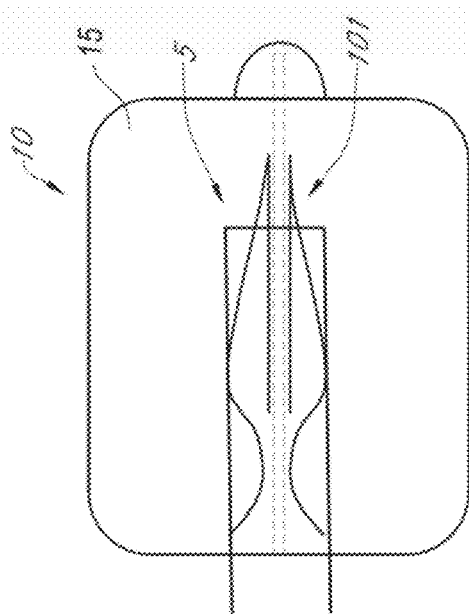

Plug Deployed

FIG. 27D

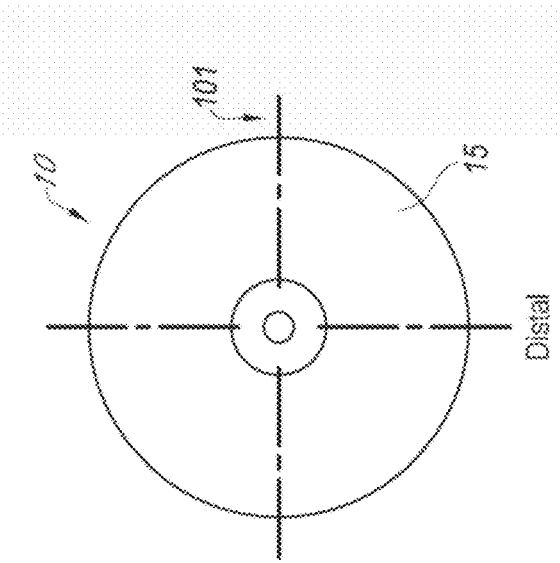

Distal

FIG. 27E


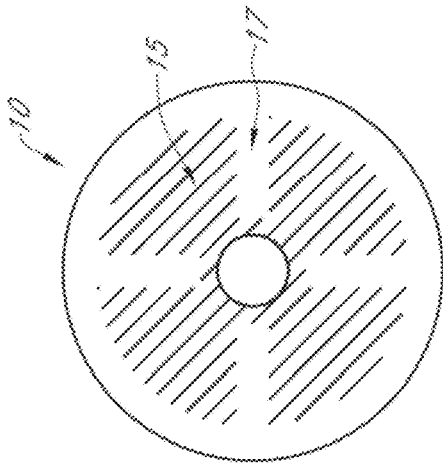


FIG. 27F

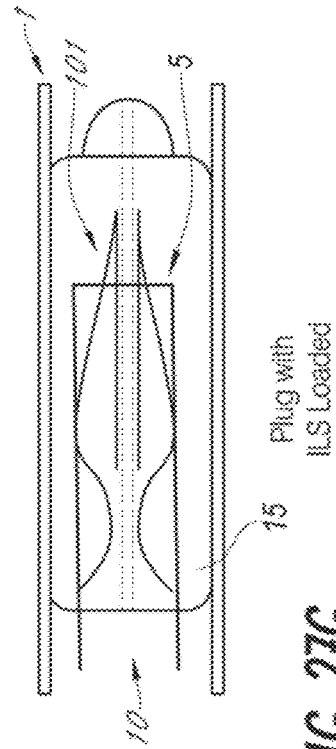

Plug with ILS Loaded

FIG. 27G

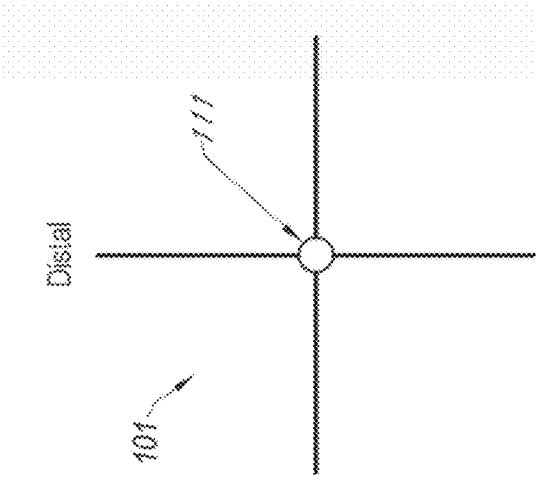


FIG. 28B

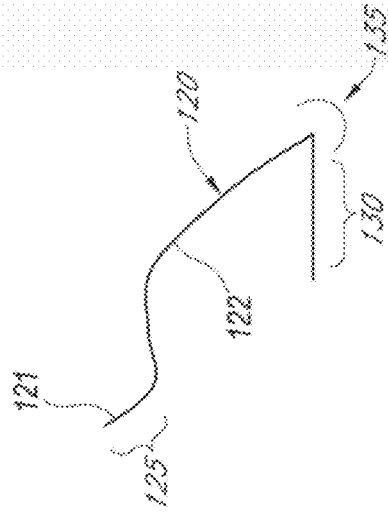


FIG. 28D

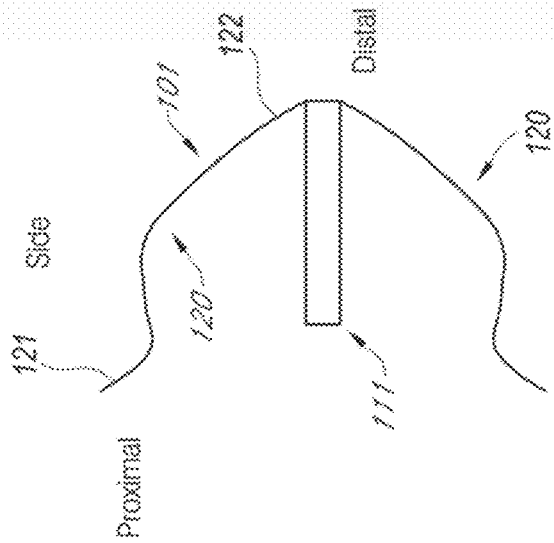


FIG. 28A

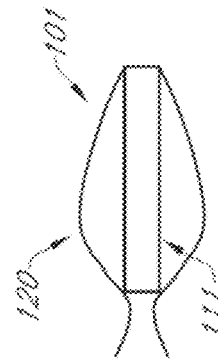


FIG. 28C

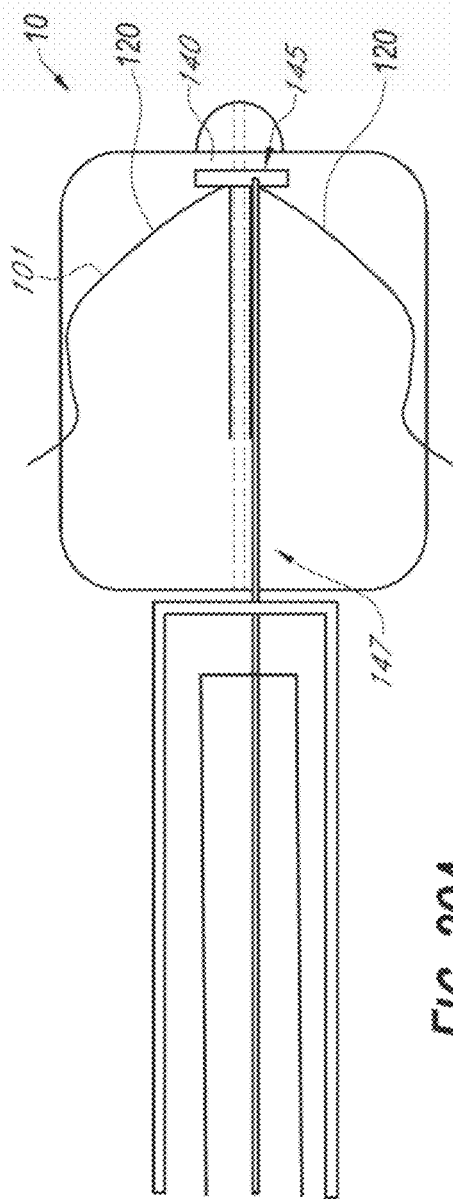


FIG. 29A

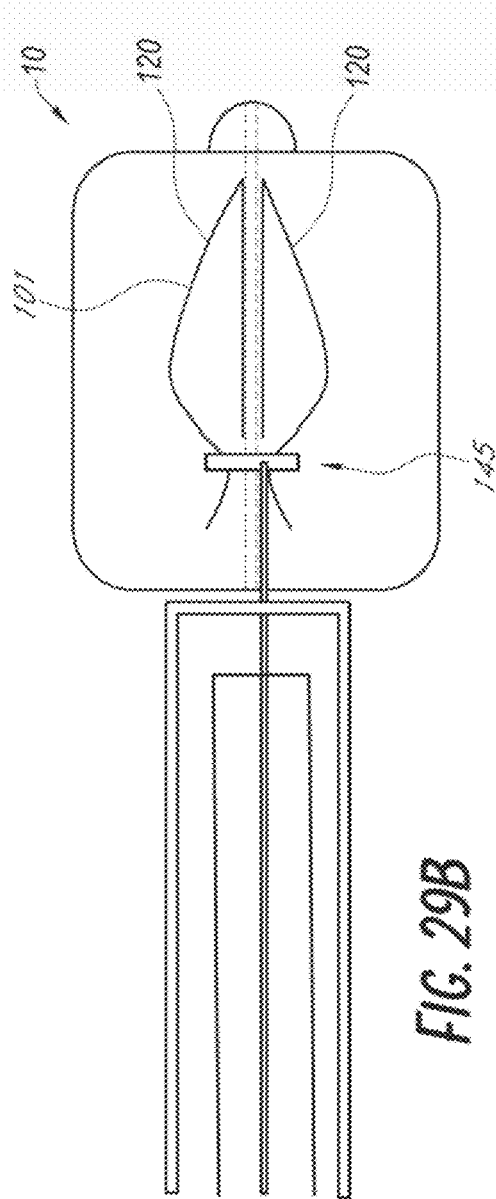


FIG. 29B

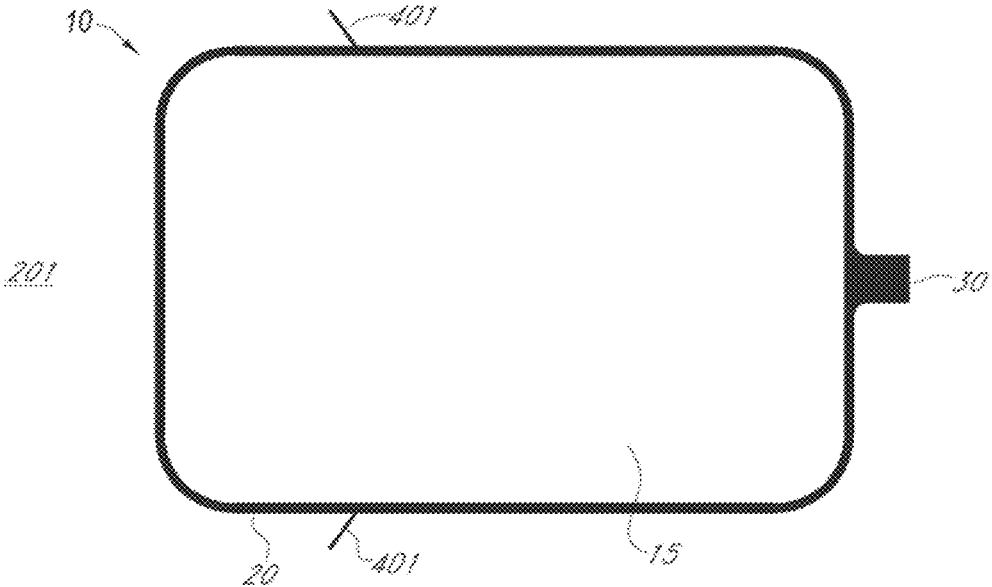


FIG. 30

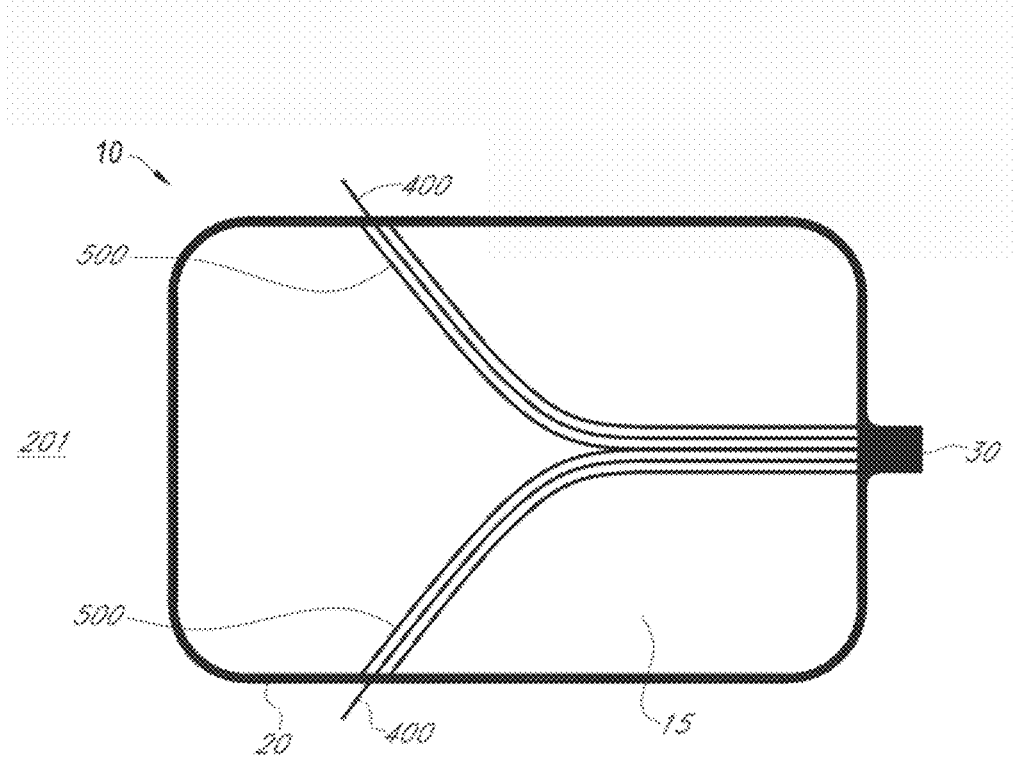


FIG. 31

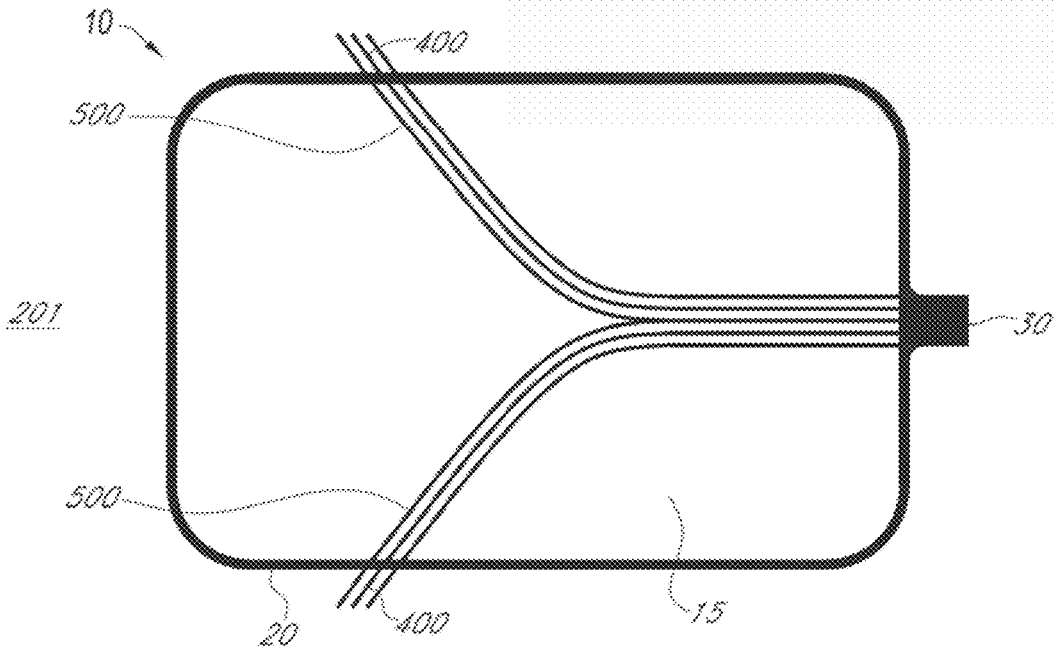


FIG. 32

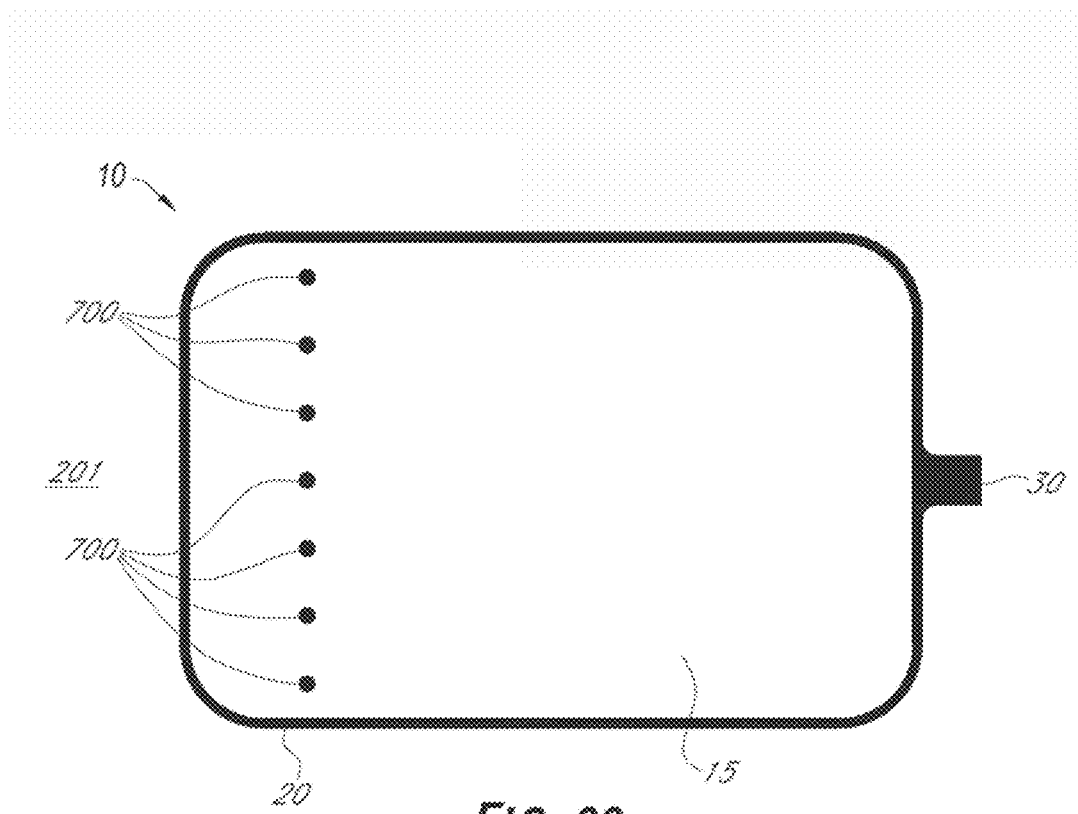


FIG. 33

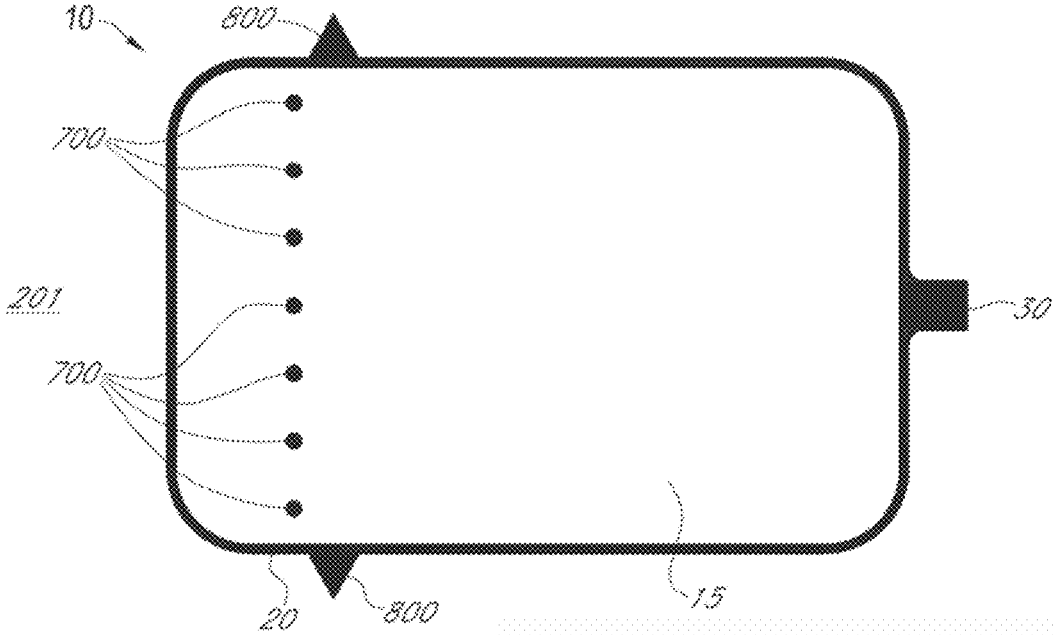


FIG. 34

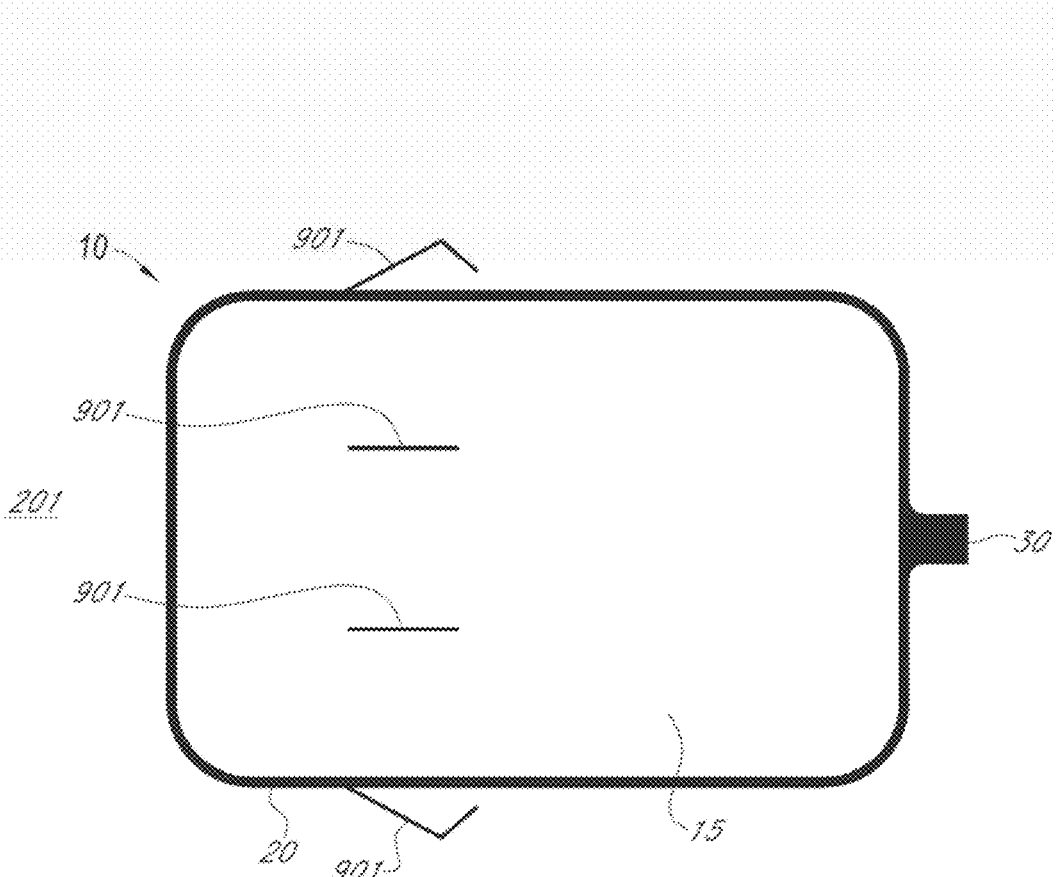


FIG. 35

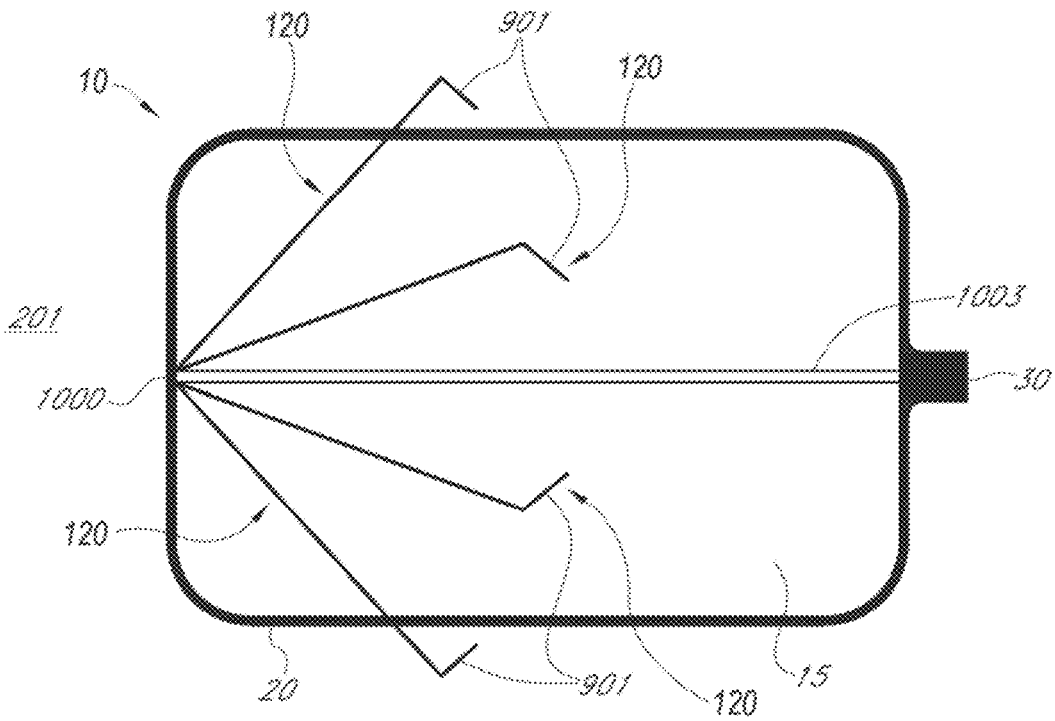


FIG. 36



FIG. 37A



FIG. 37B



FIG. 37C

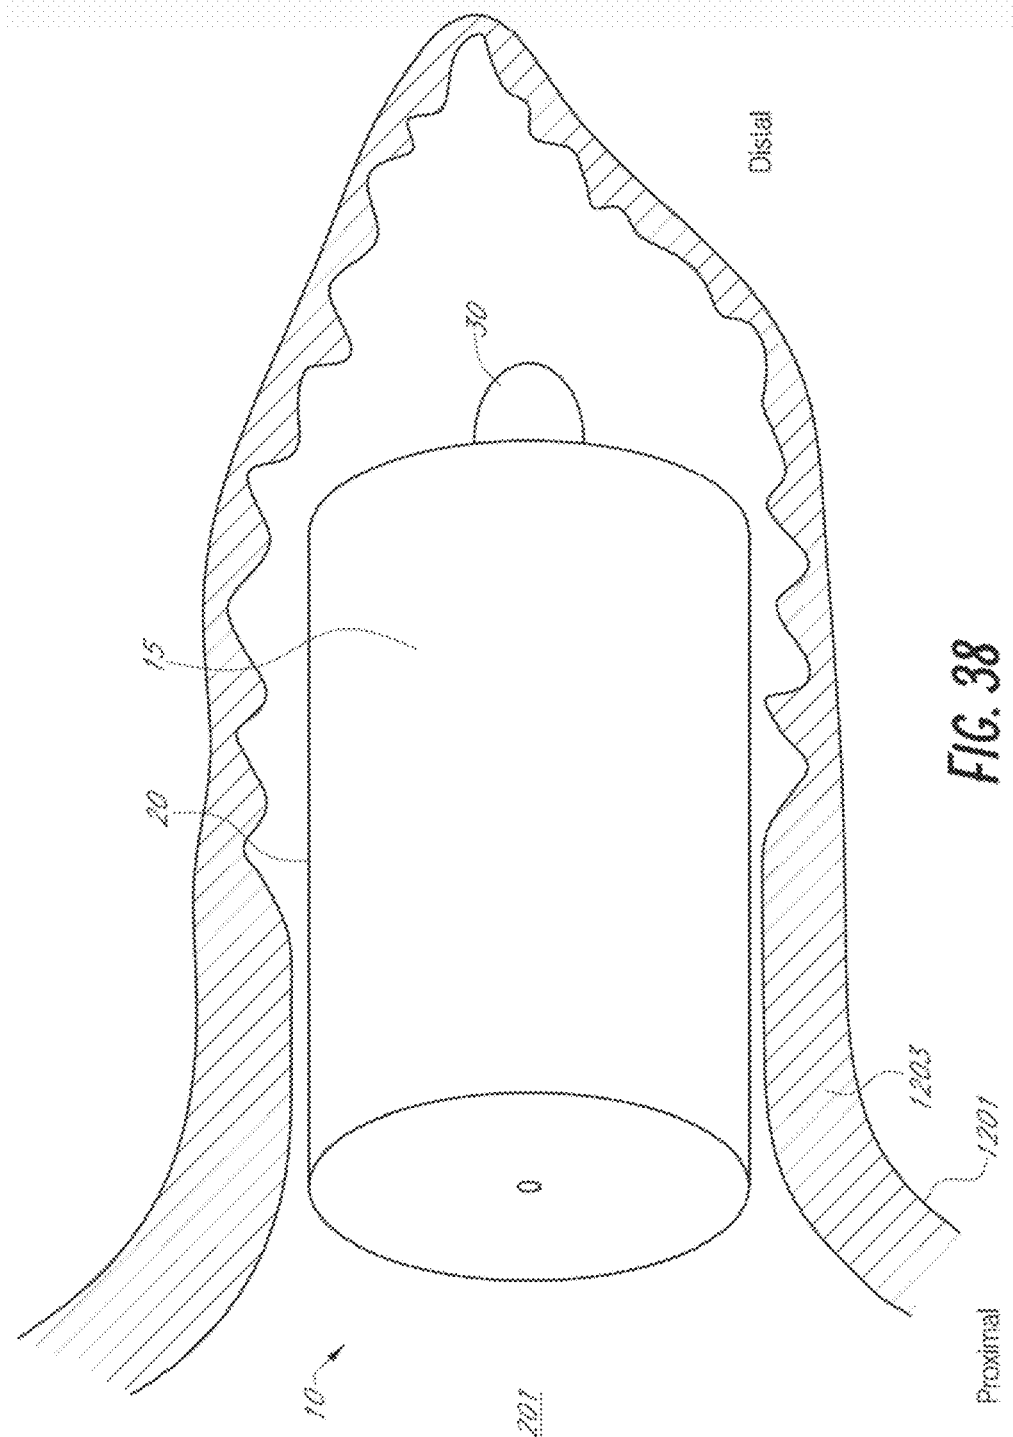


FIG. 38

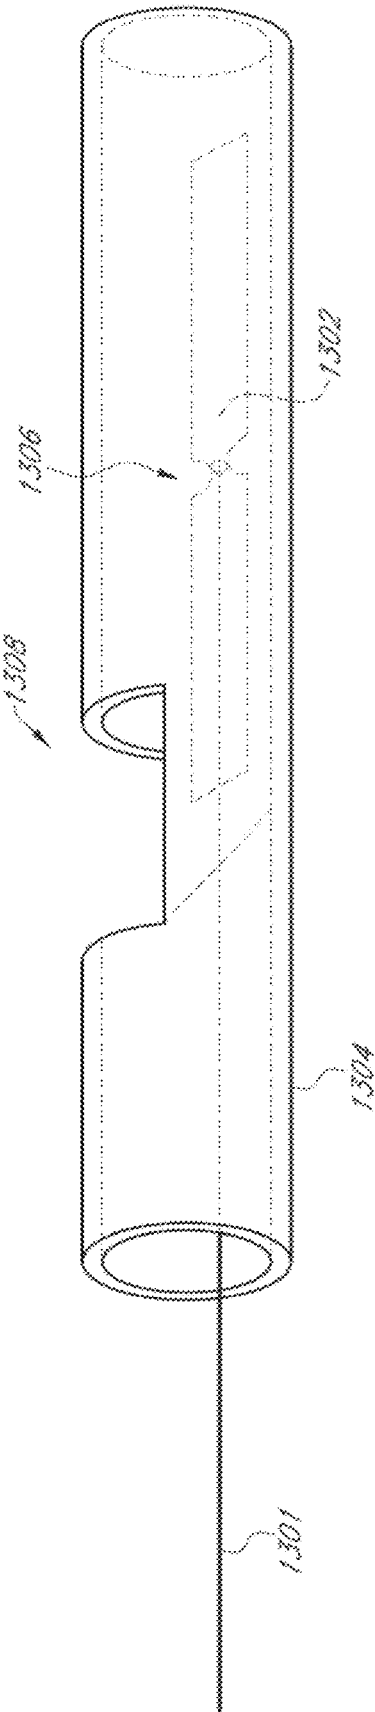


FIG. 39A

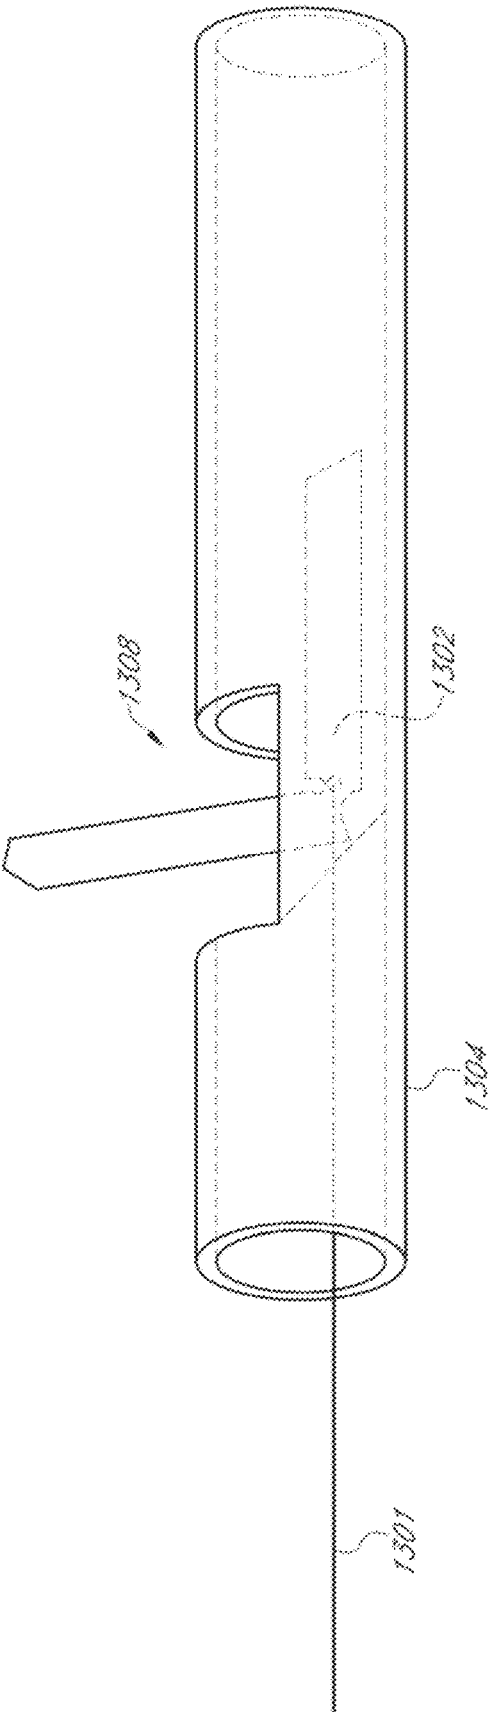


FIG. 39B

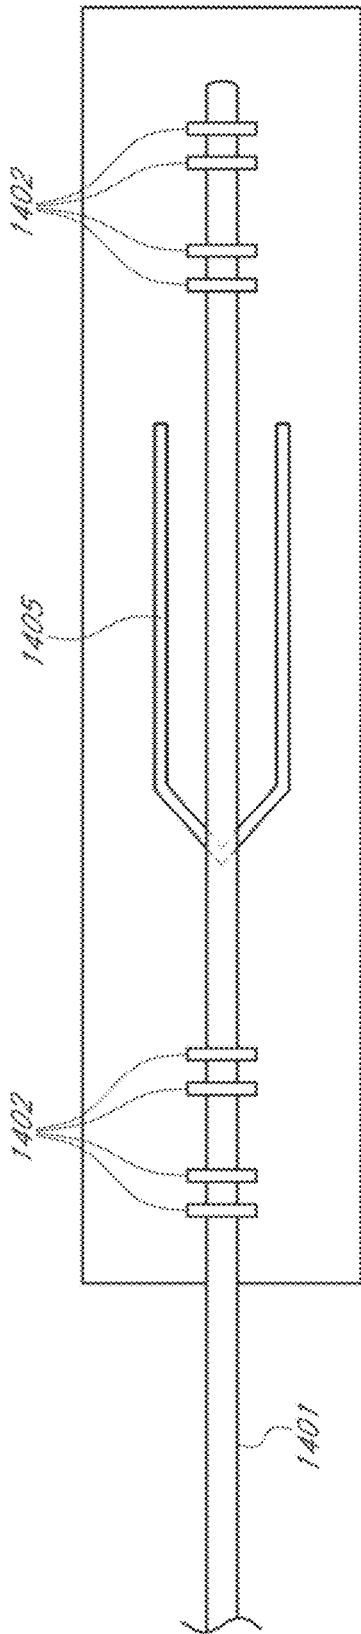


FIG. 40A

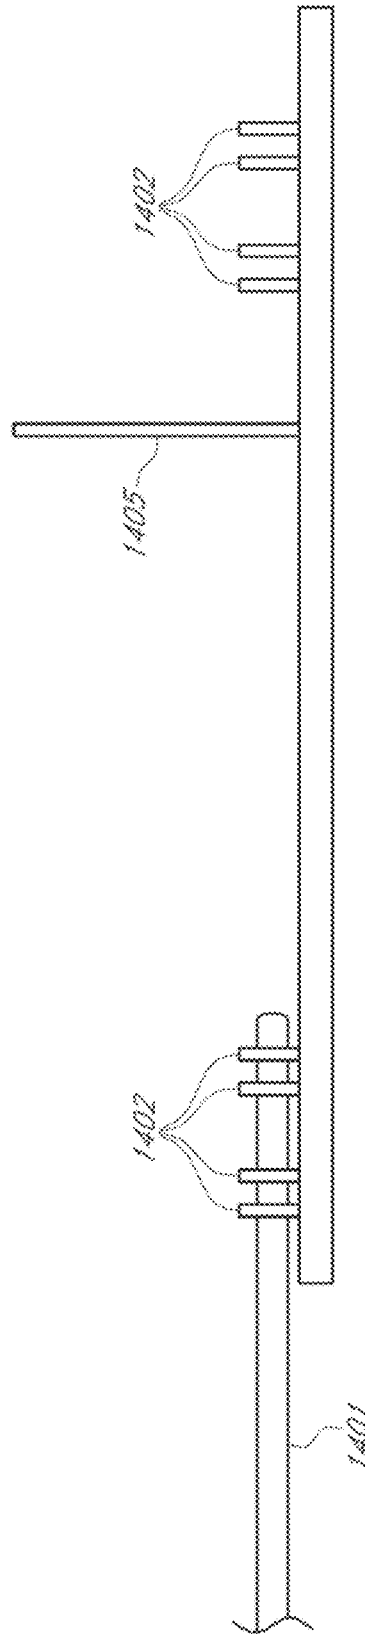


FIG. 40B

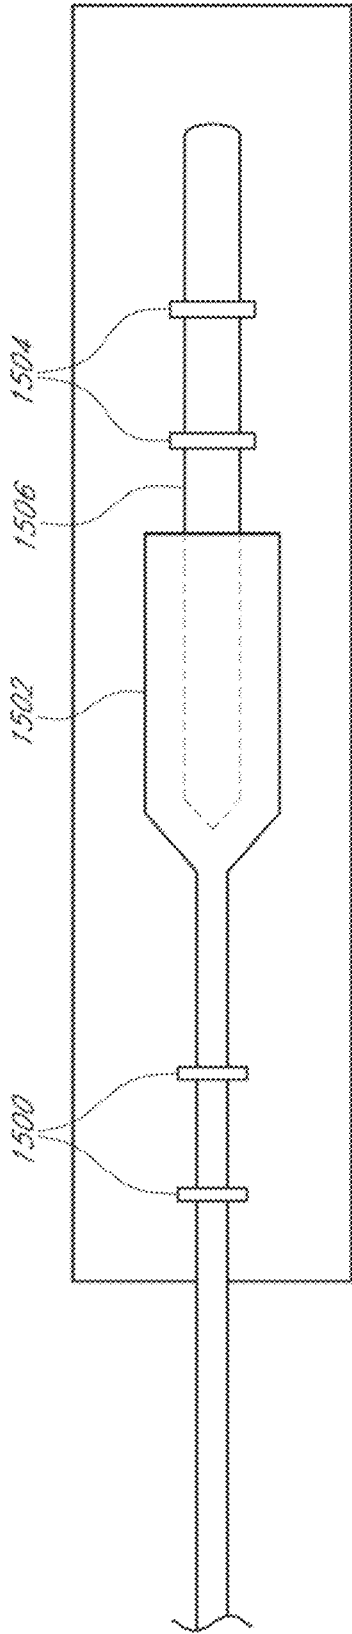


FIG. 41A

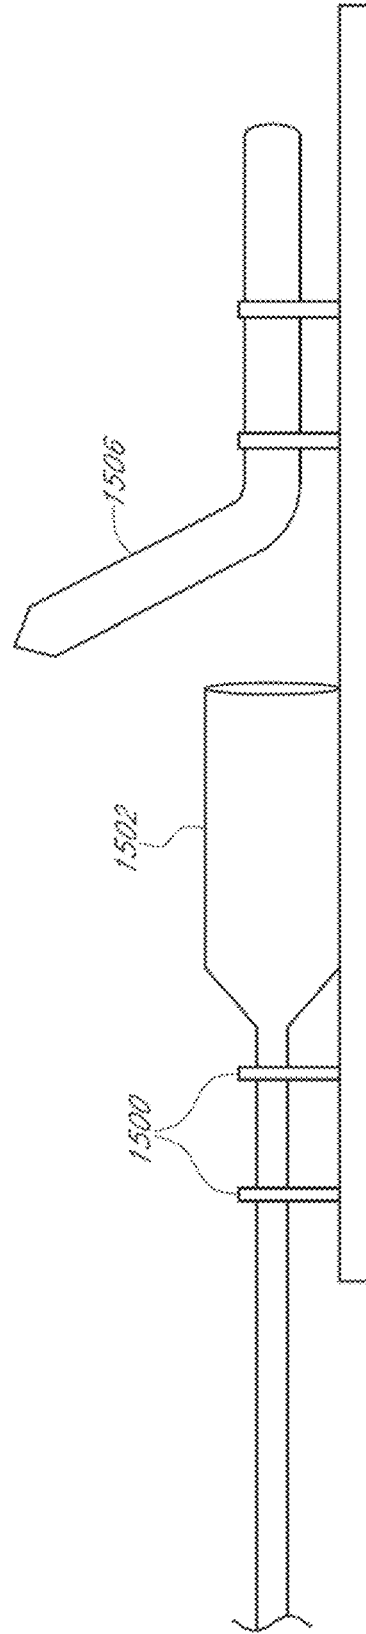


FIG. 41B

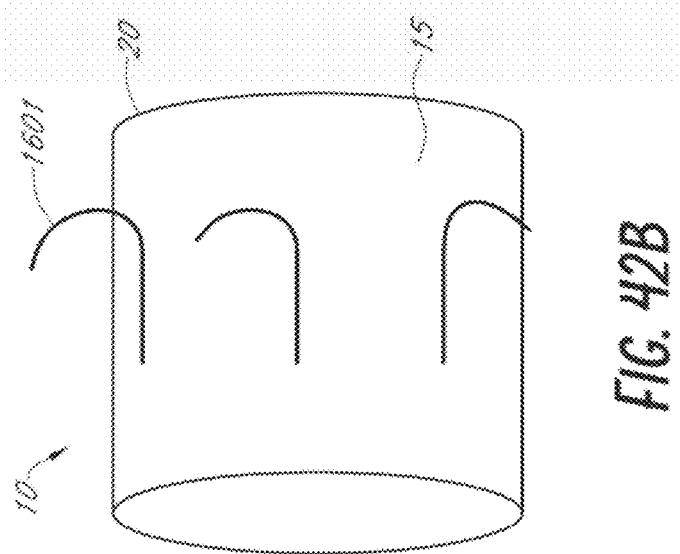


FIG. 42B

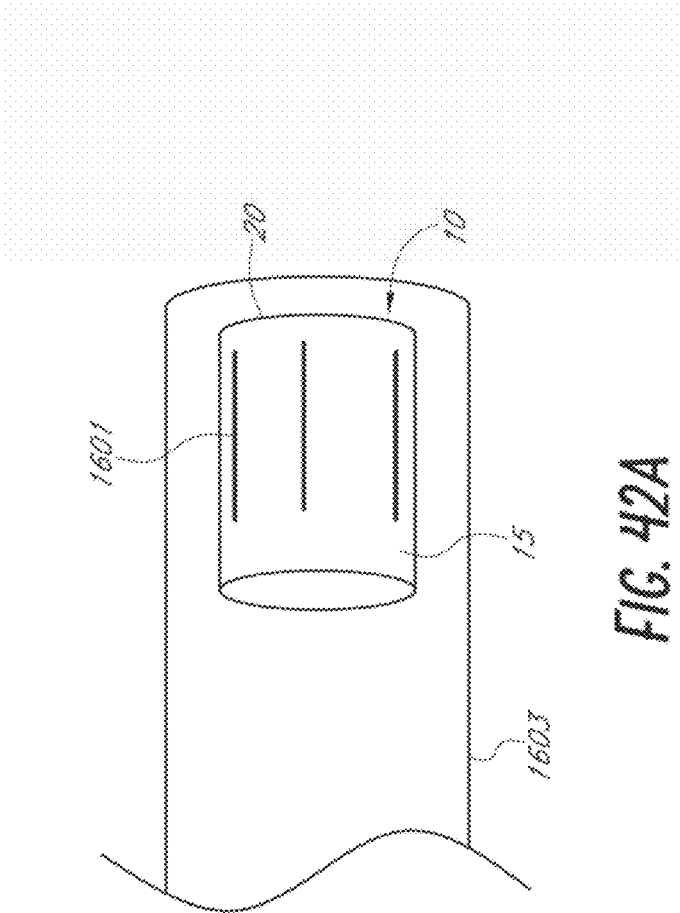


FIG. 42A

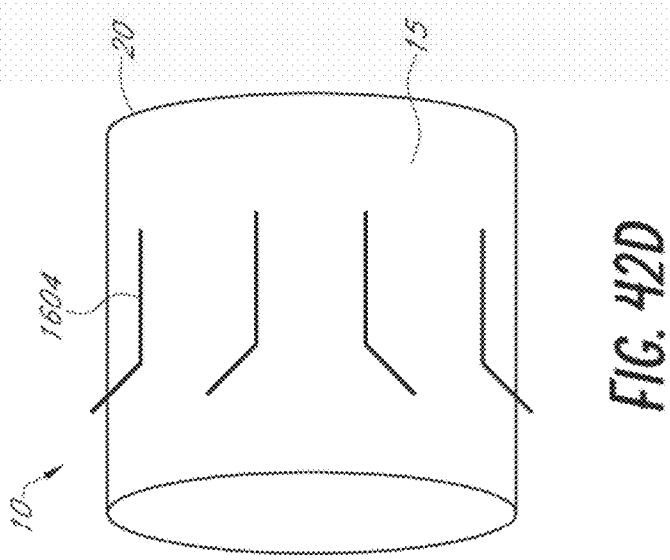


FIG. 42D

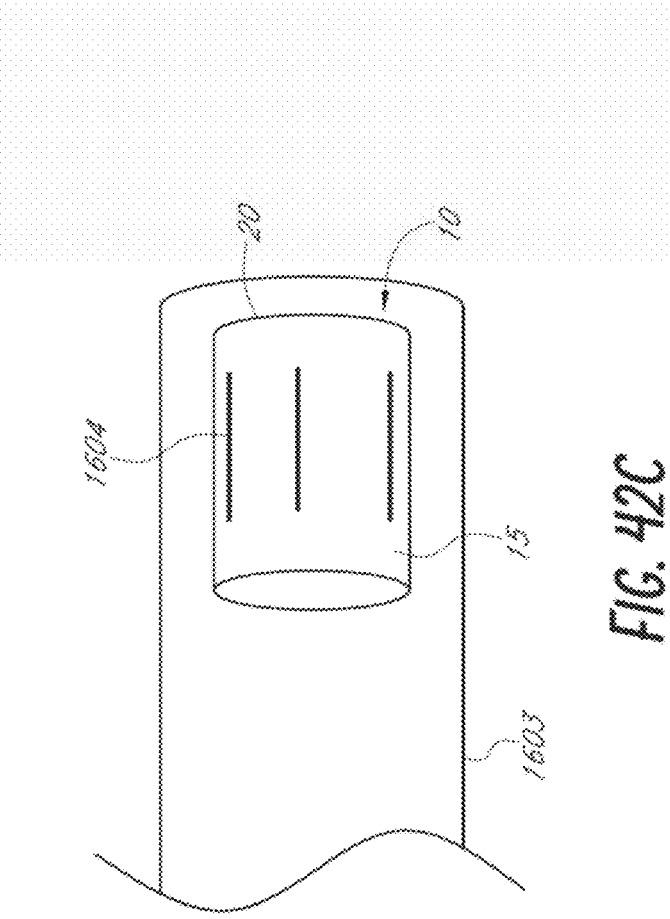


FIG. 42C

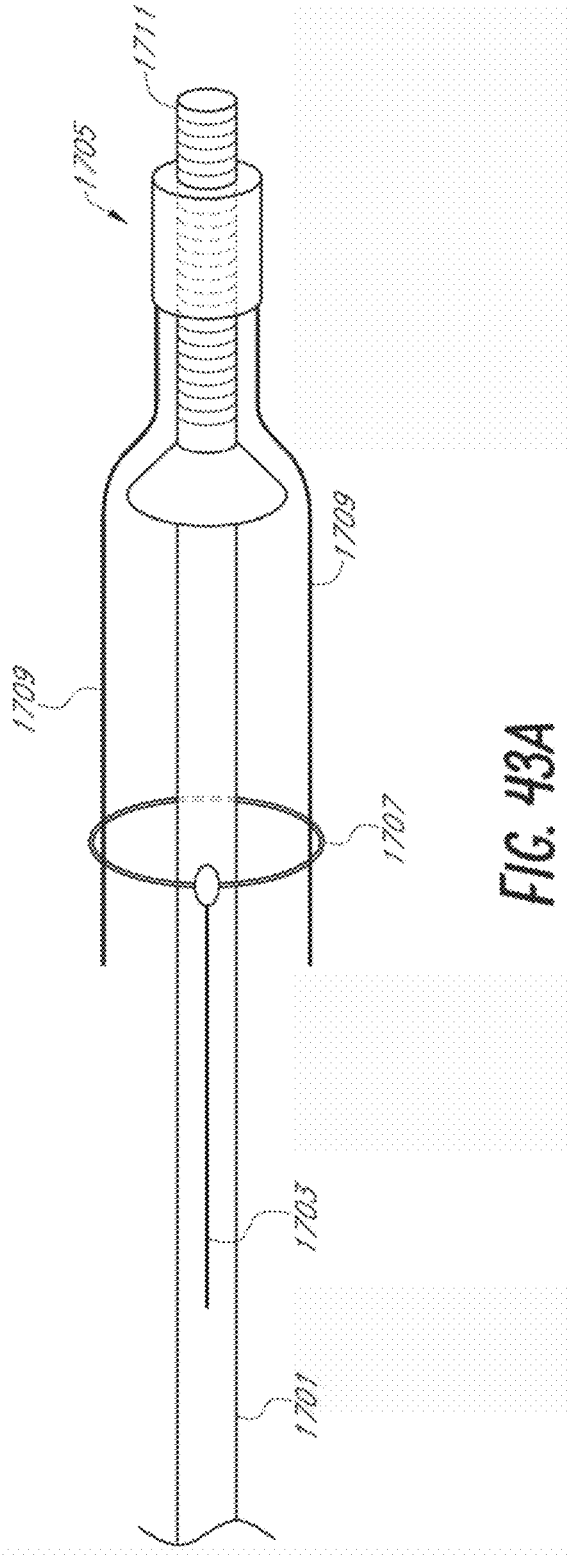
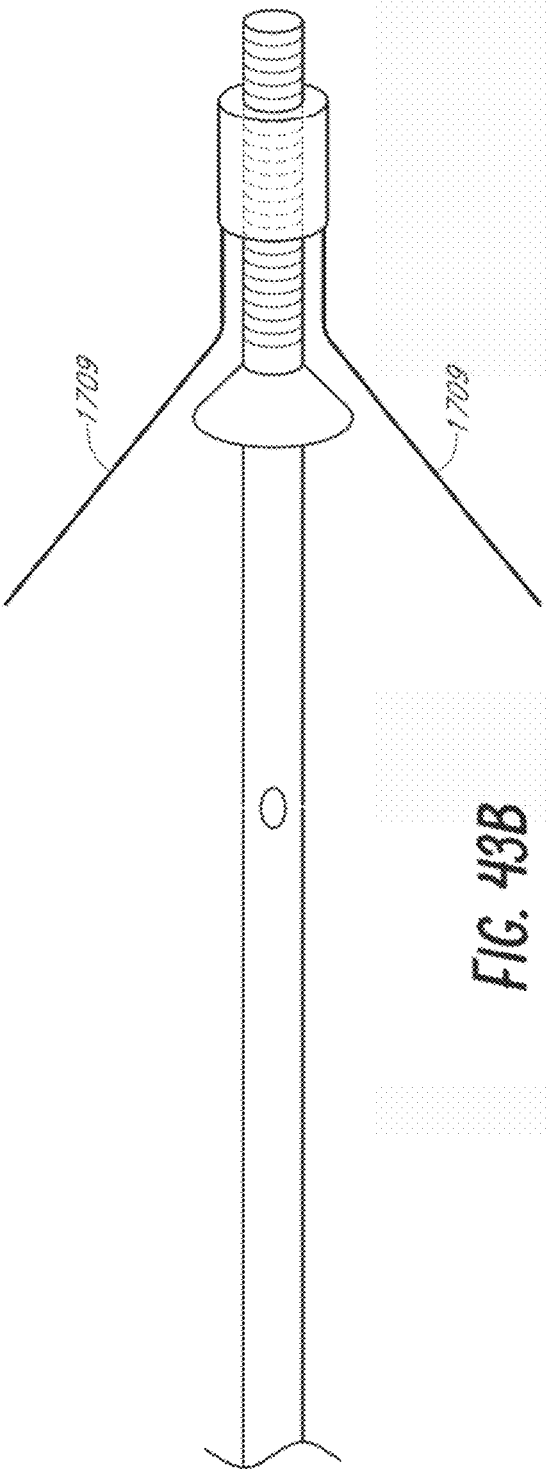


FIG. 43A



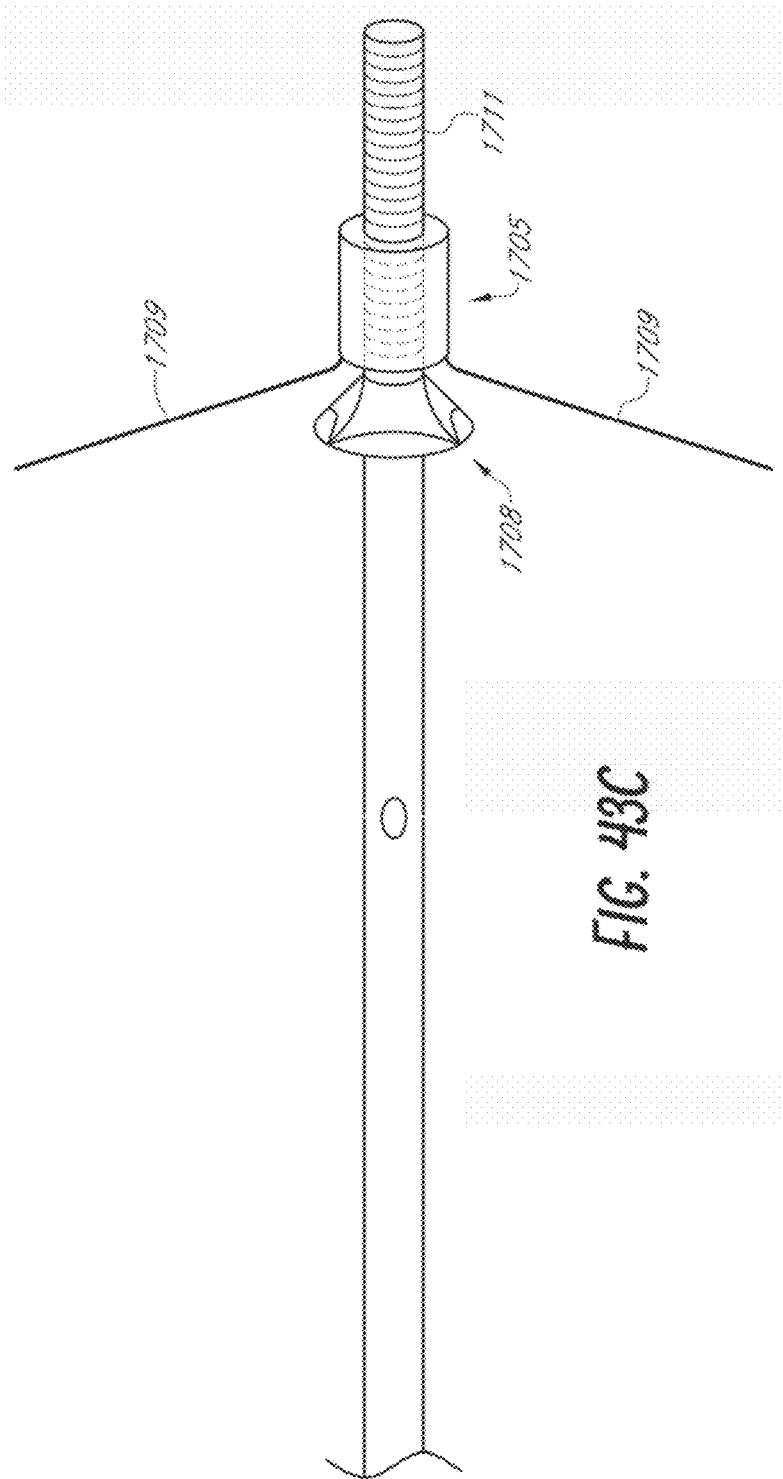


FIG. 43C

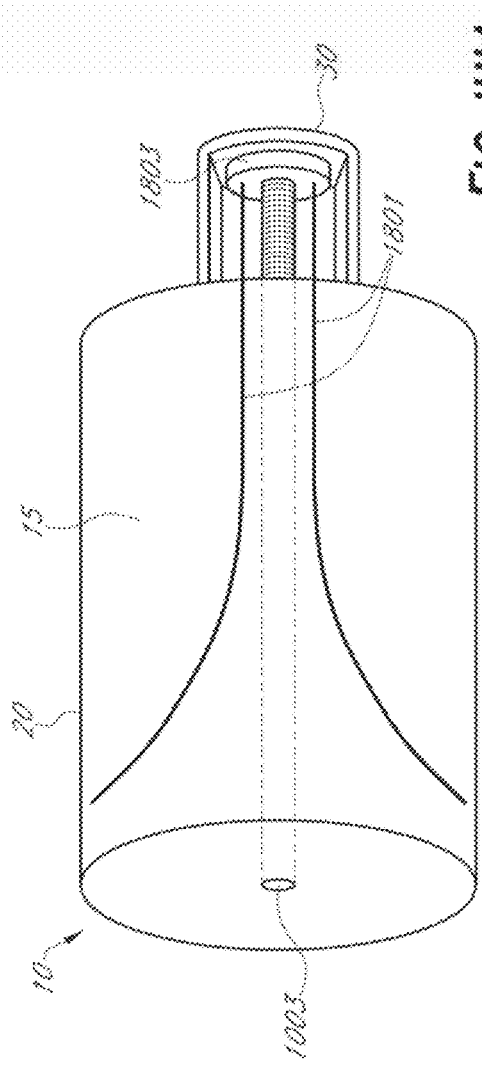


FIG. 44A

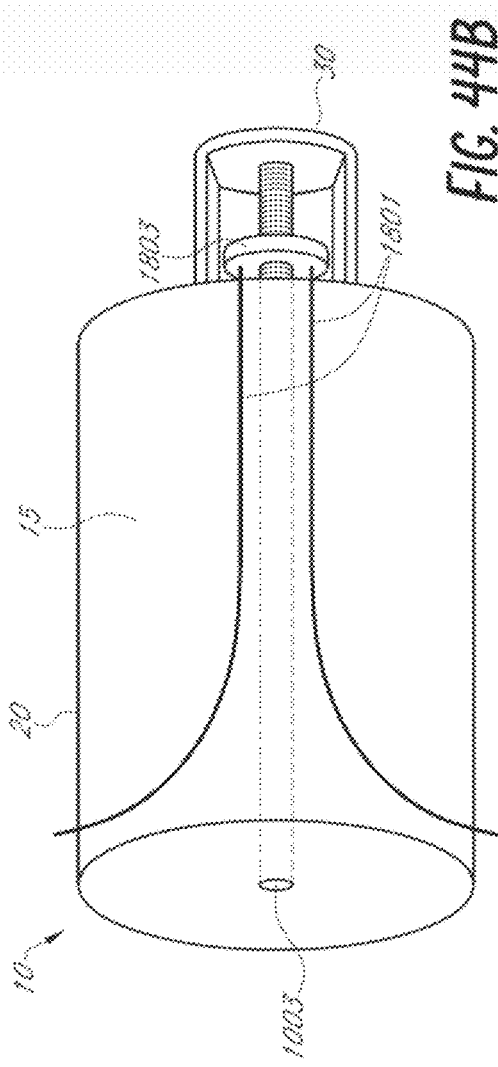


FIG. 44B

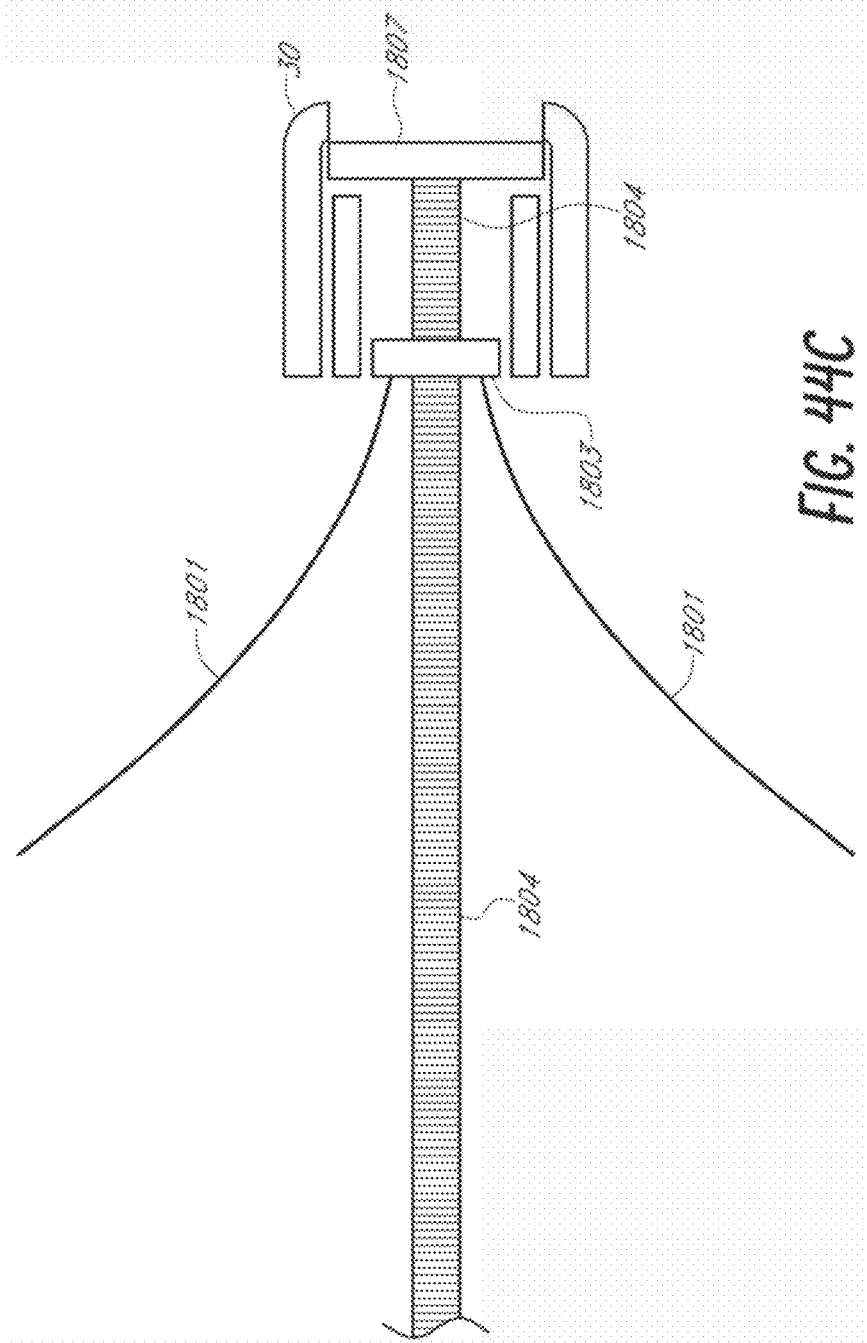


FIG. 44C

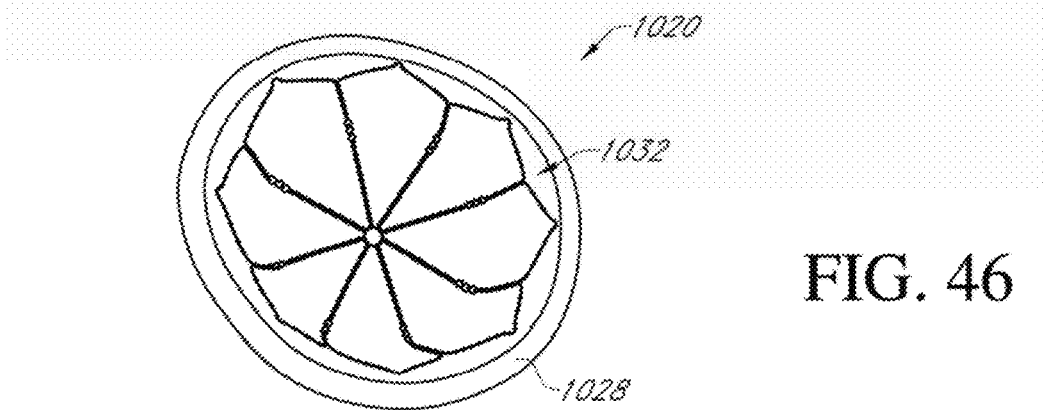


FIG. 46

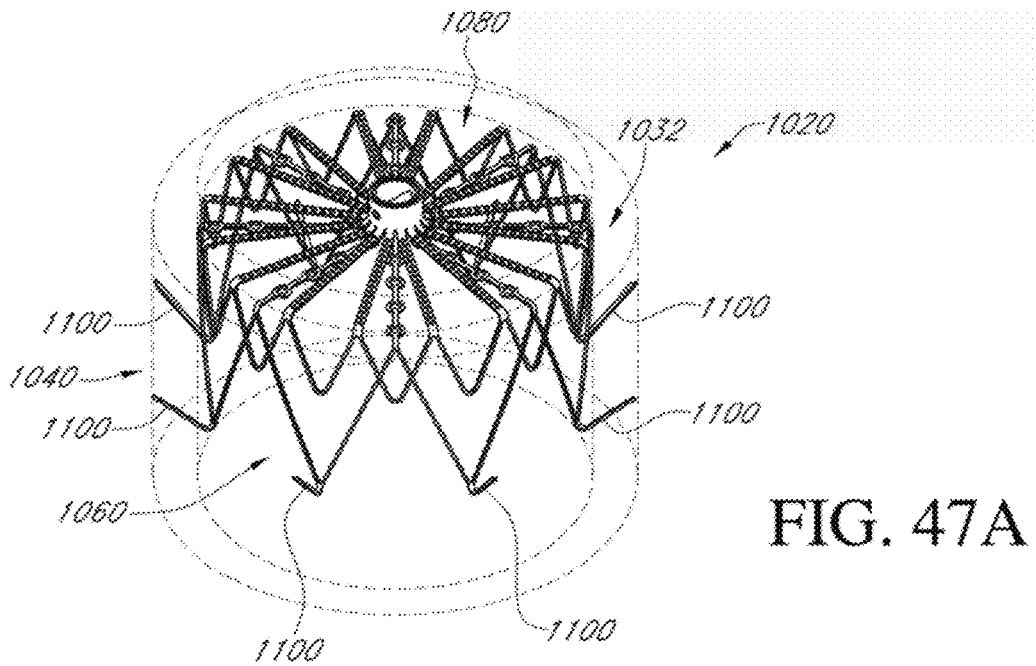


FIG. 47A

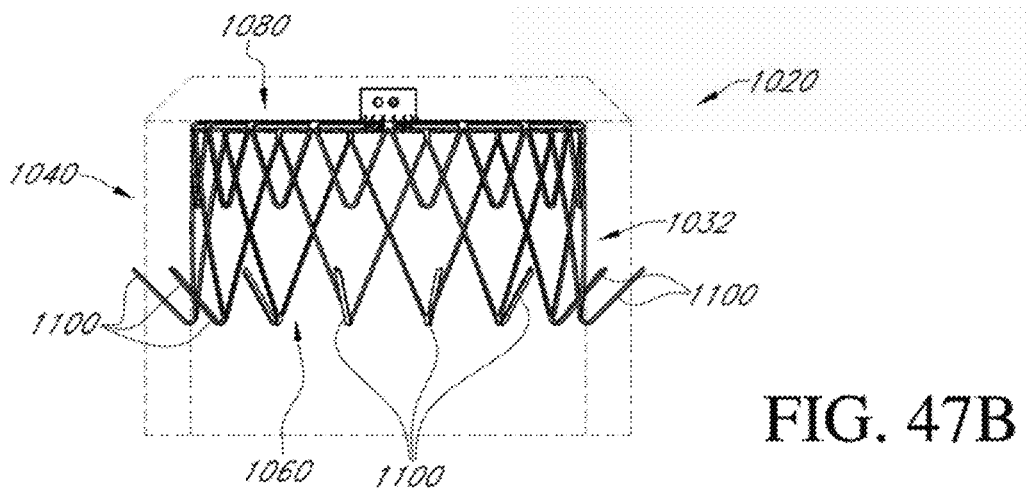


FIG. 47B

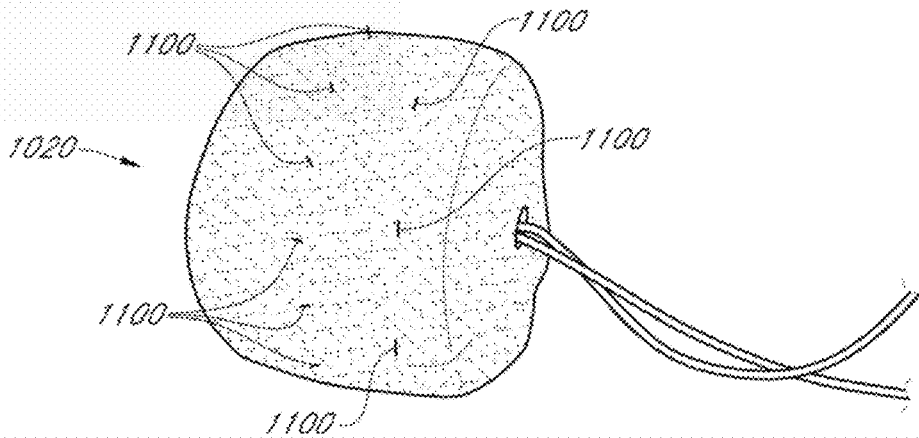


FIG. 48

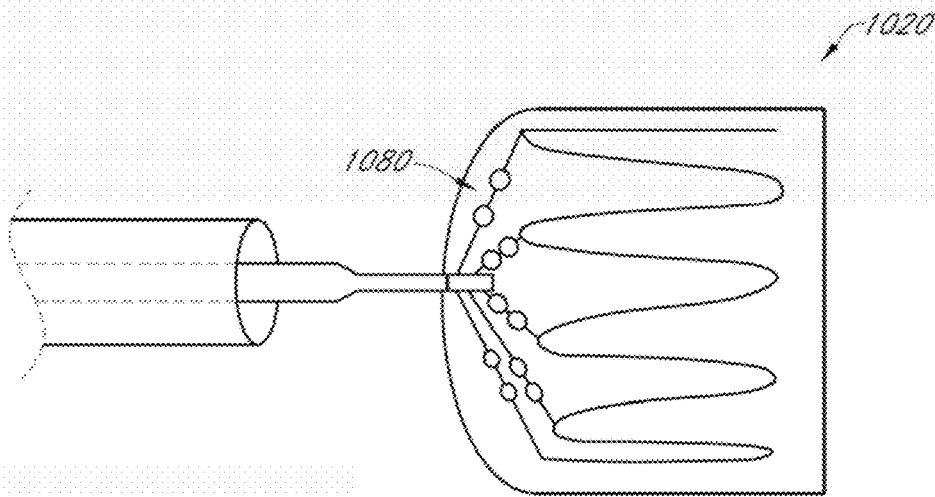


FIG. 49

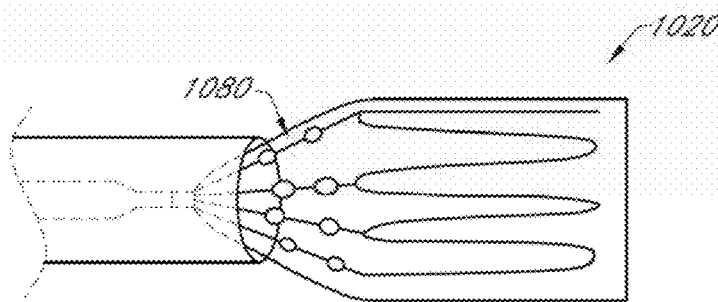


FIG. 50

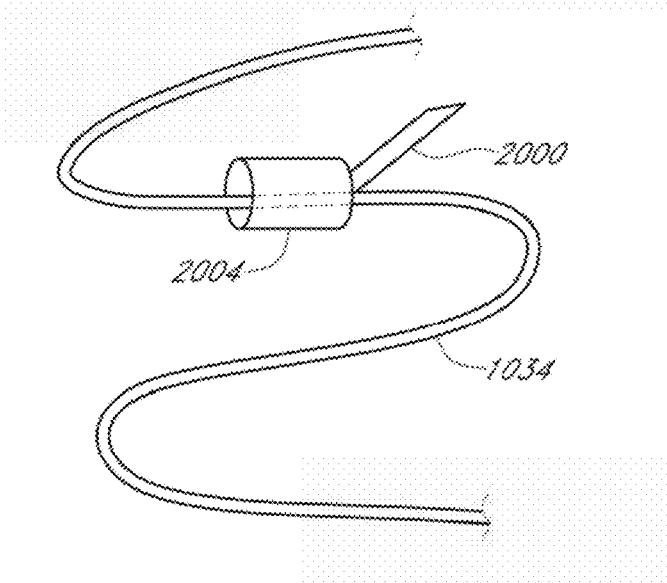


FIG. 51

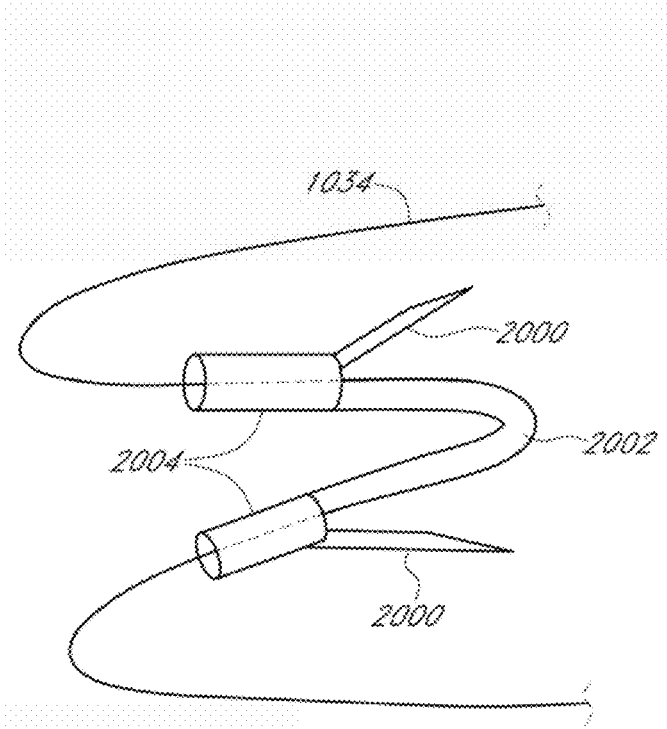


FIG. 52

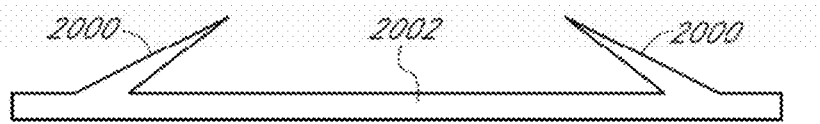


FIG. 53

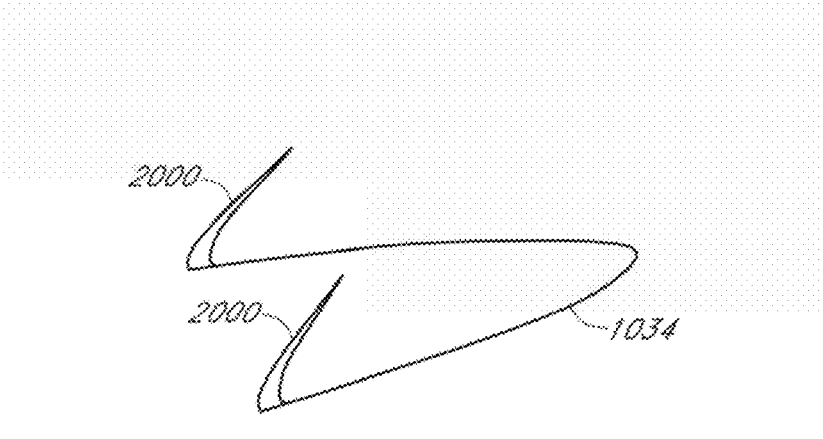


FIG. 54

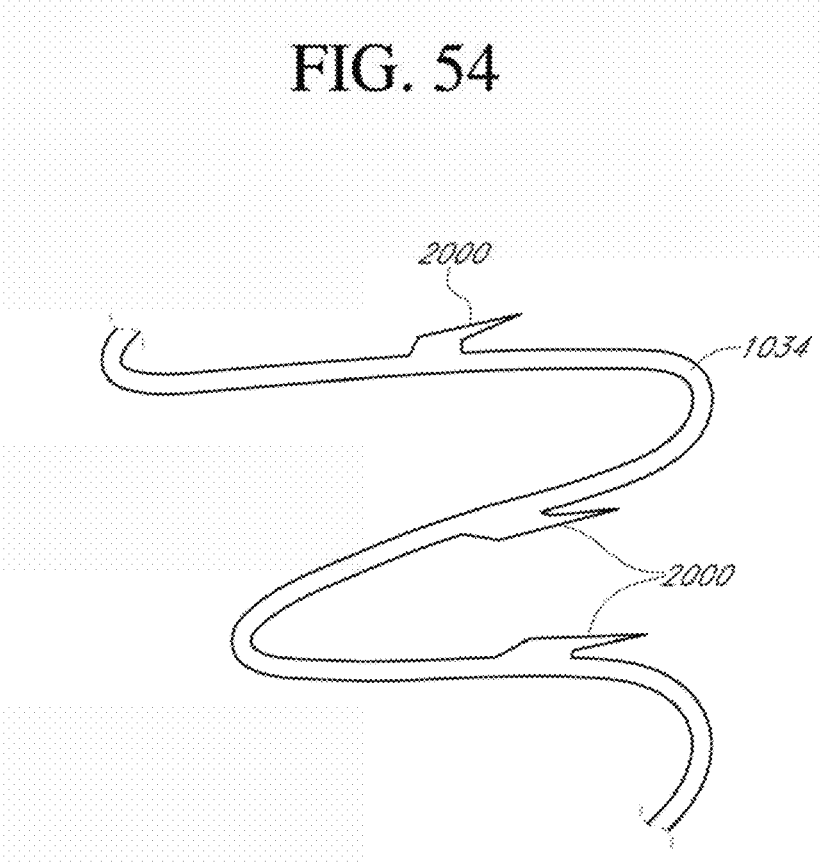


FIG. 55

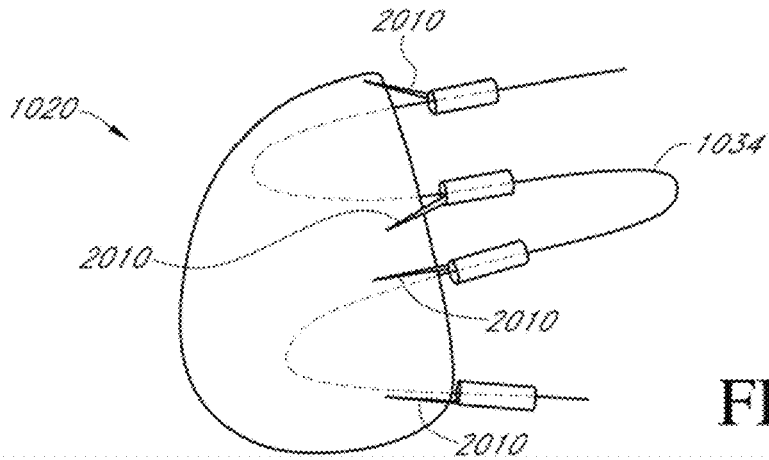


FIG. 56

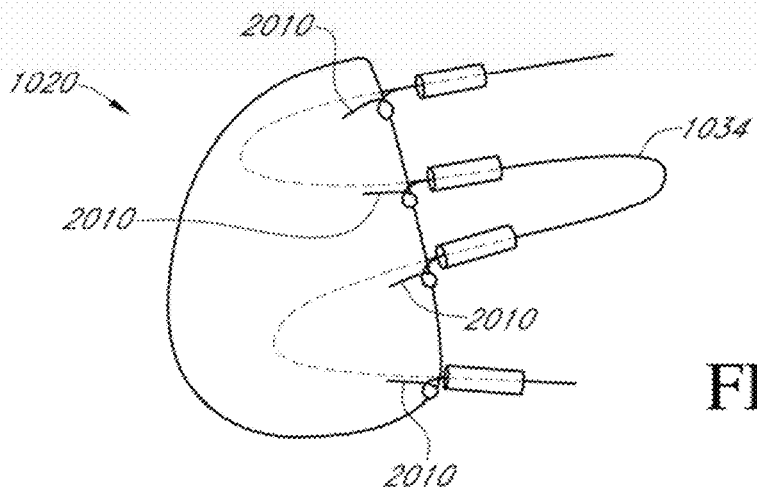


FIG. 57

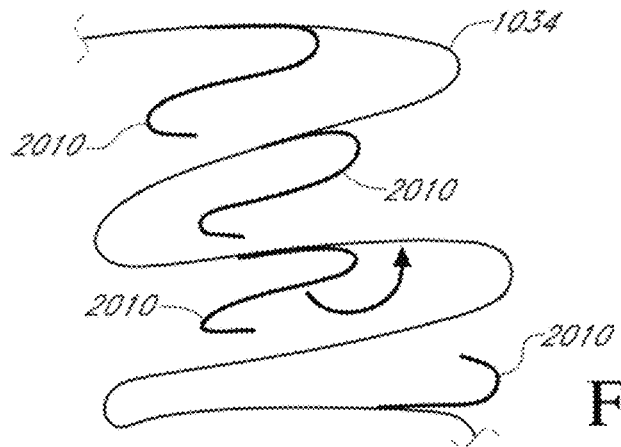


FIG. 58

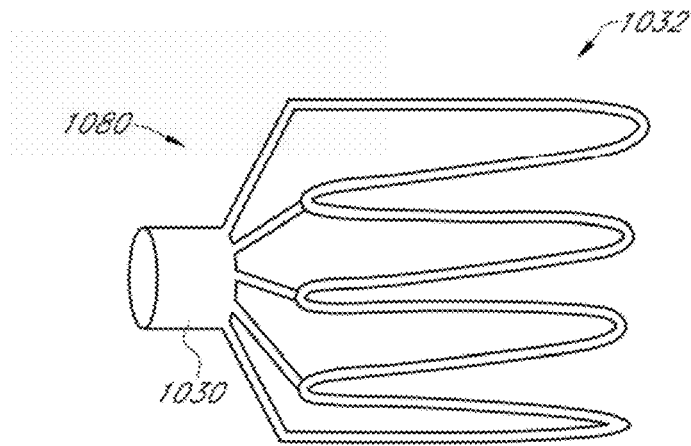


FIG. 59

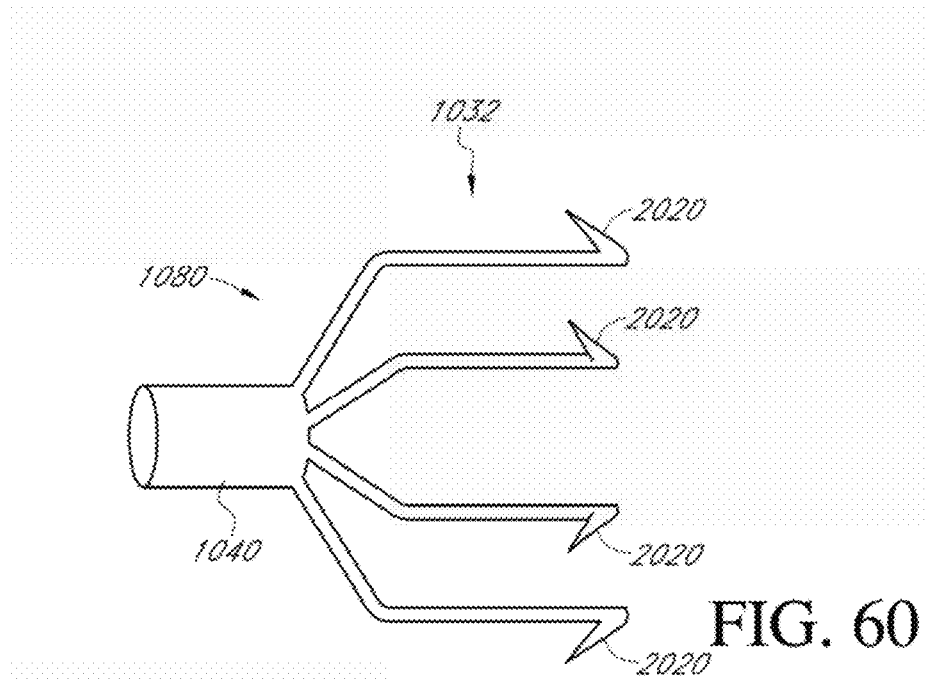


FIG. 60

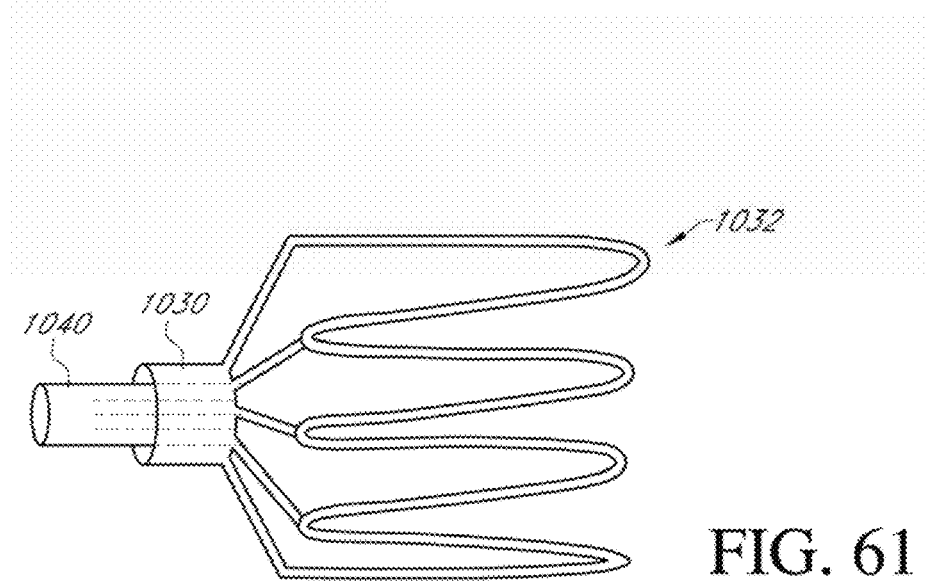


FIG. 61

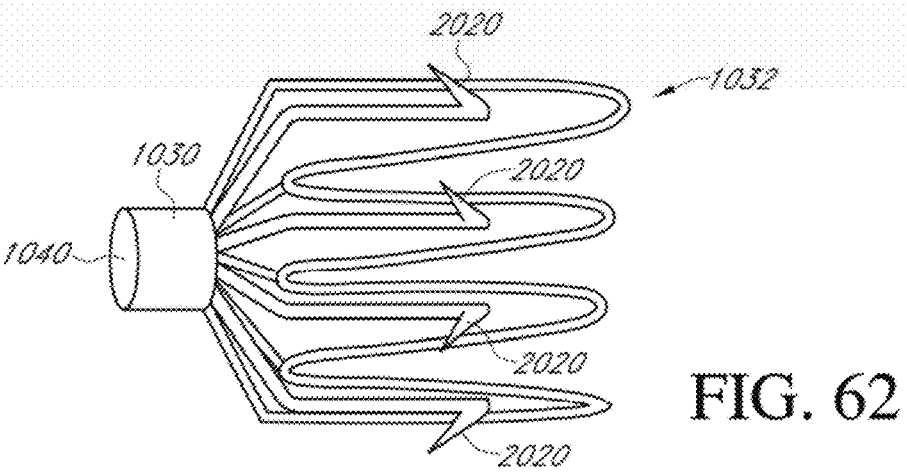


FIG. 62

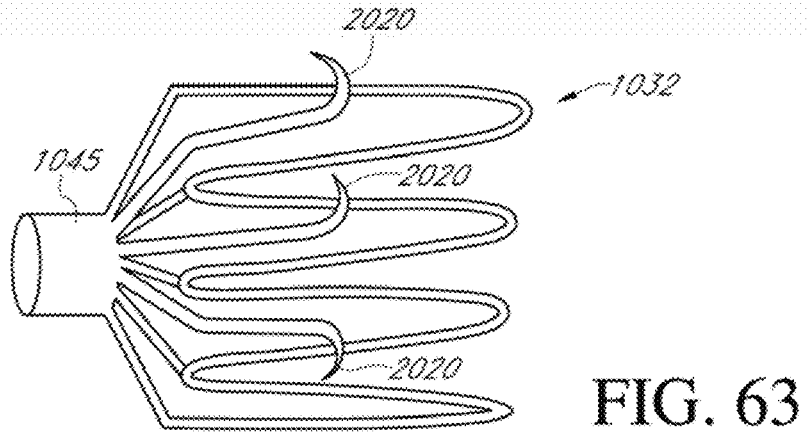


FIG. 63

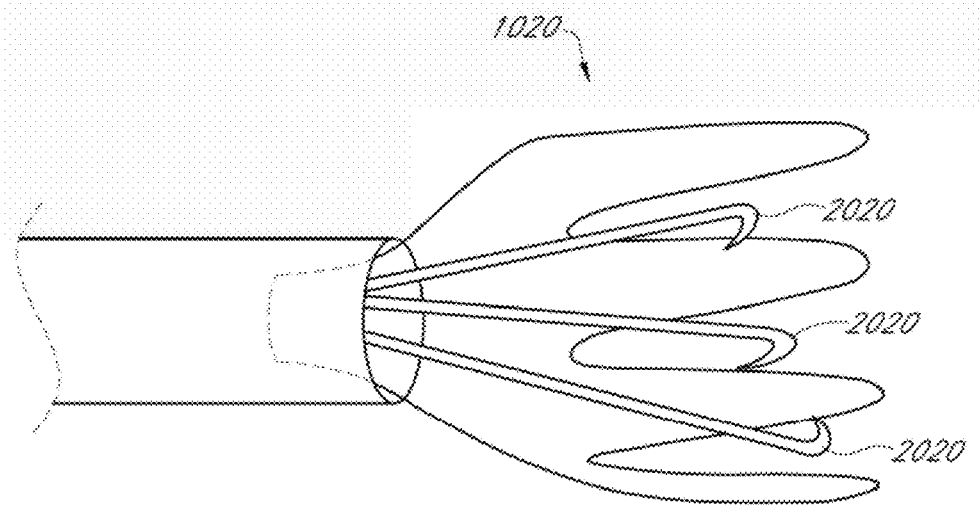


FIG. 64

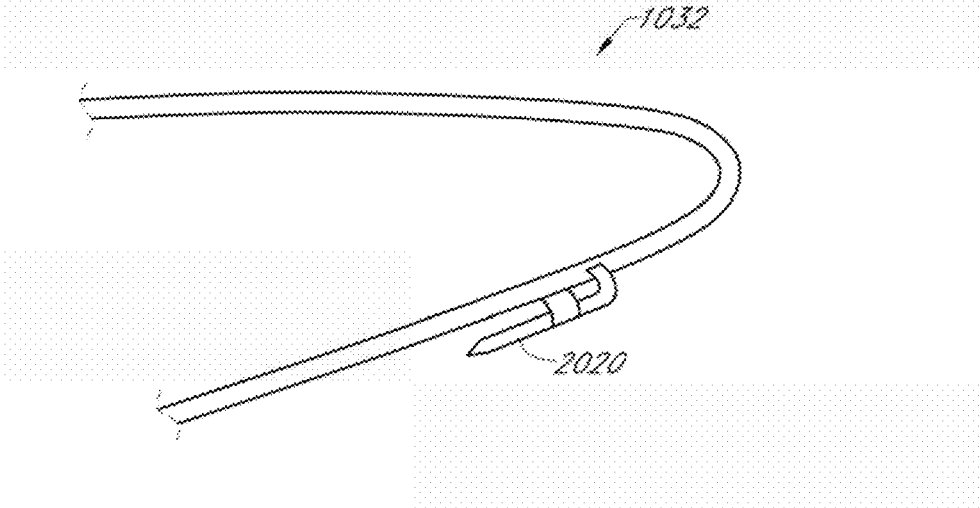


FIG. 65

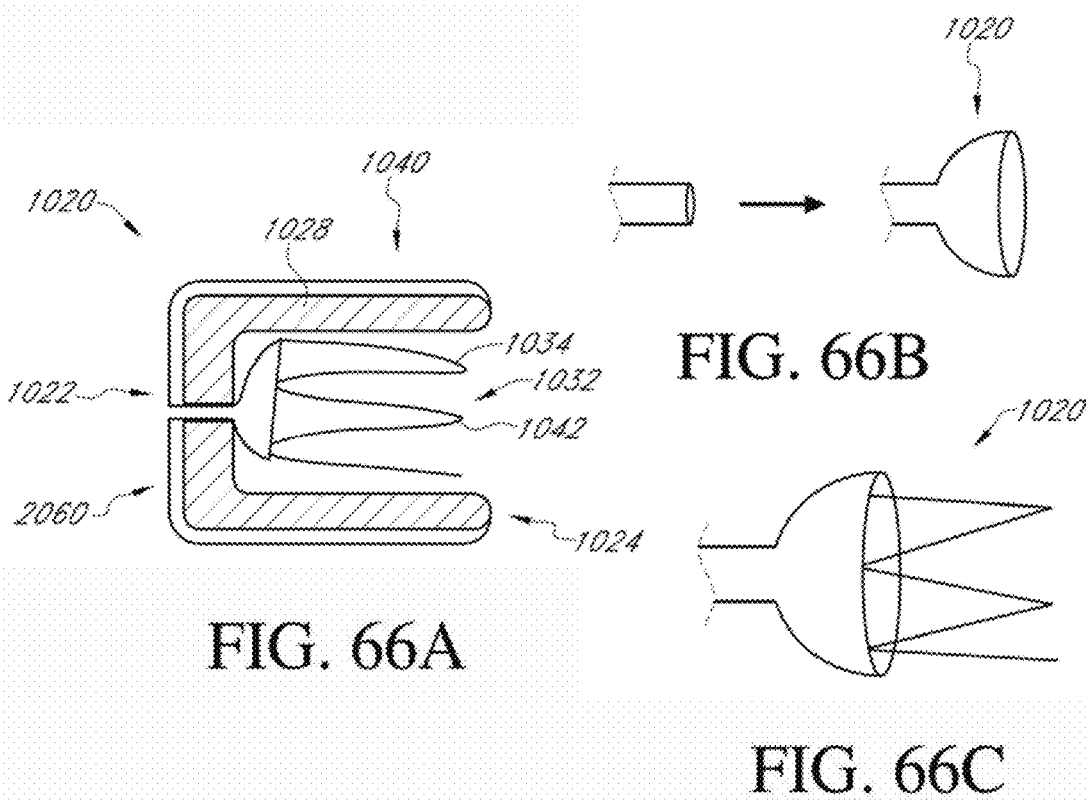


FIG. 66A

FIG. 66B

FIG. 66C

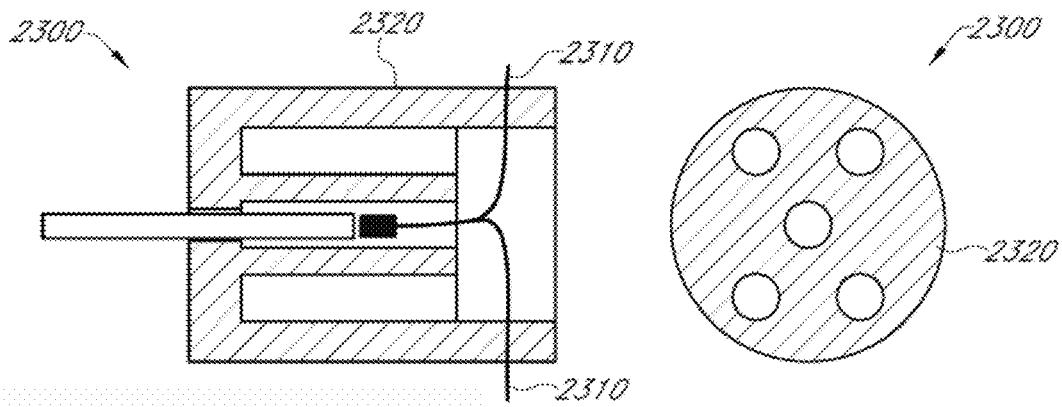


FIG. 67

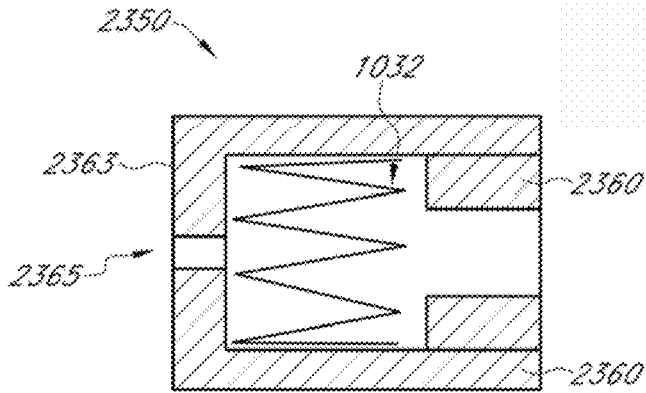


FIG. 68A

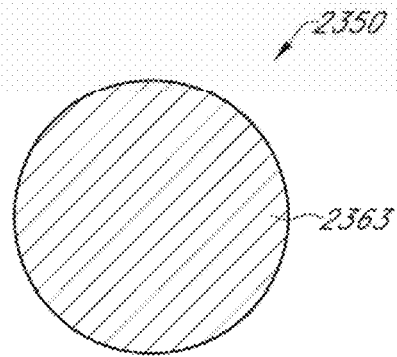


FIG. 68B

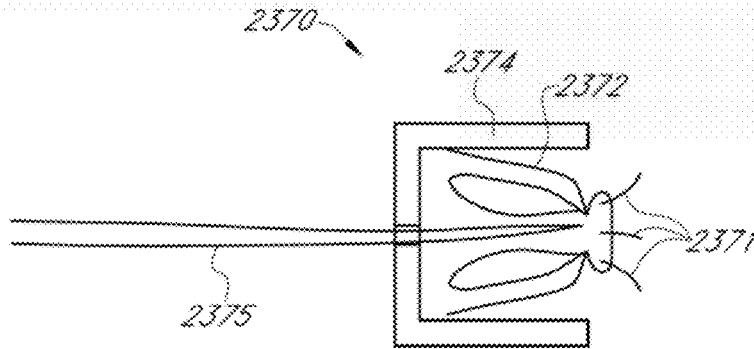


FIG. 69

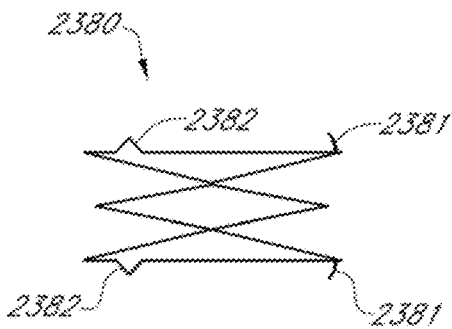


FIG. 70

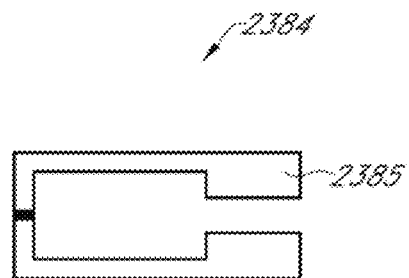


FIG. 71

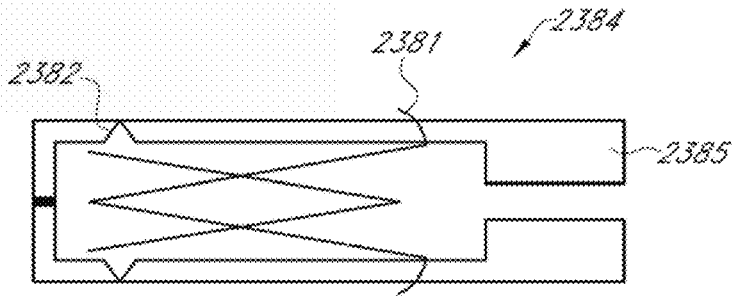


FIG. 72

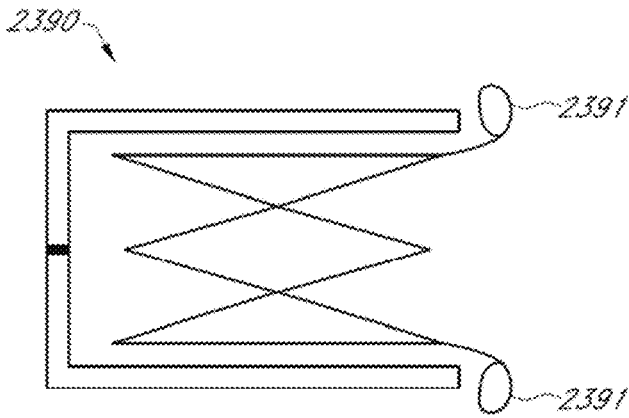


FIG. 73

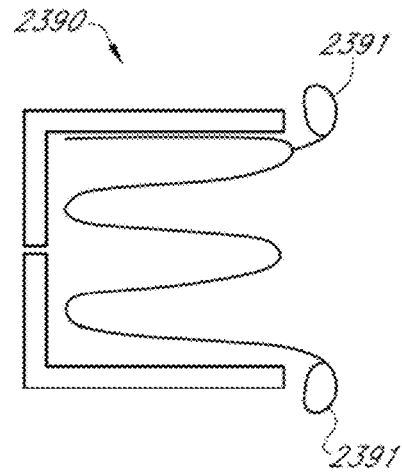


FIG. 74

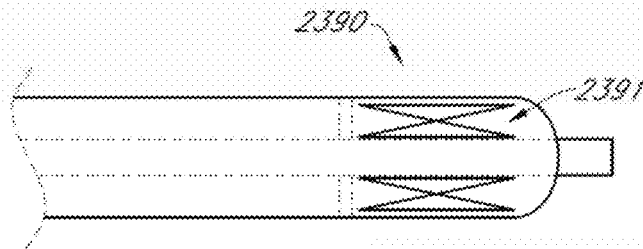


FIG. 75

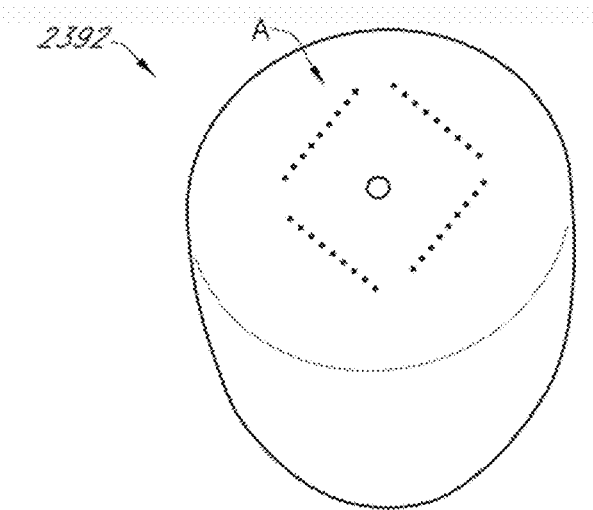


FIG. 76

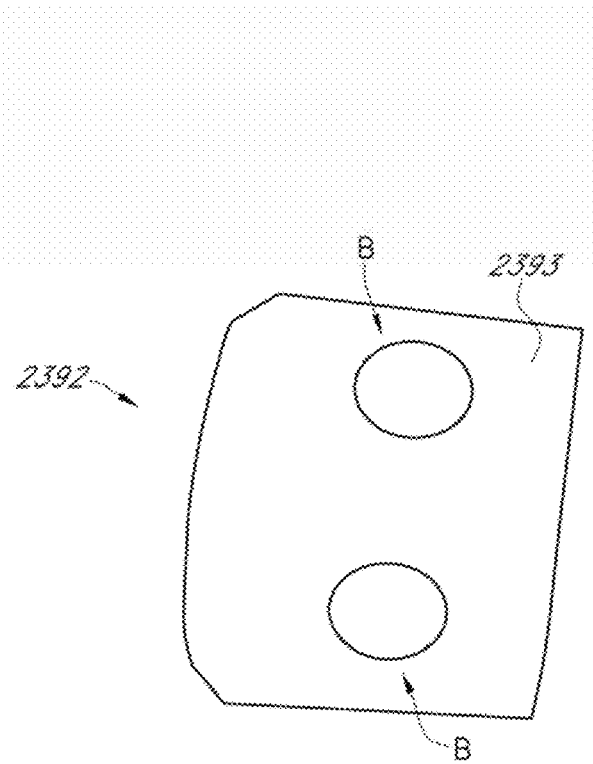


FIG. 77

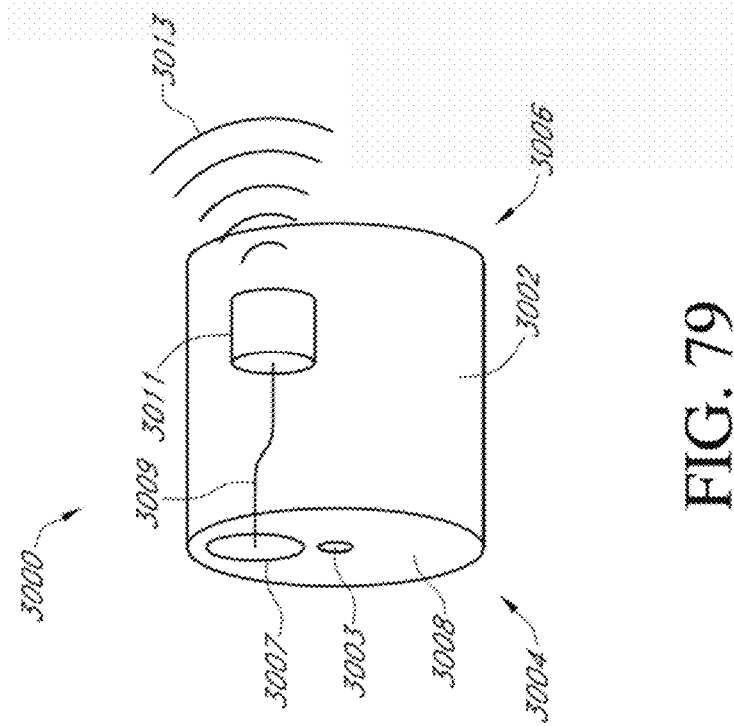


FIG. 78

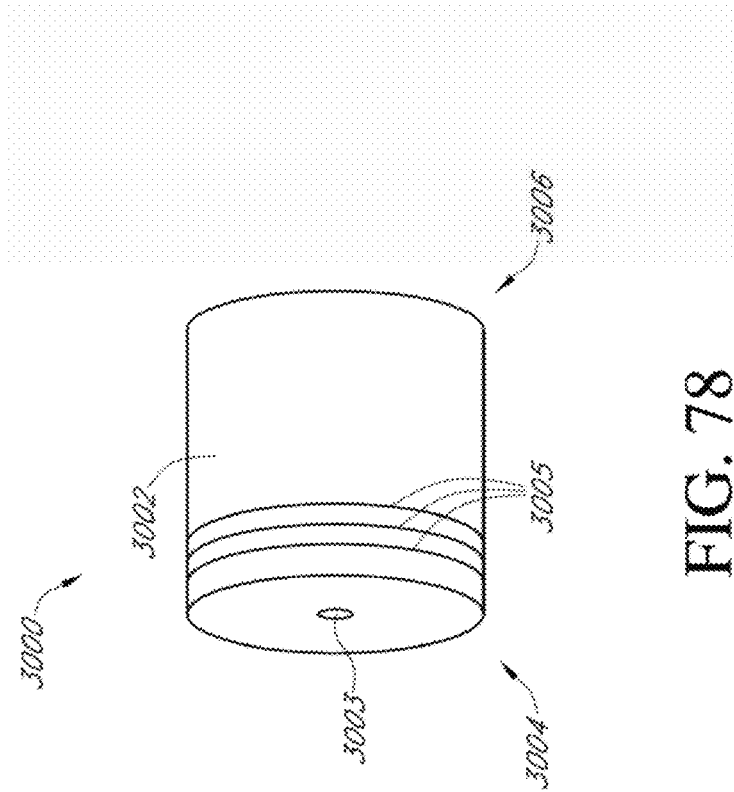


FIG. 79

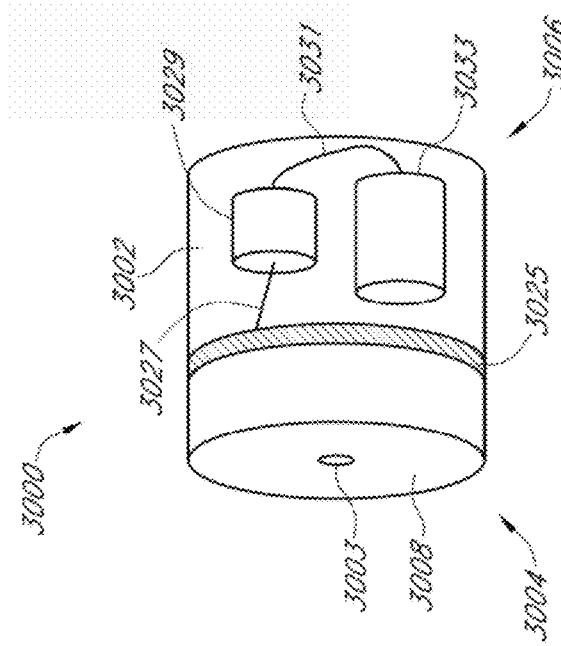


FIG. 80

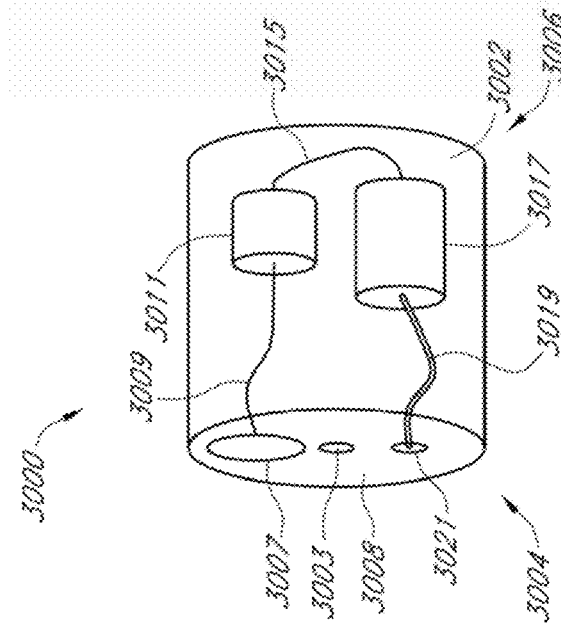


FIG. 81

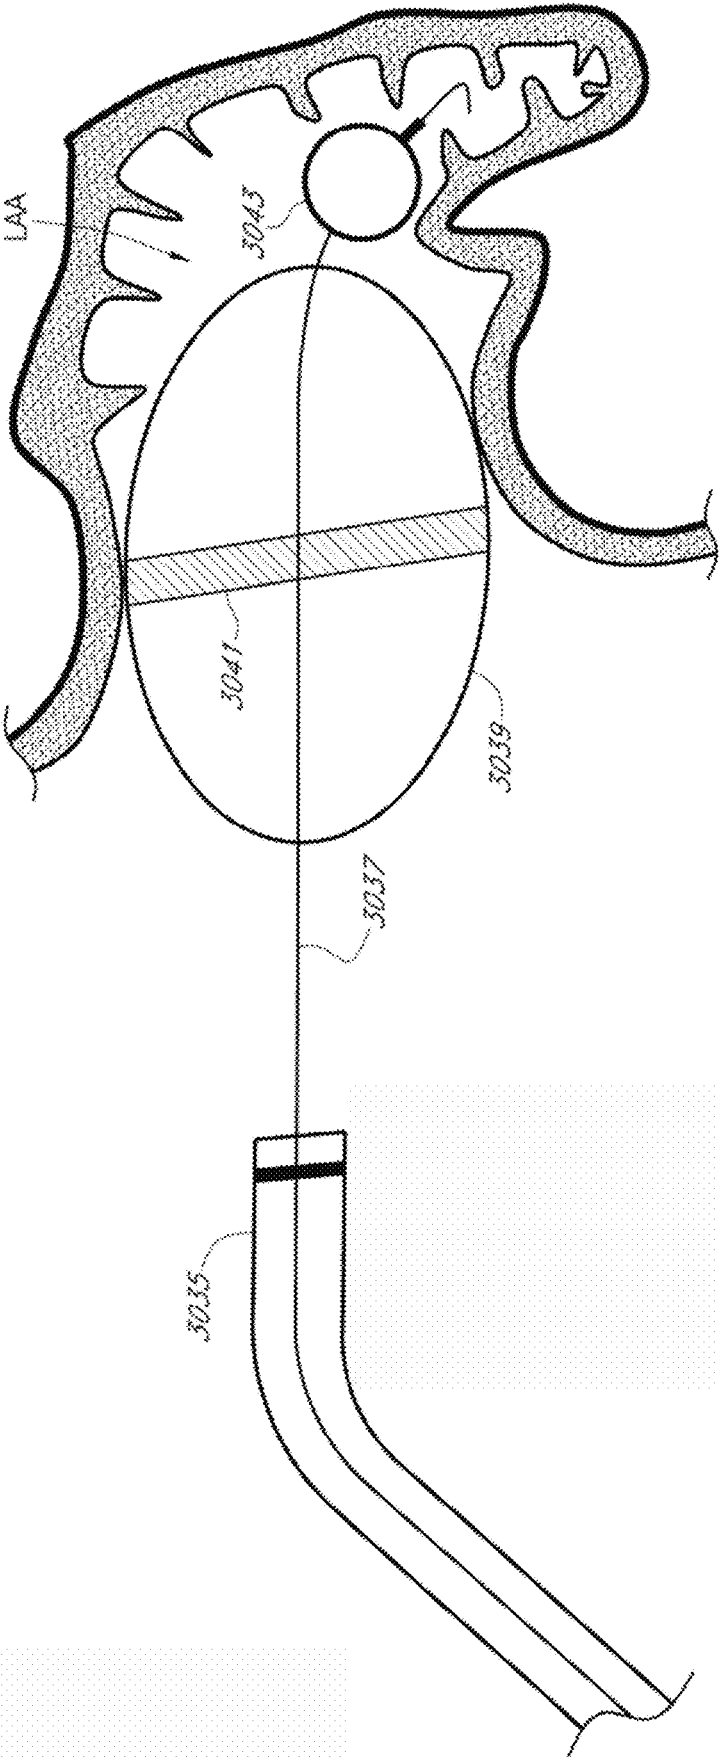


FIG. 82

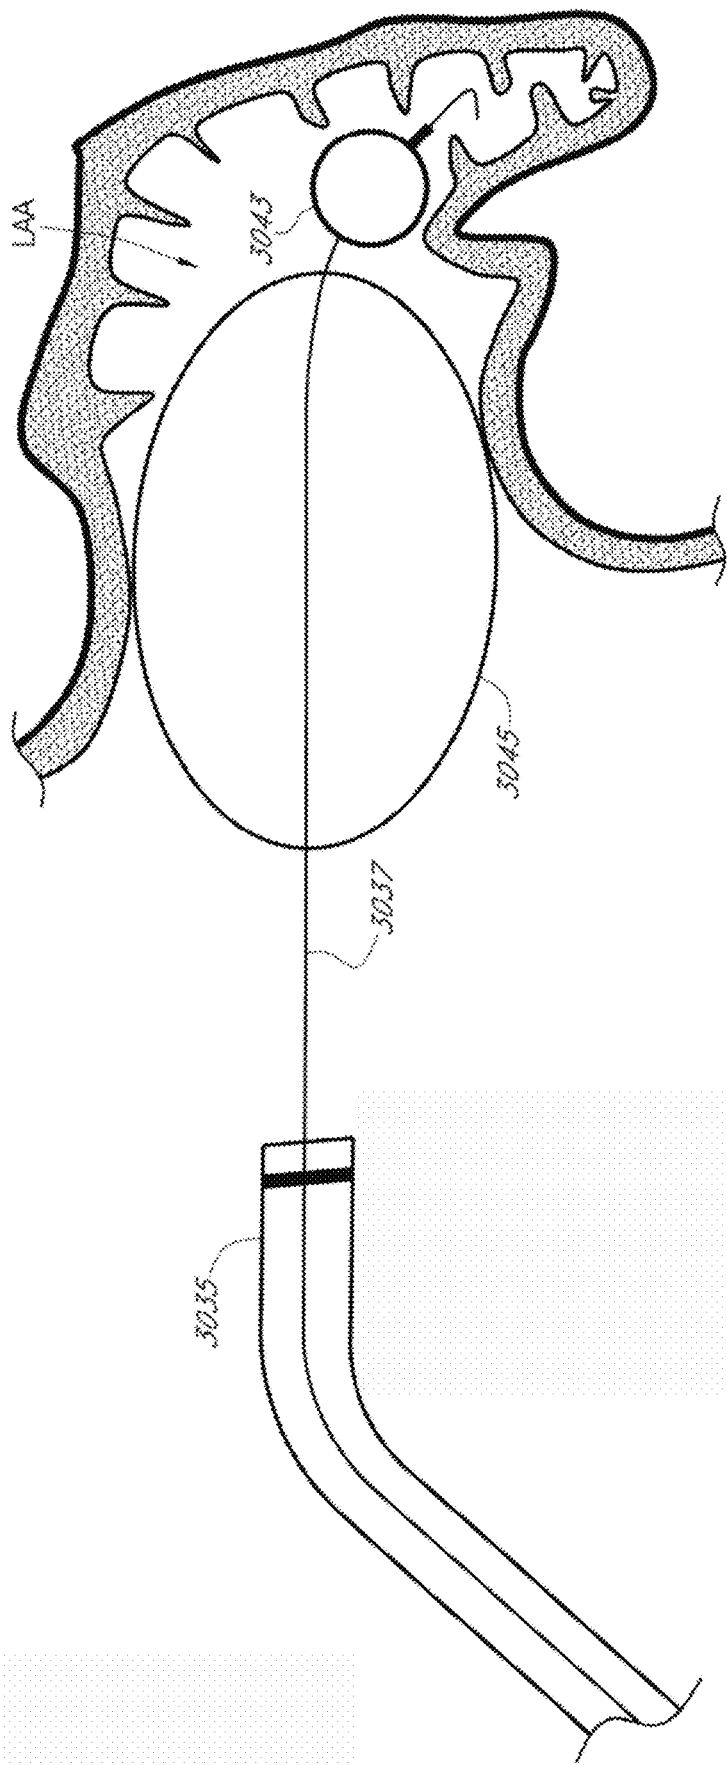


FIG. 83

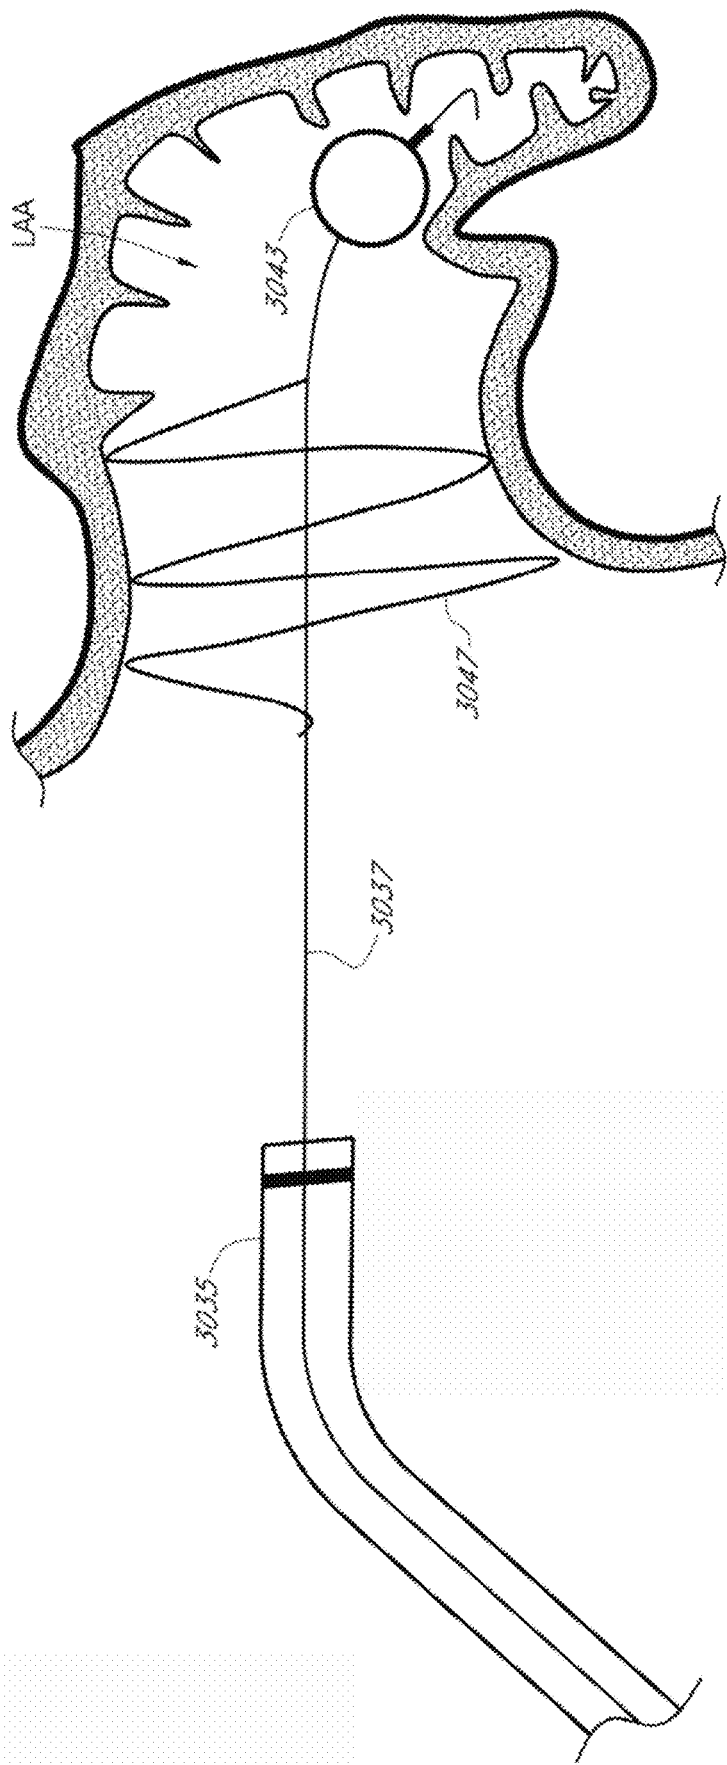


FIG. 84

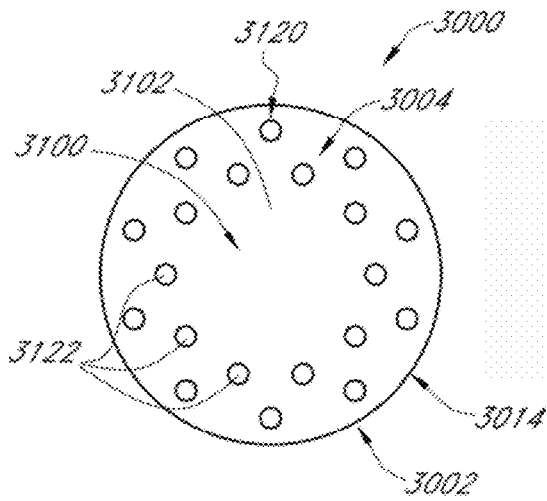


FIG. 85A

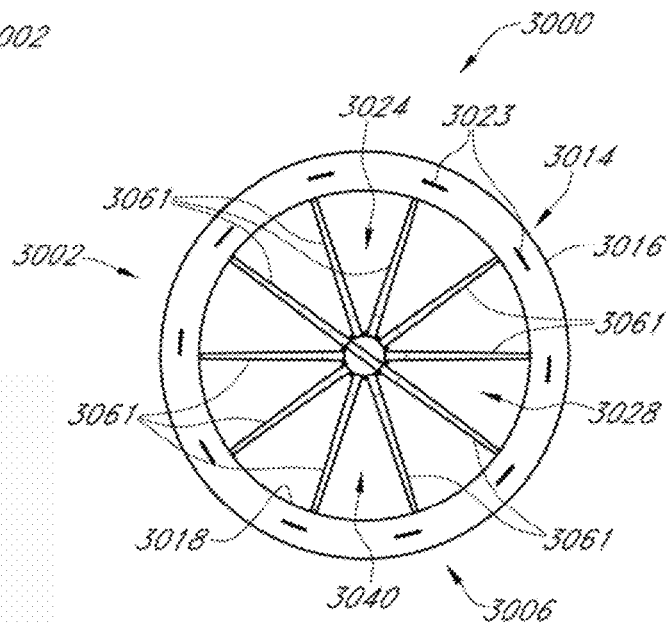


FIG. 85B

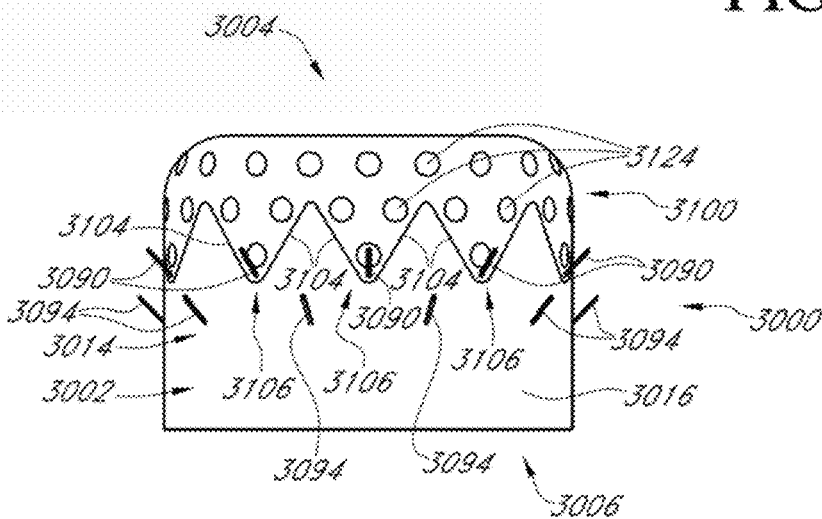


FIG. 85C

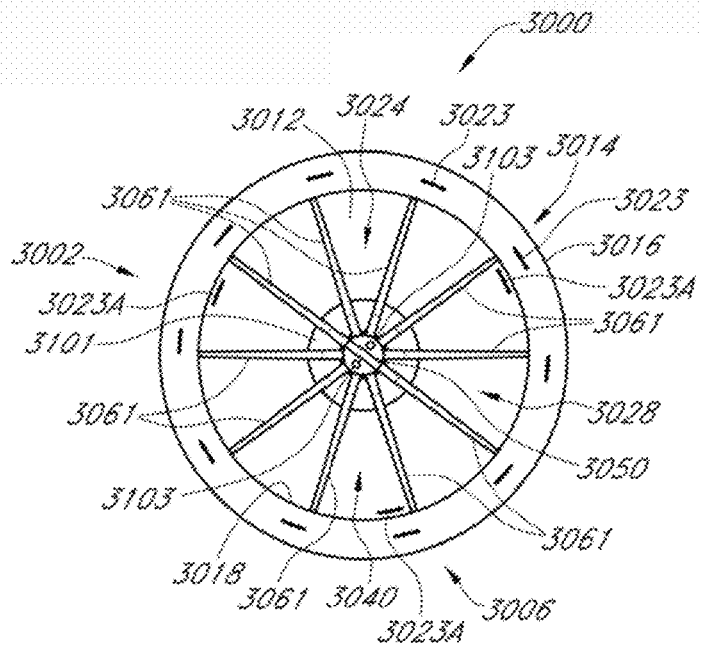


FIG. 85D

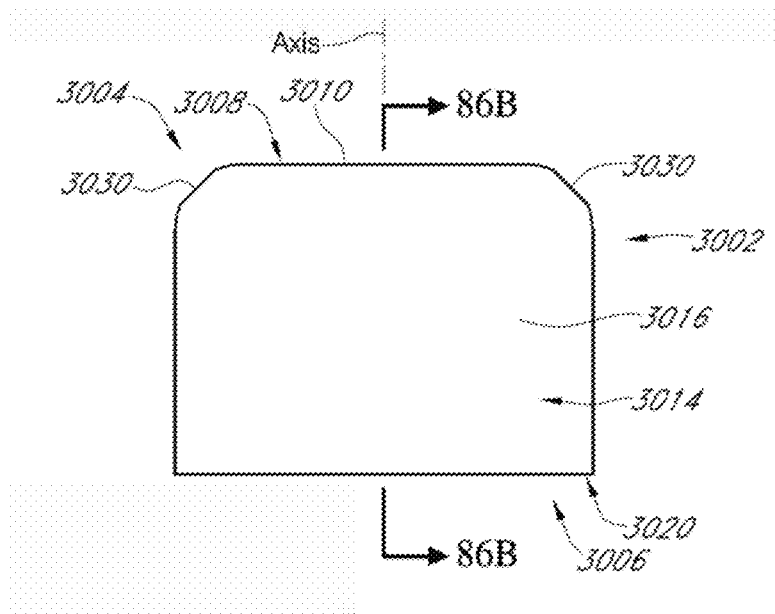


FIG. 86A

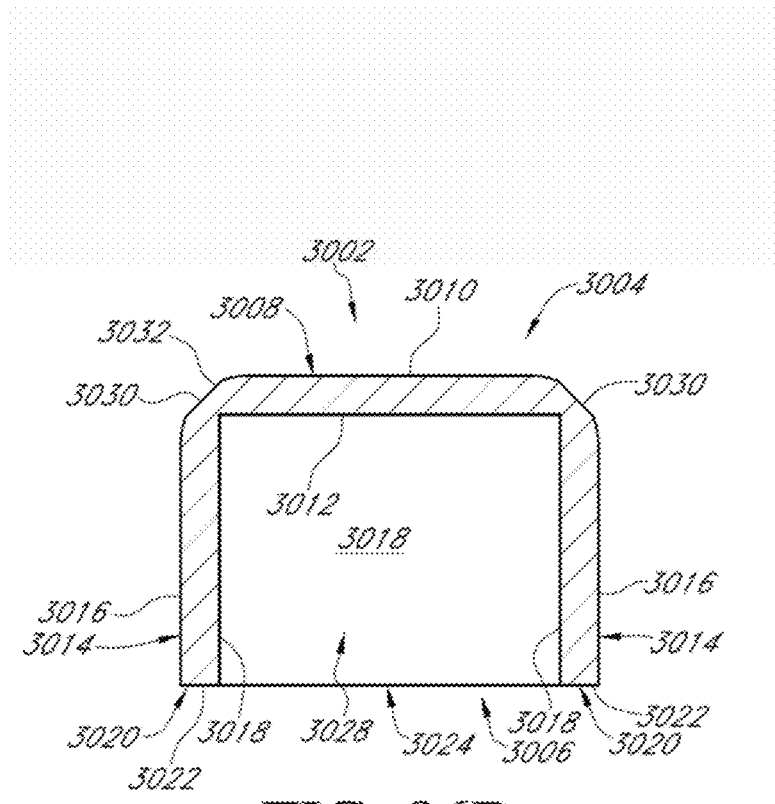


FIG. 86B

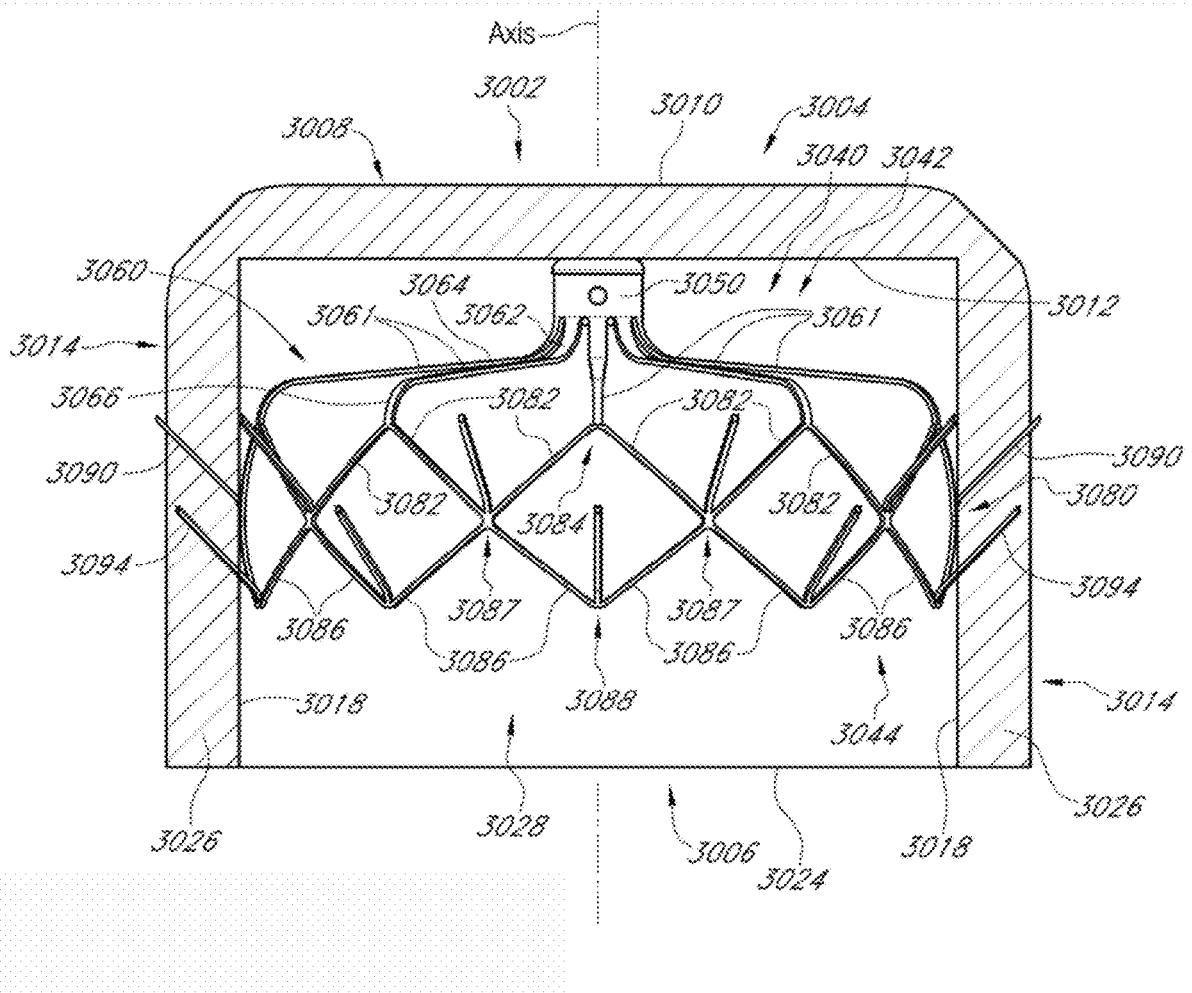


FIG. 86C

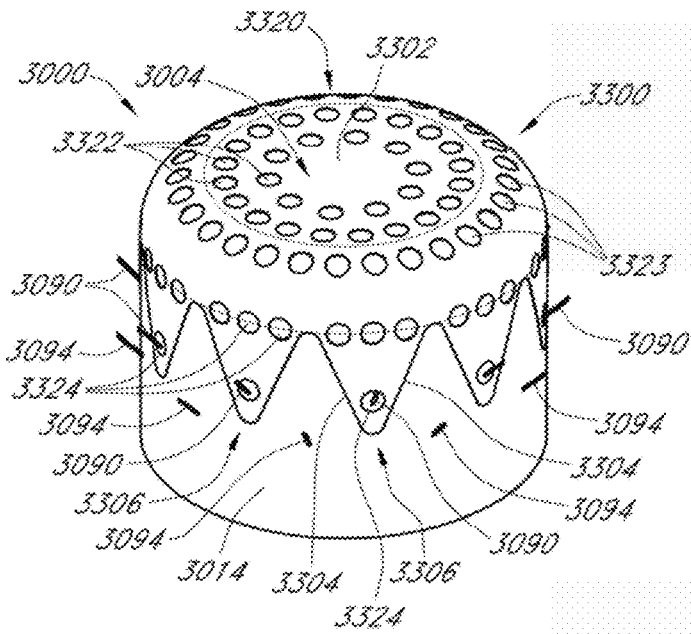


FIG. 87A

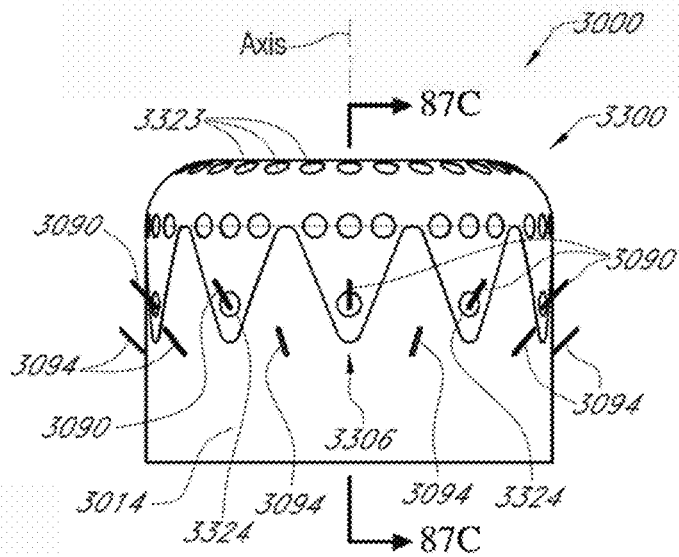


FIG. 87B

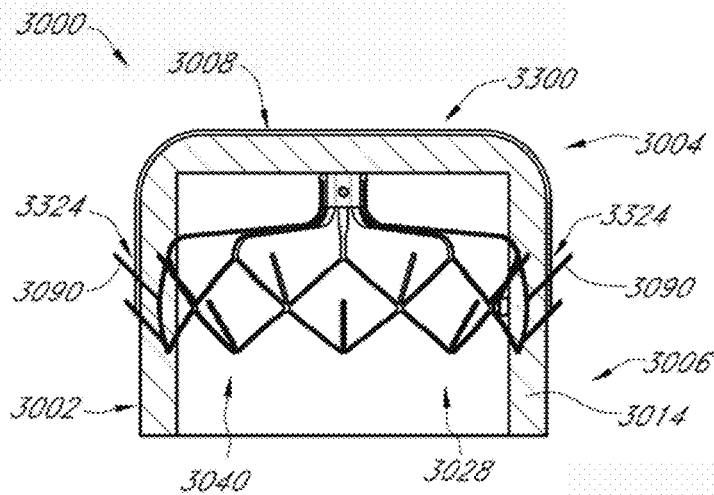


FIG. 87C

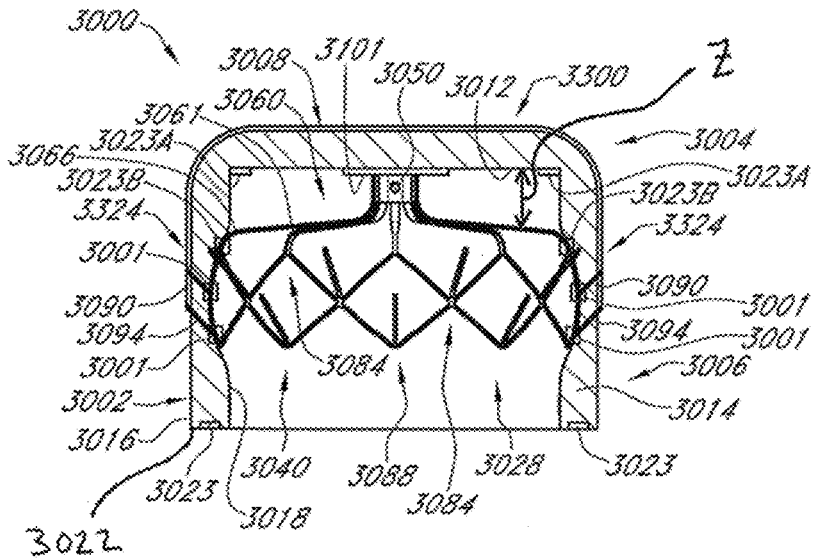


FIG. 87D

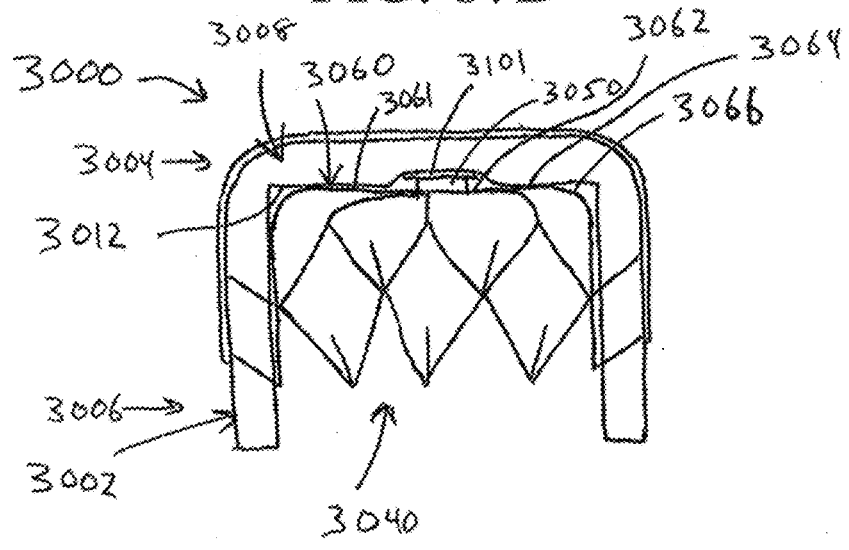


FIG. 87E

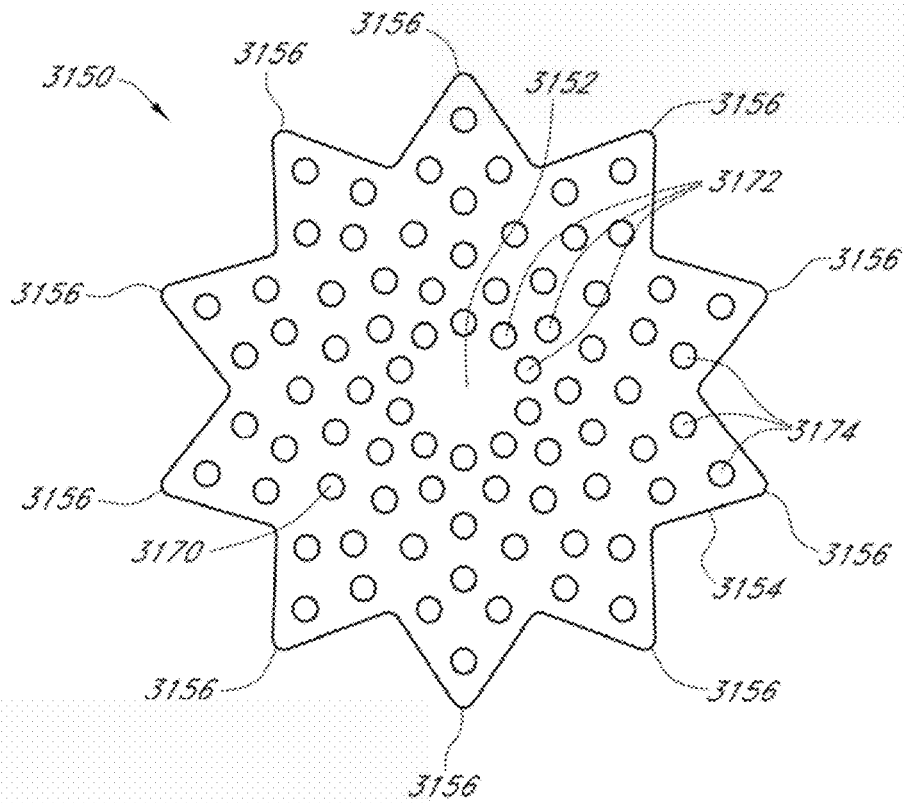


FIG. 88A

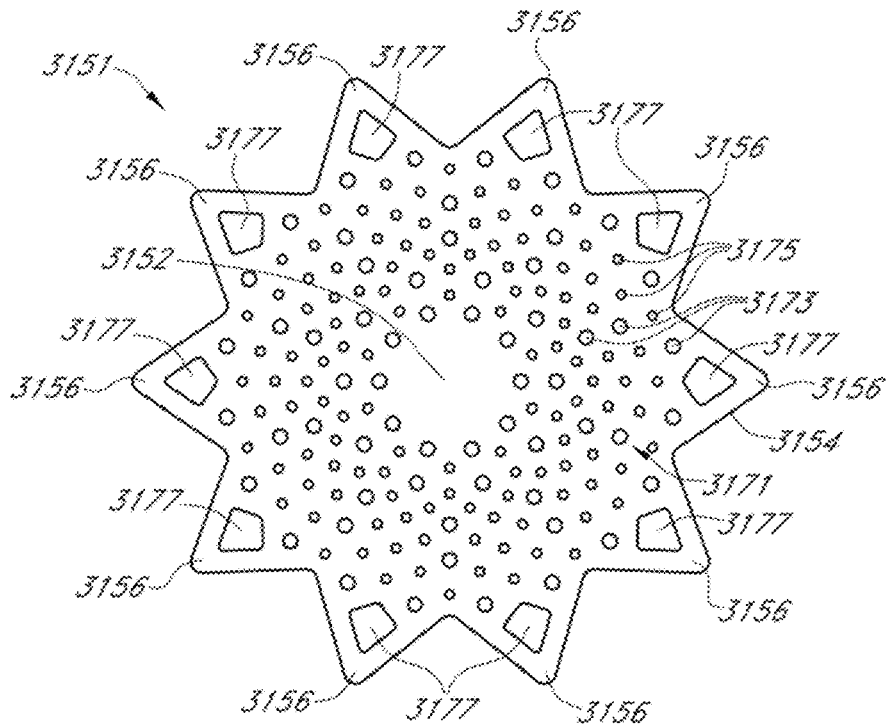


FIG. 88B

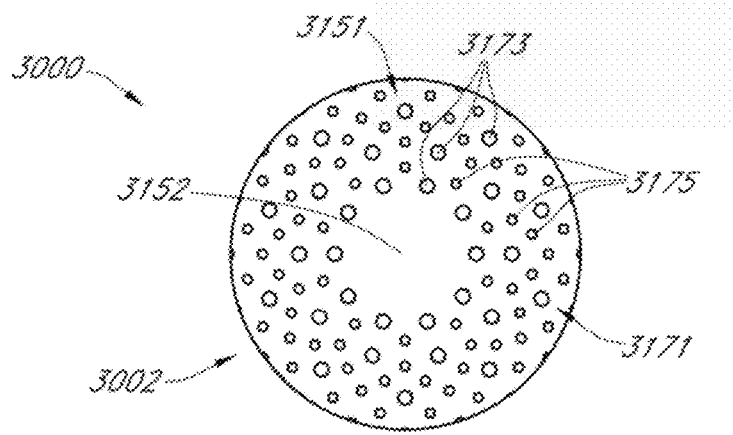


FIG. 88C

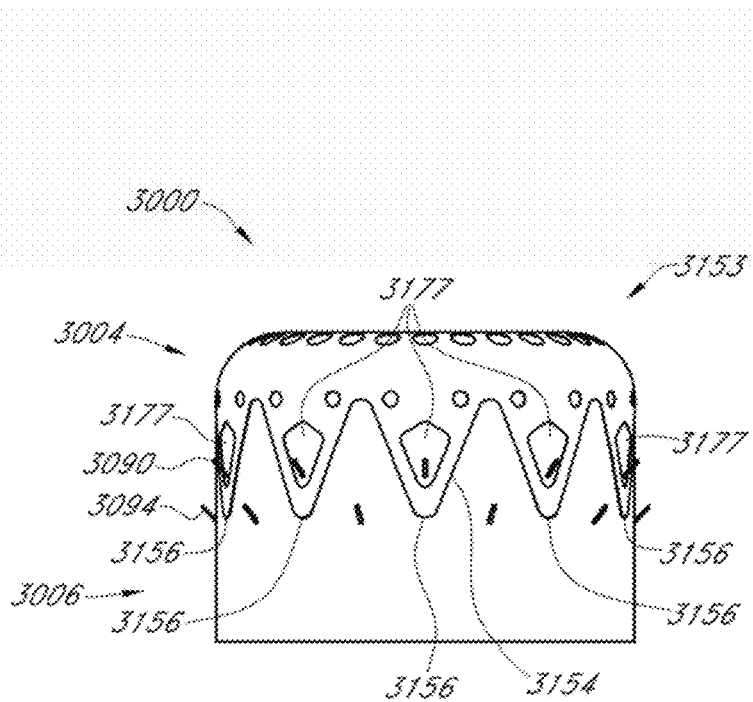


FIG. 88D

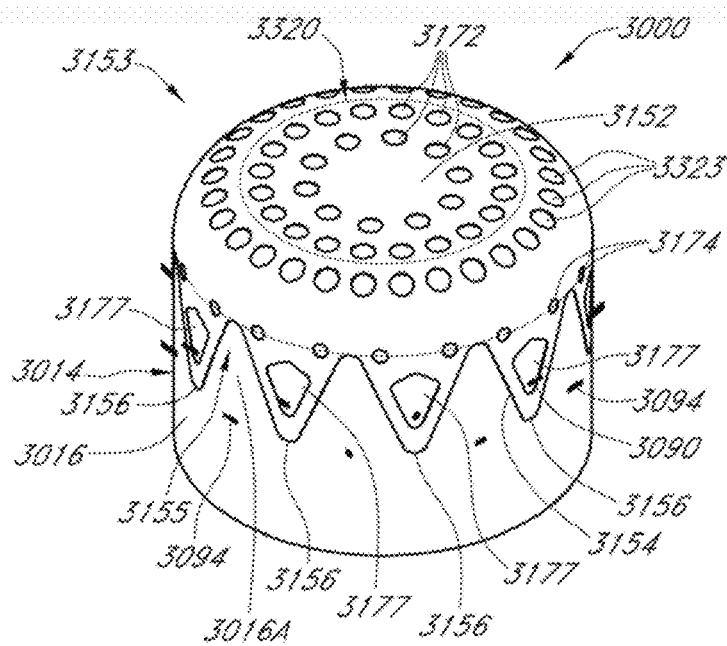


FIG. 88E

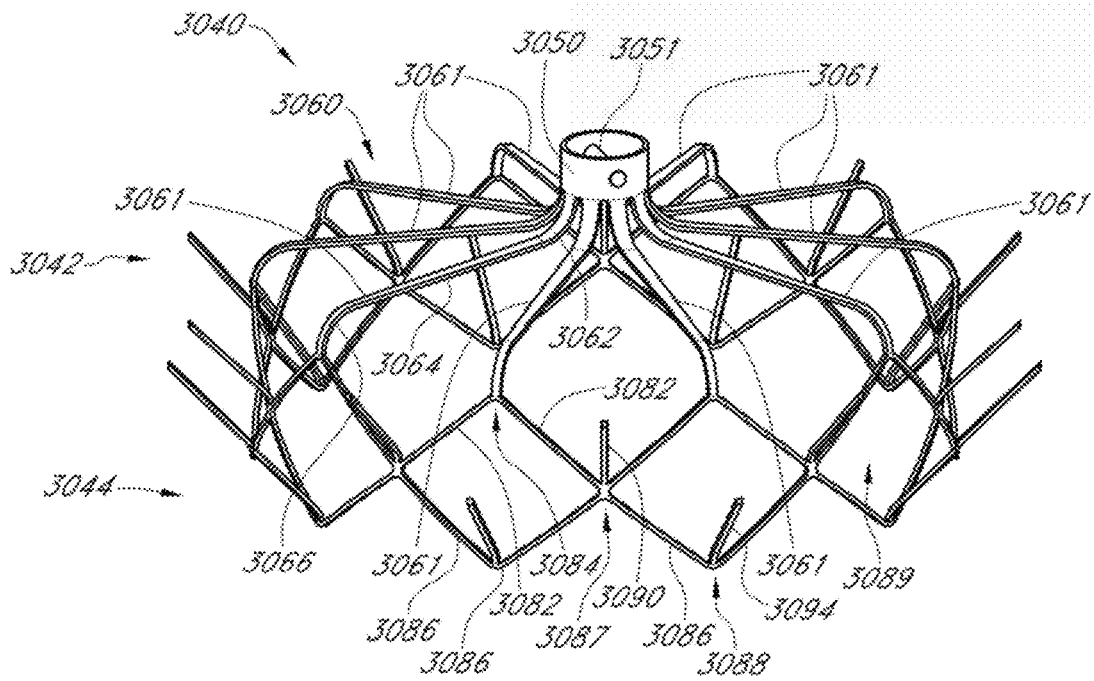


FIG. 89A

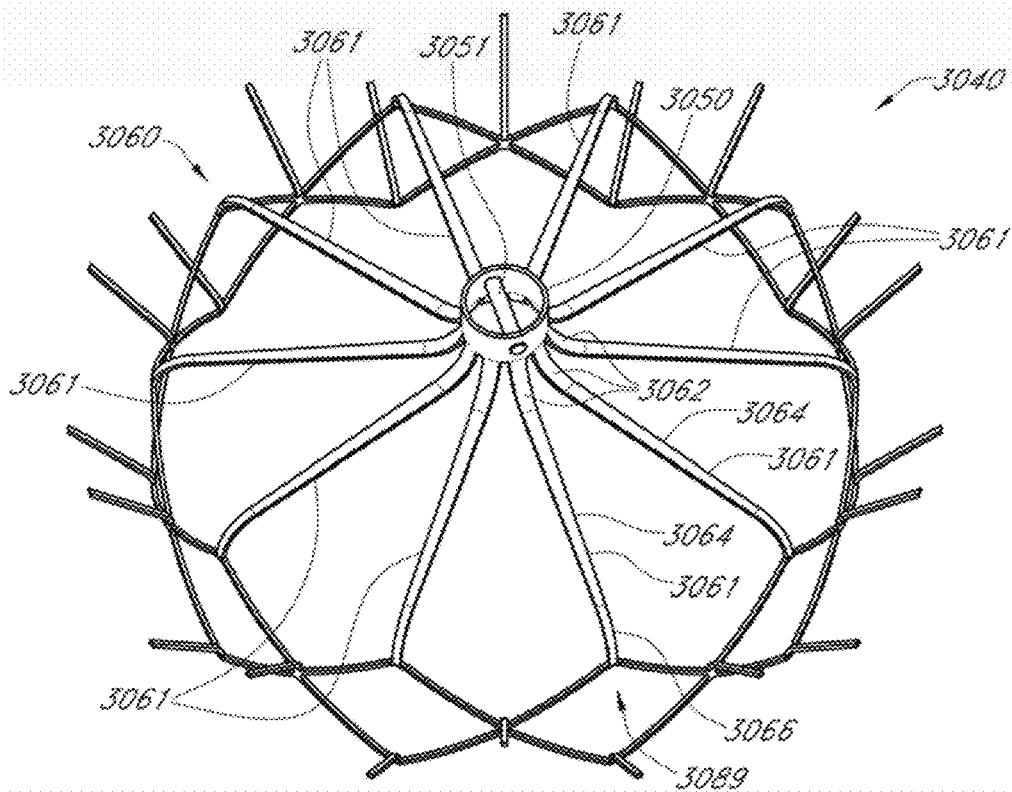


FIG. 89B

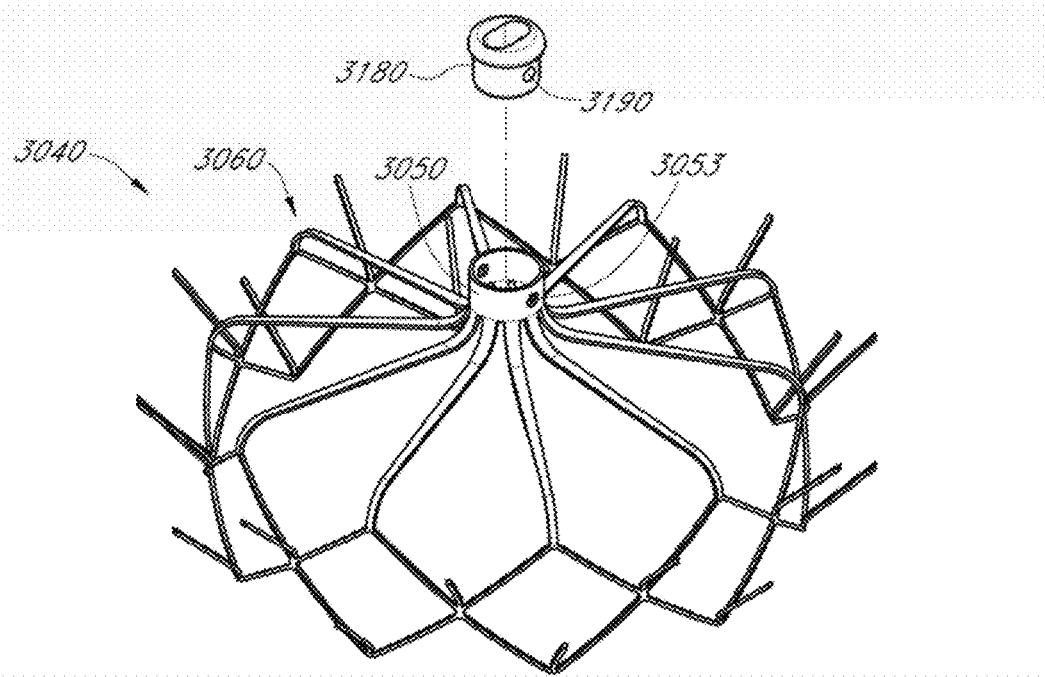


FIG. 90A

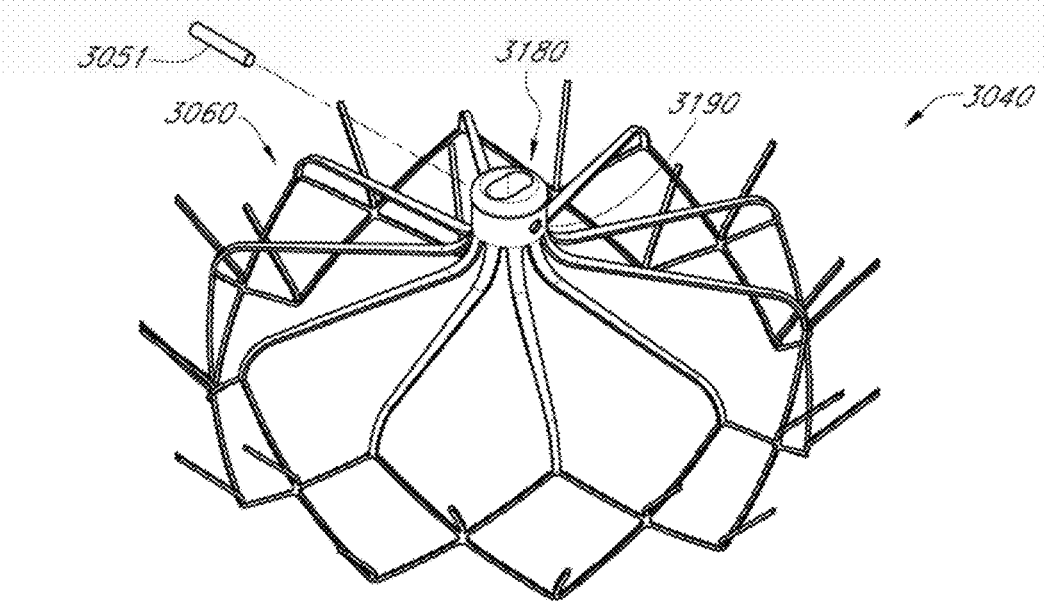


FIG. 90B

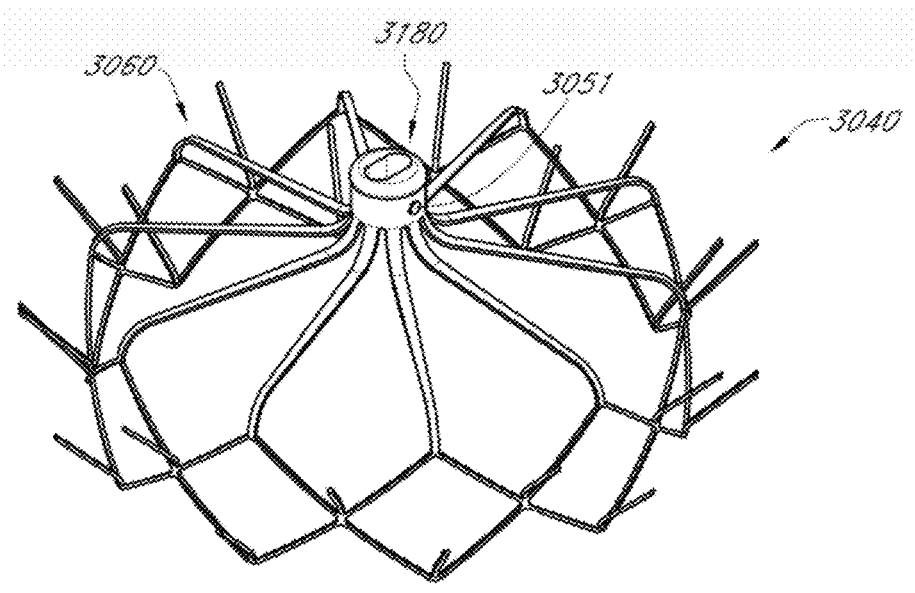


FIG. 90C

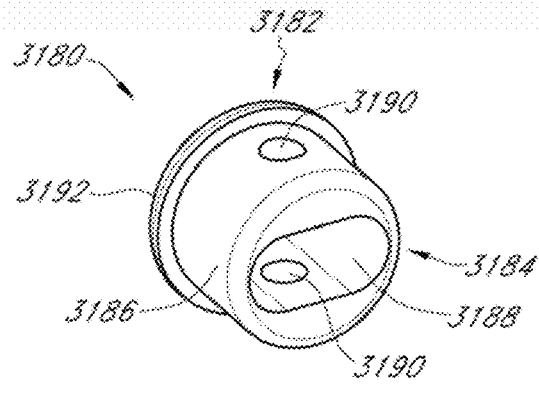


FIG. 90D

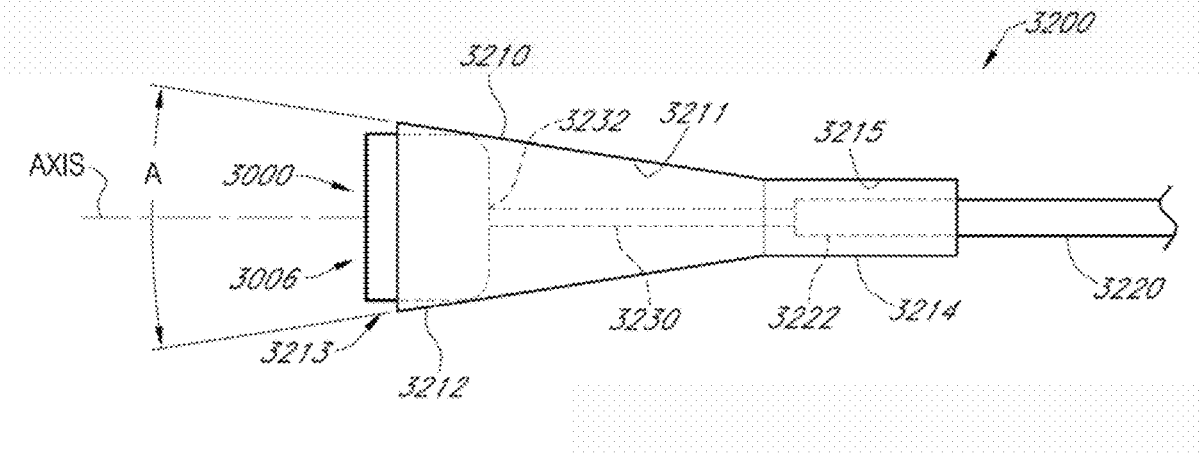


FIG. 91

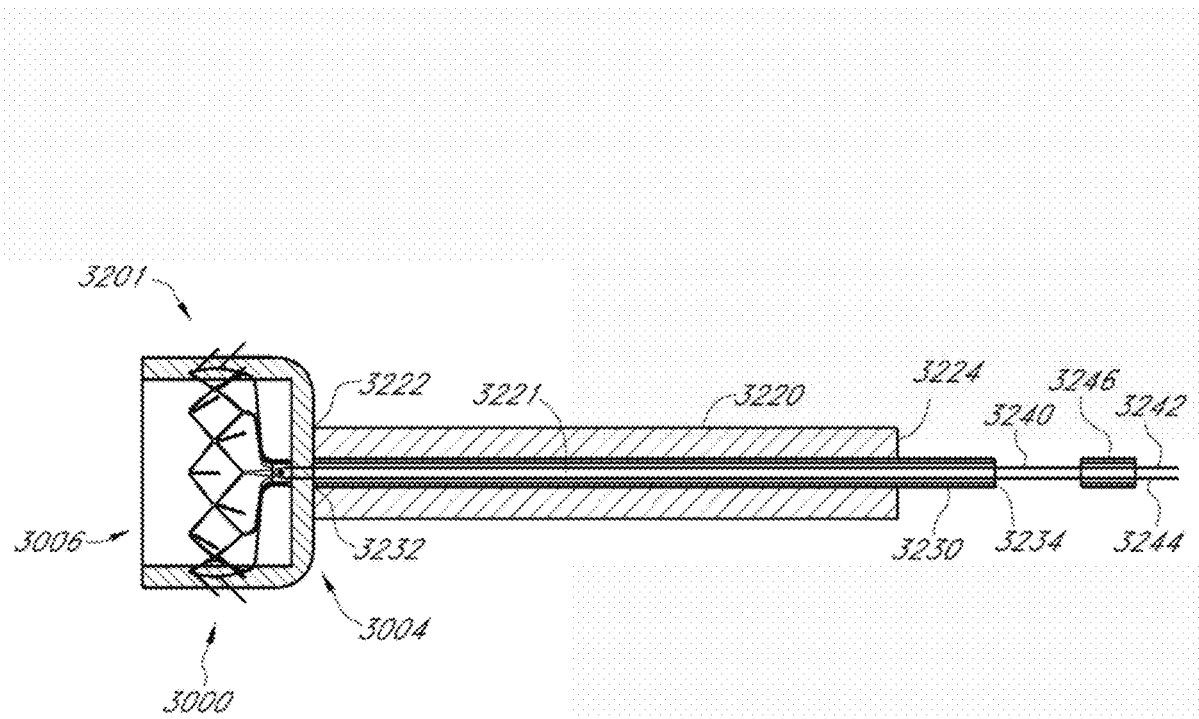


FIG. 92A

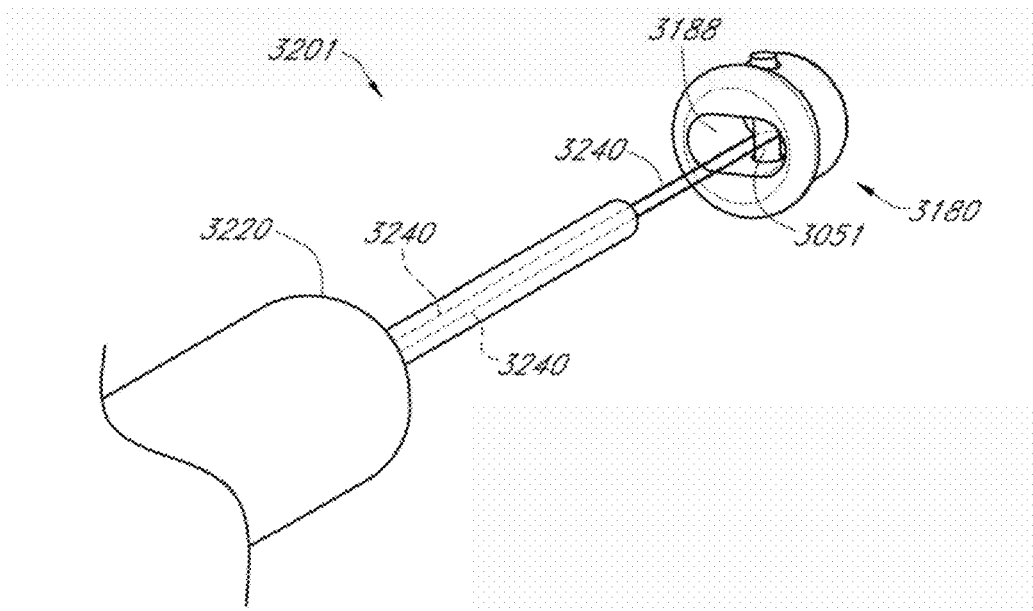


FIG. 92B

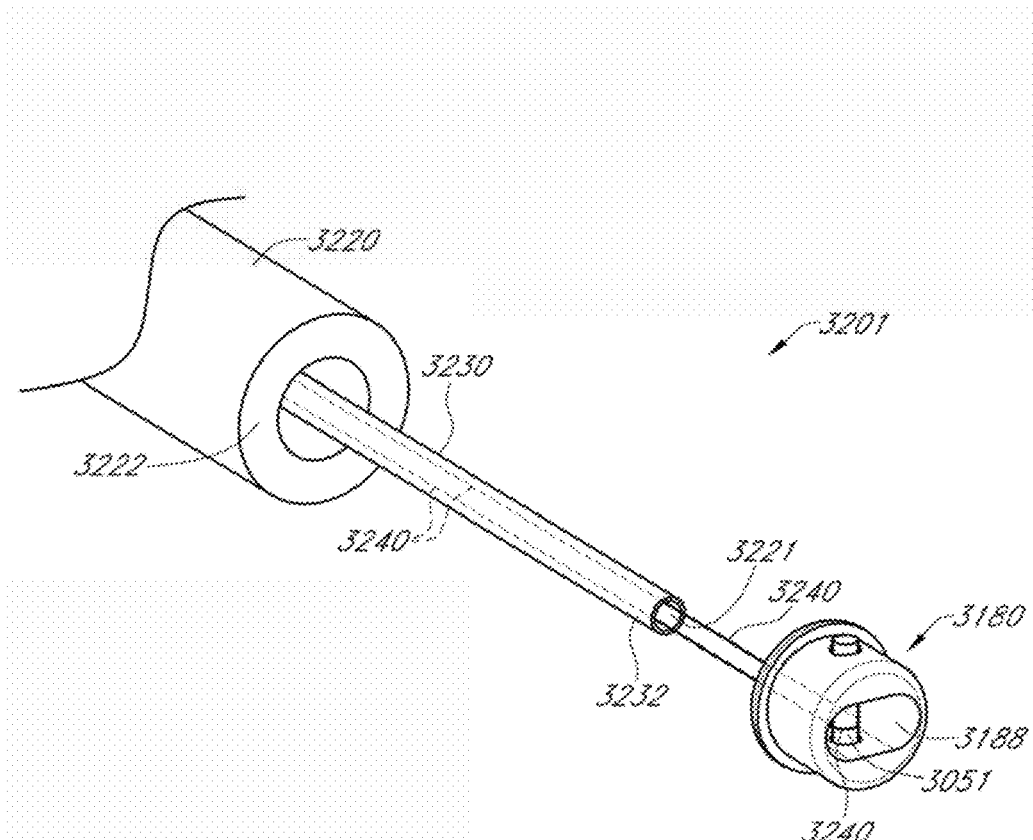


FIG. 92C

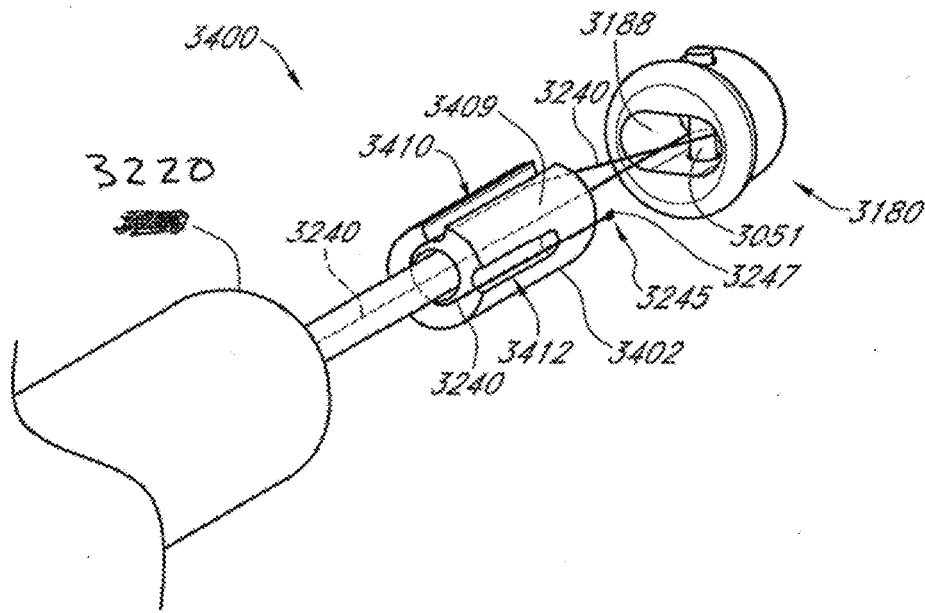


FIG. 93A

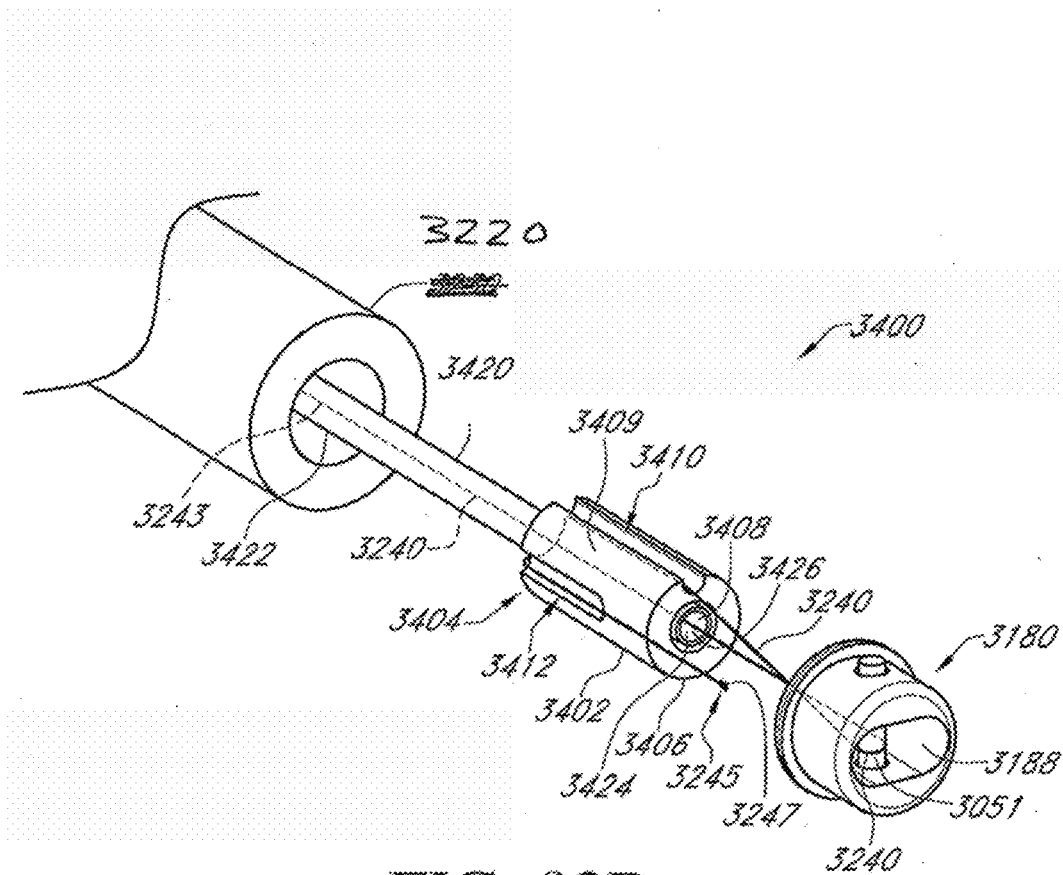


FIG. 93B

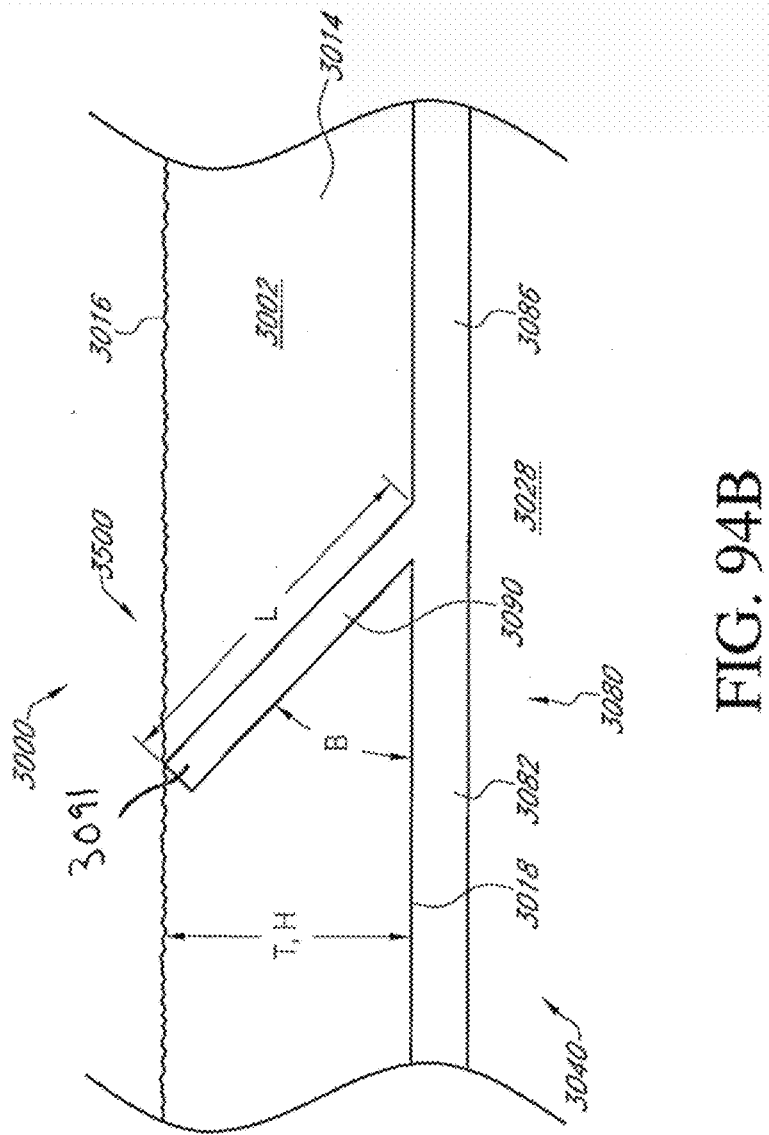


FIG. 94B

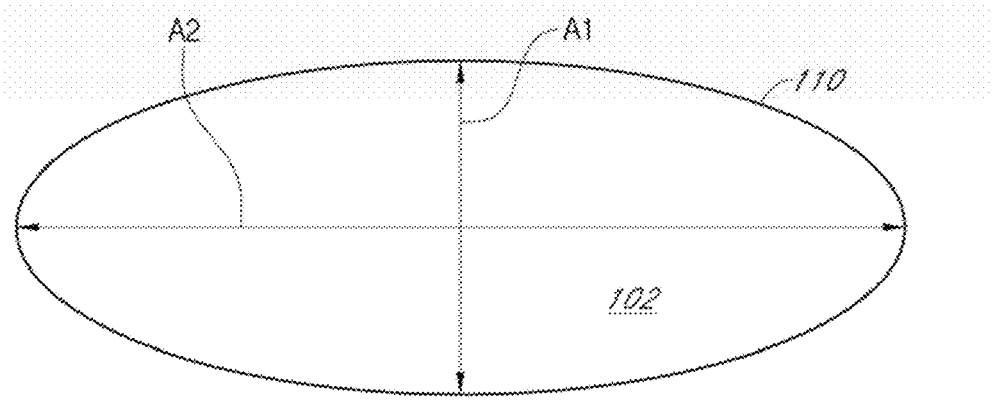


FIG. 95A

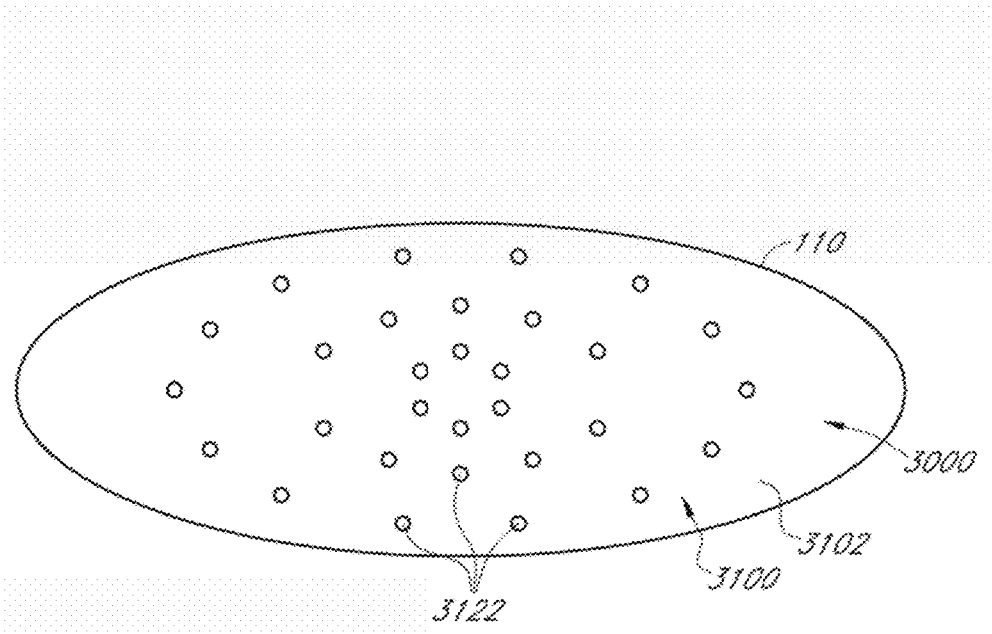


FIG. 95B

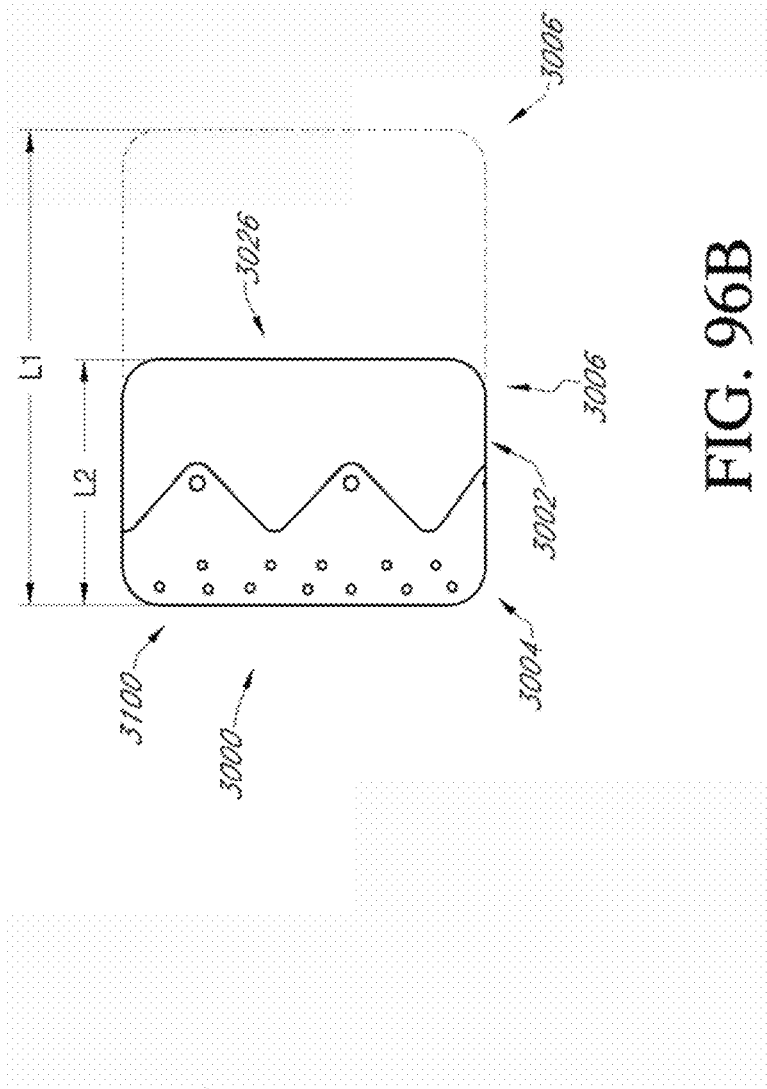


FIG. 96A

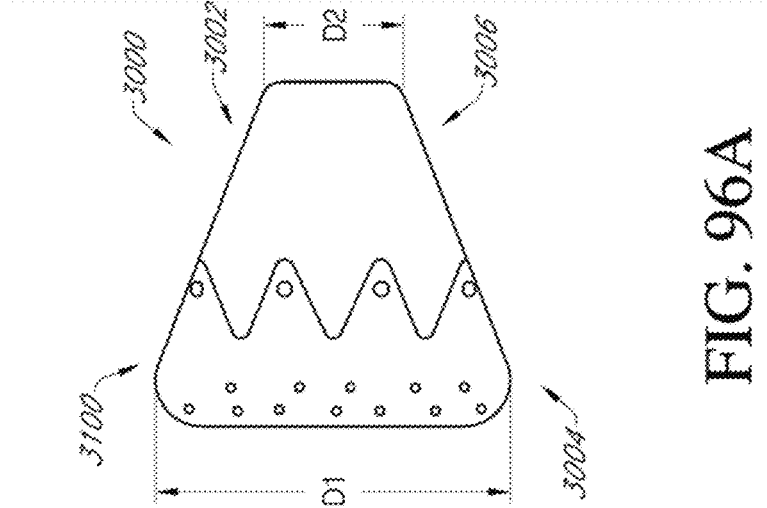


FIG. 96B

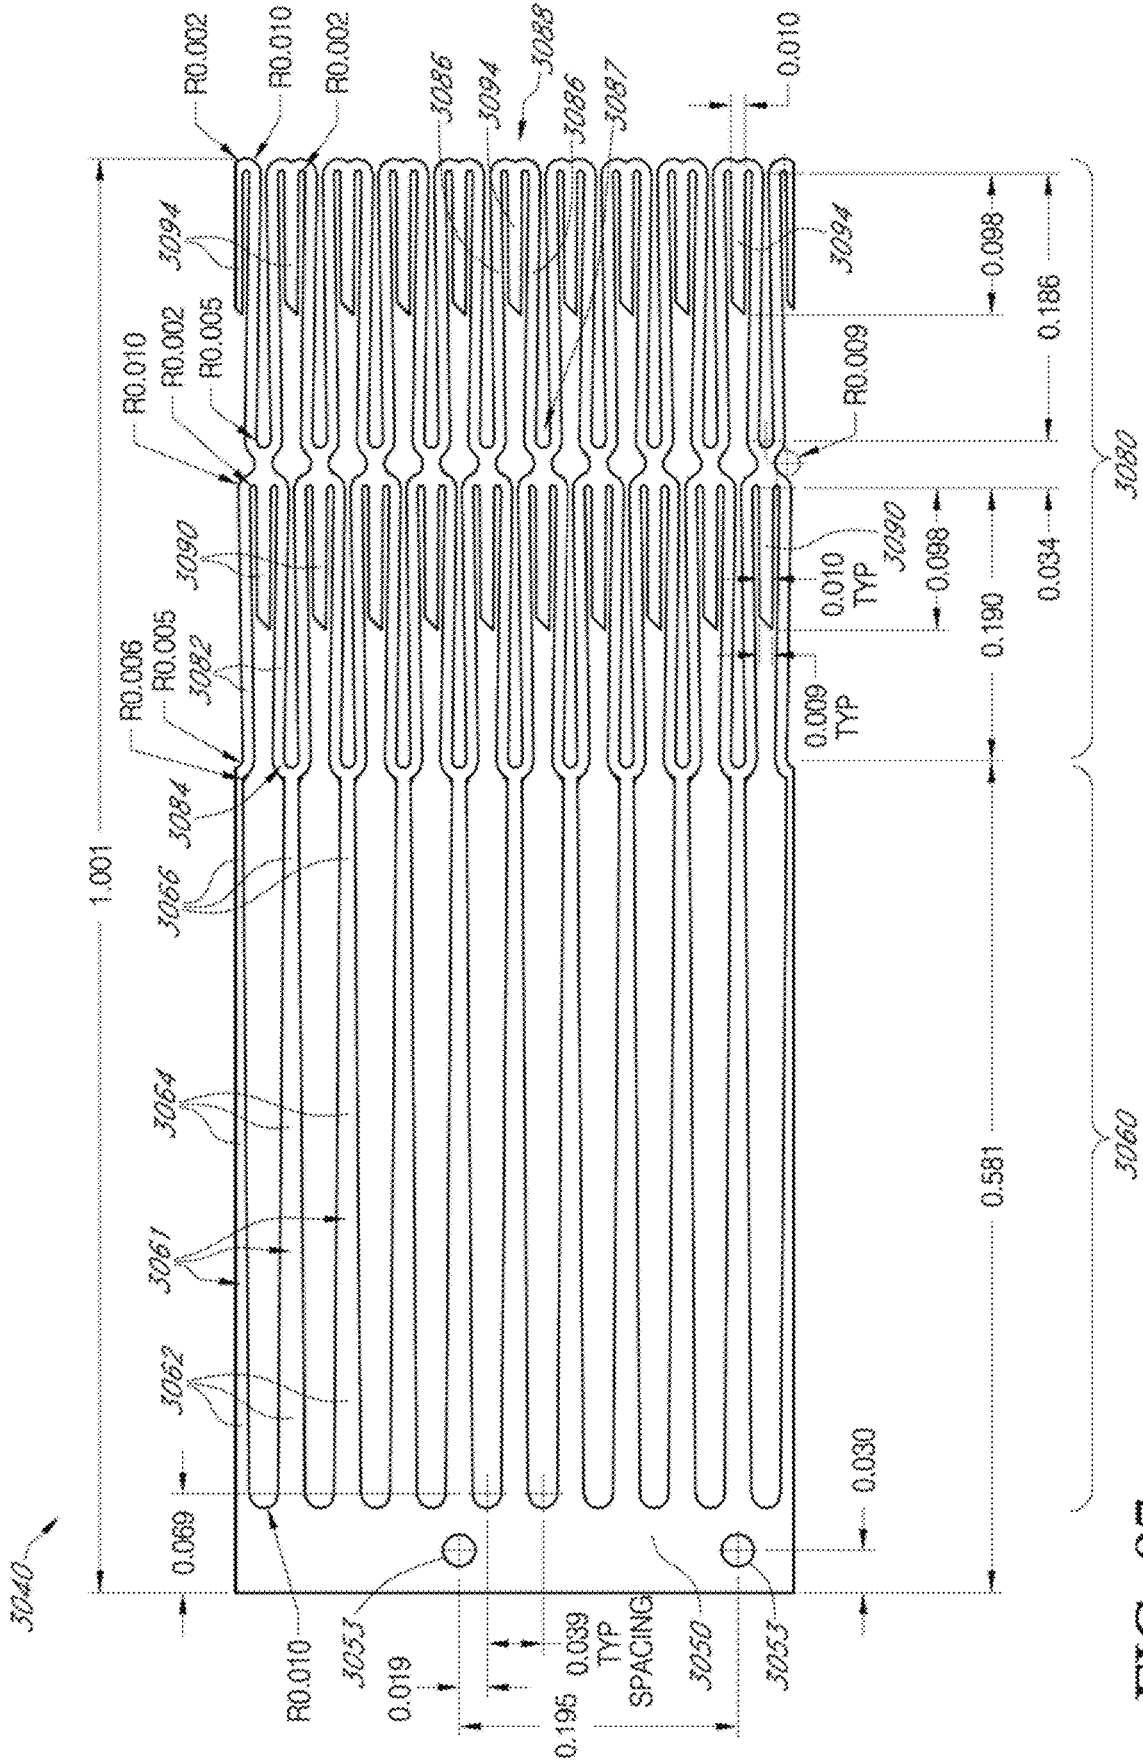


FIG. 97

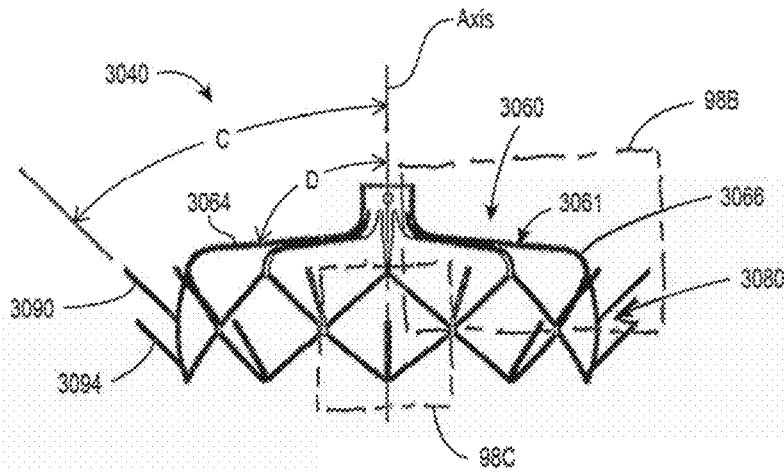


FIG. 98A

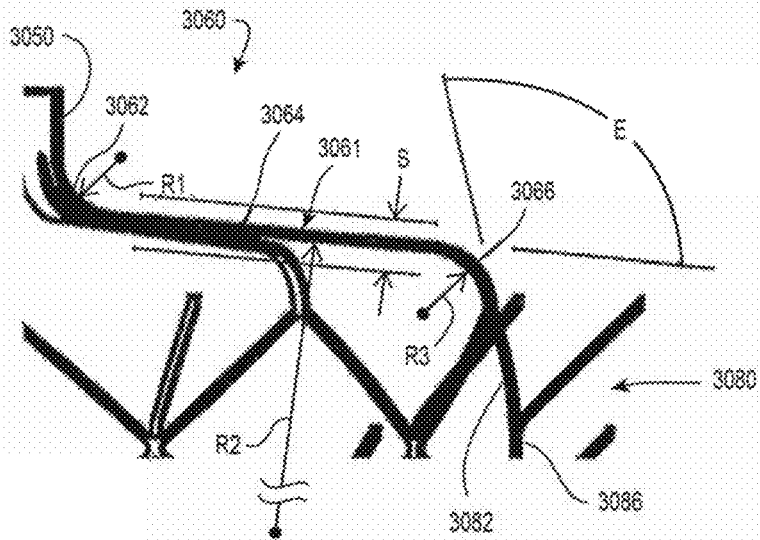


FIG. 98B

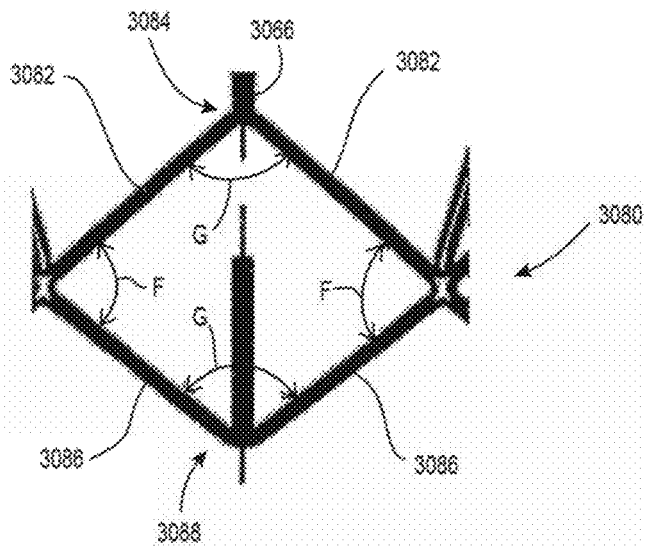


FIG. 98C

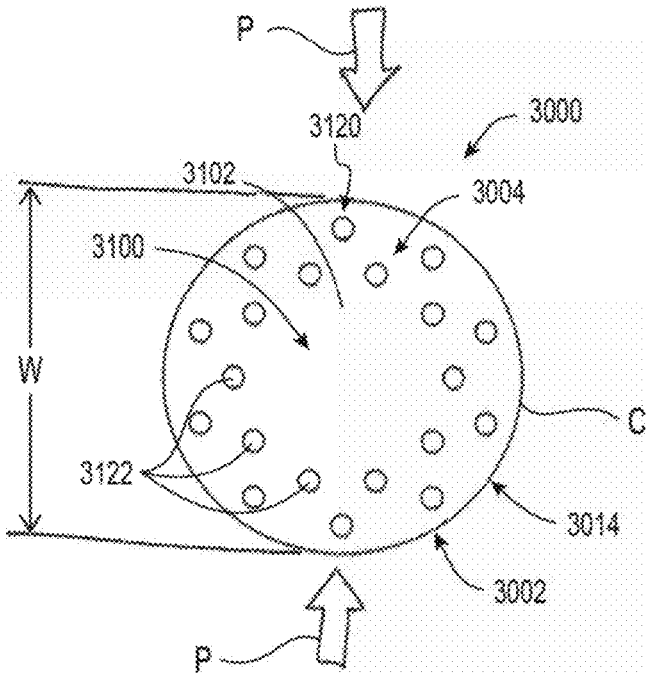


FIG. 99A

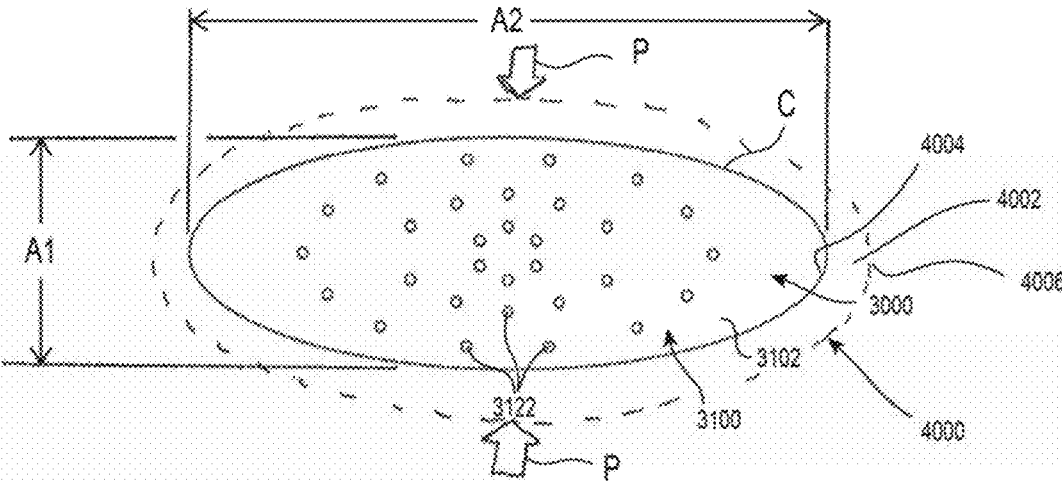


FIG. 99B

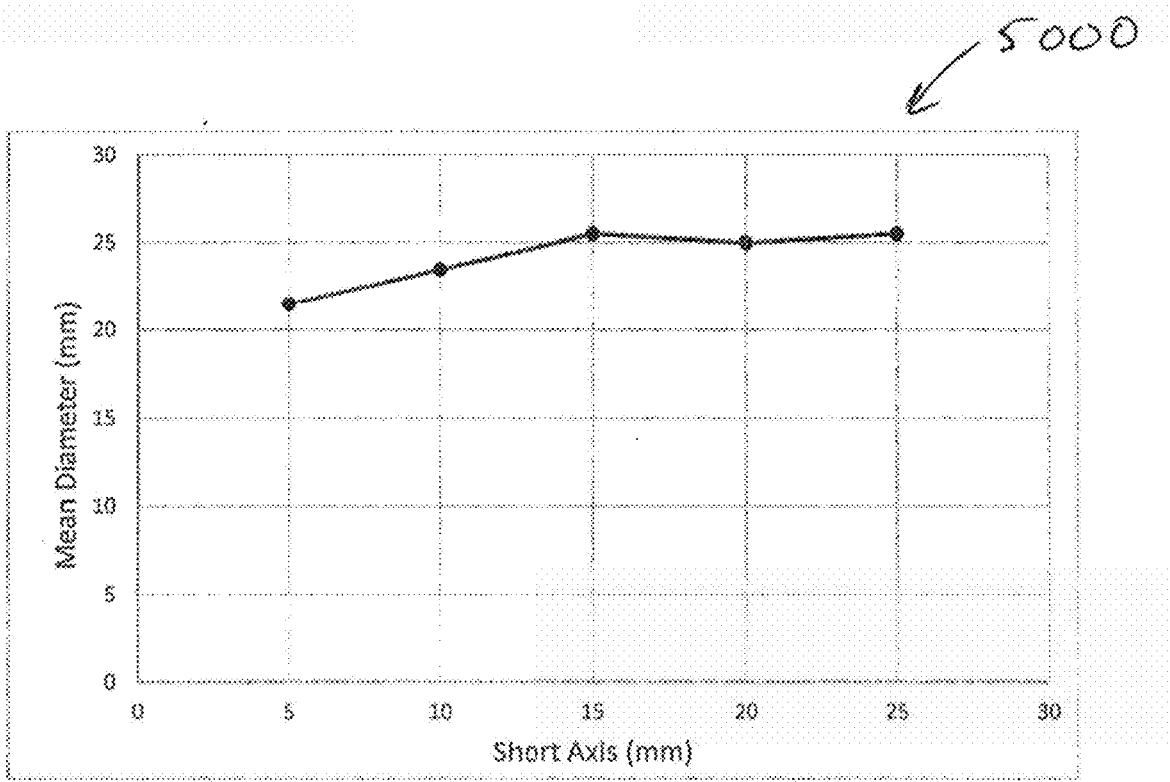


FIG. 100A

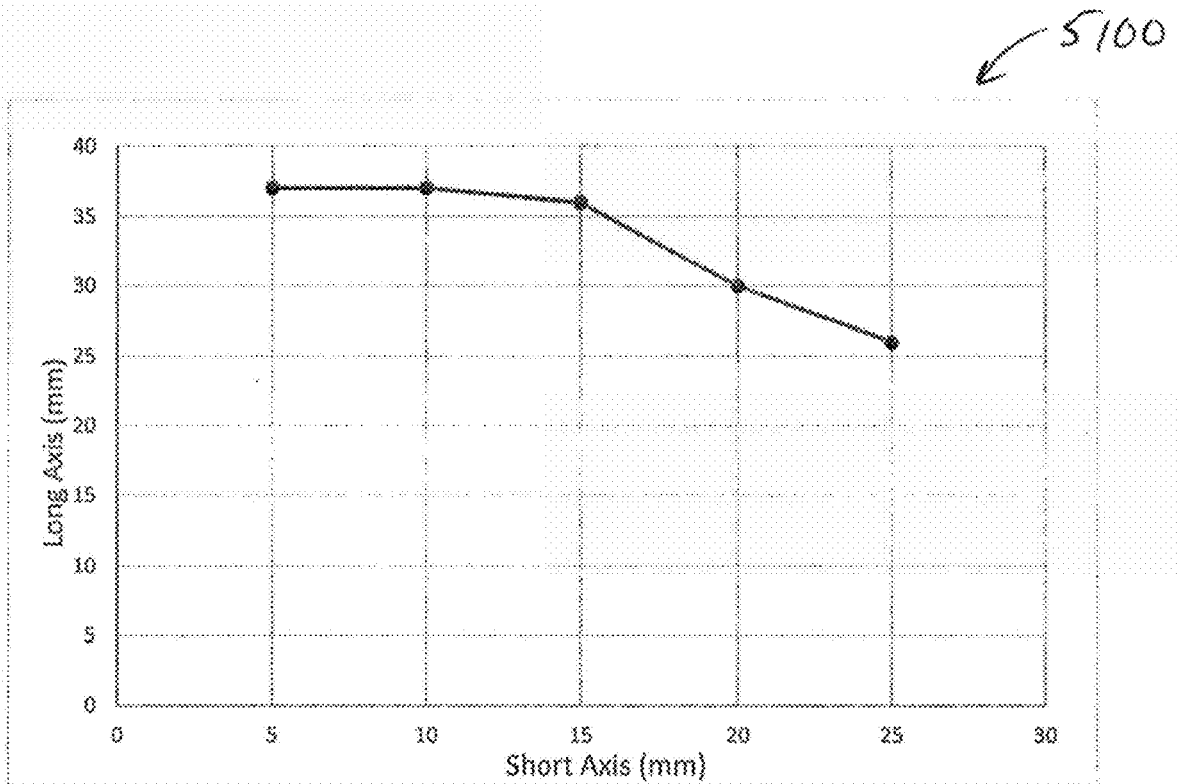


FIG. 100B

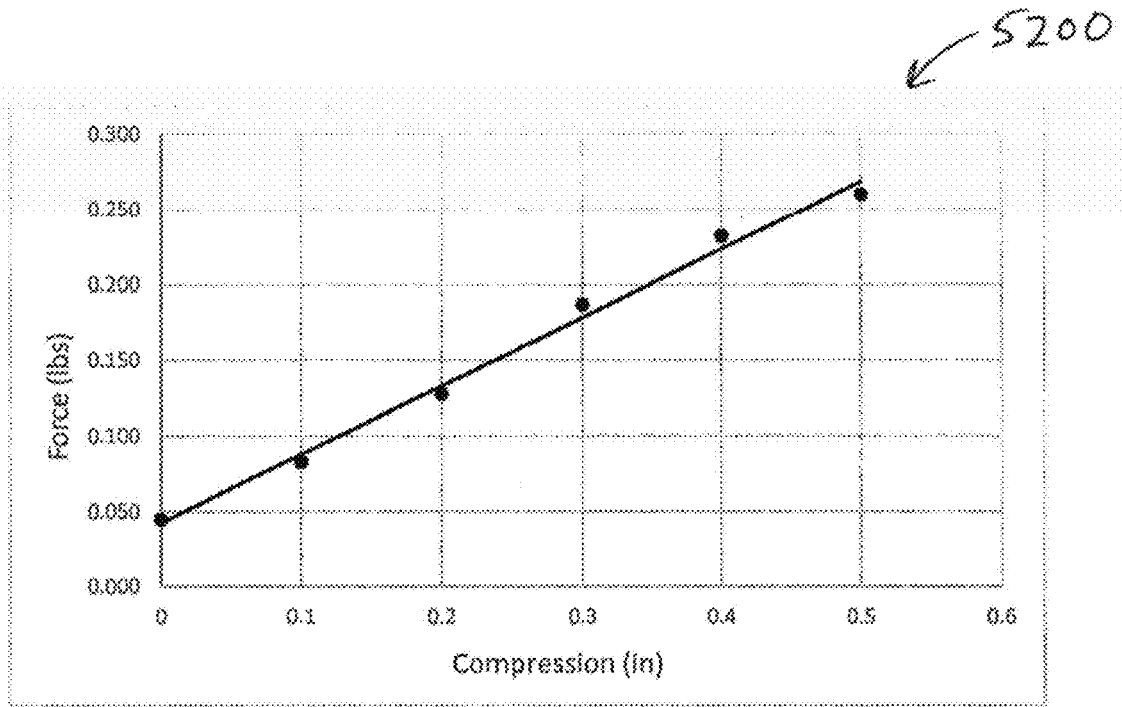


FIG. 100C

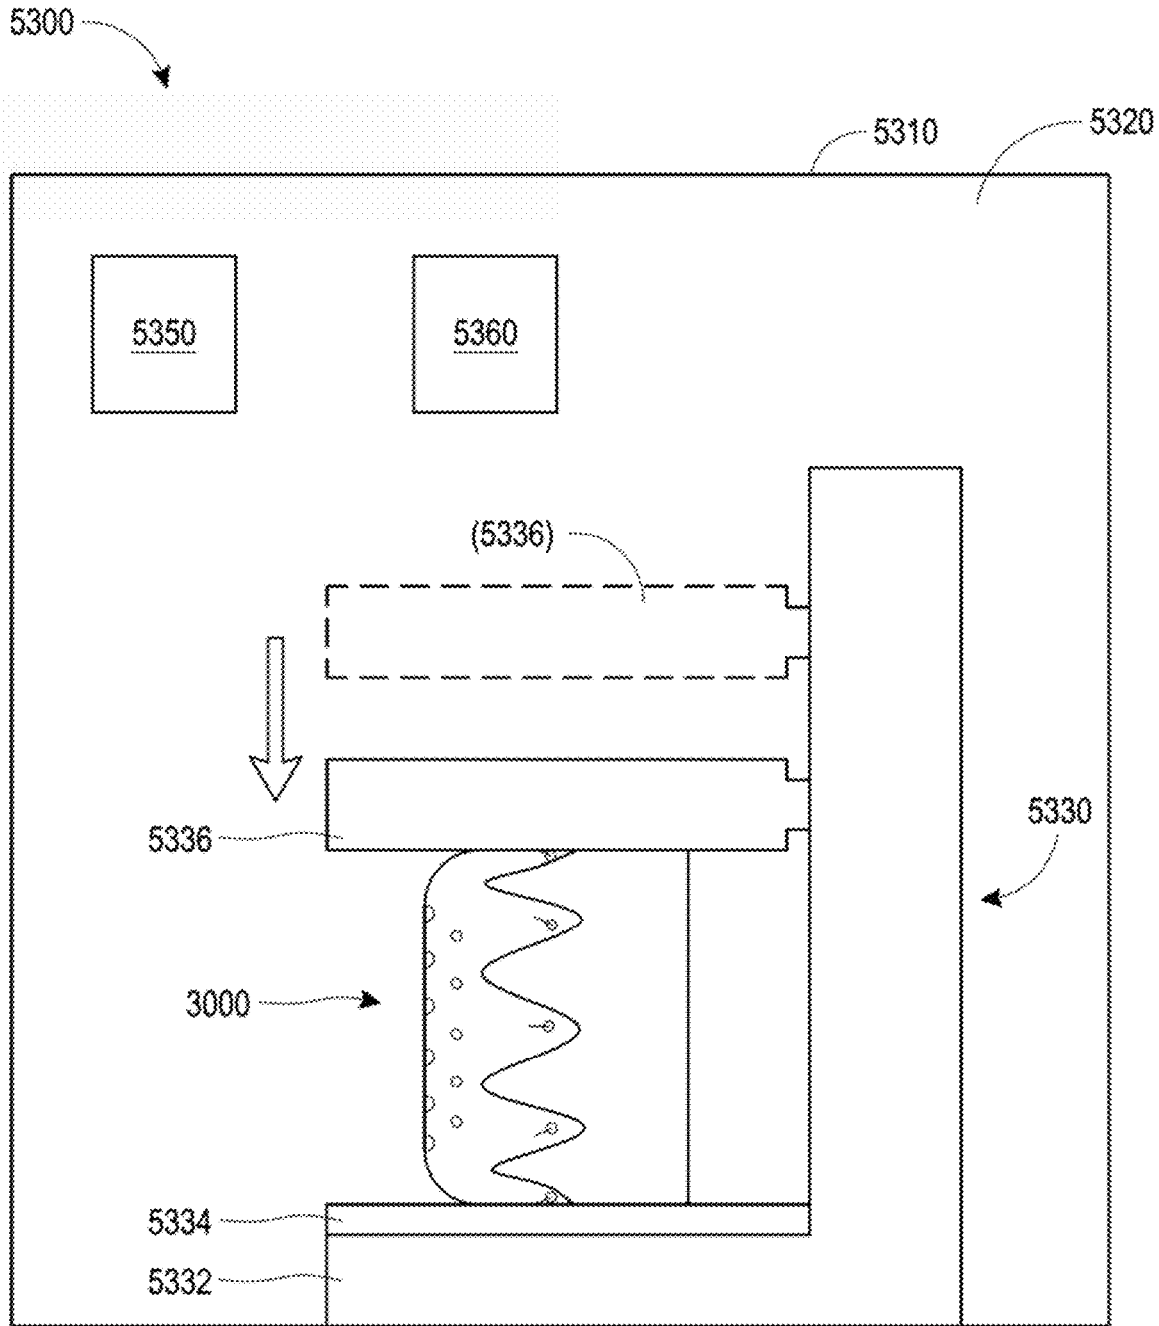


Fig. 101

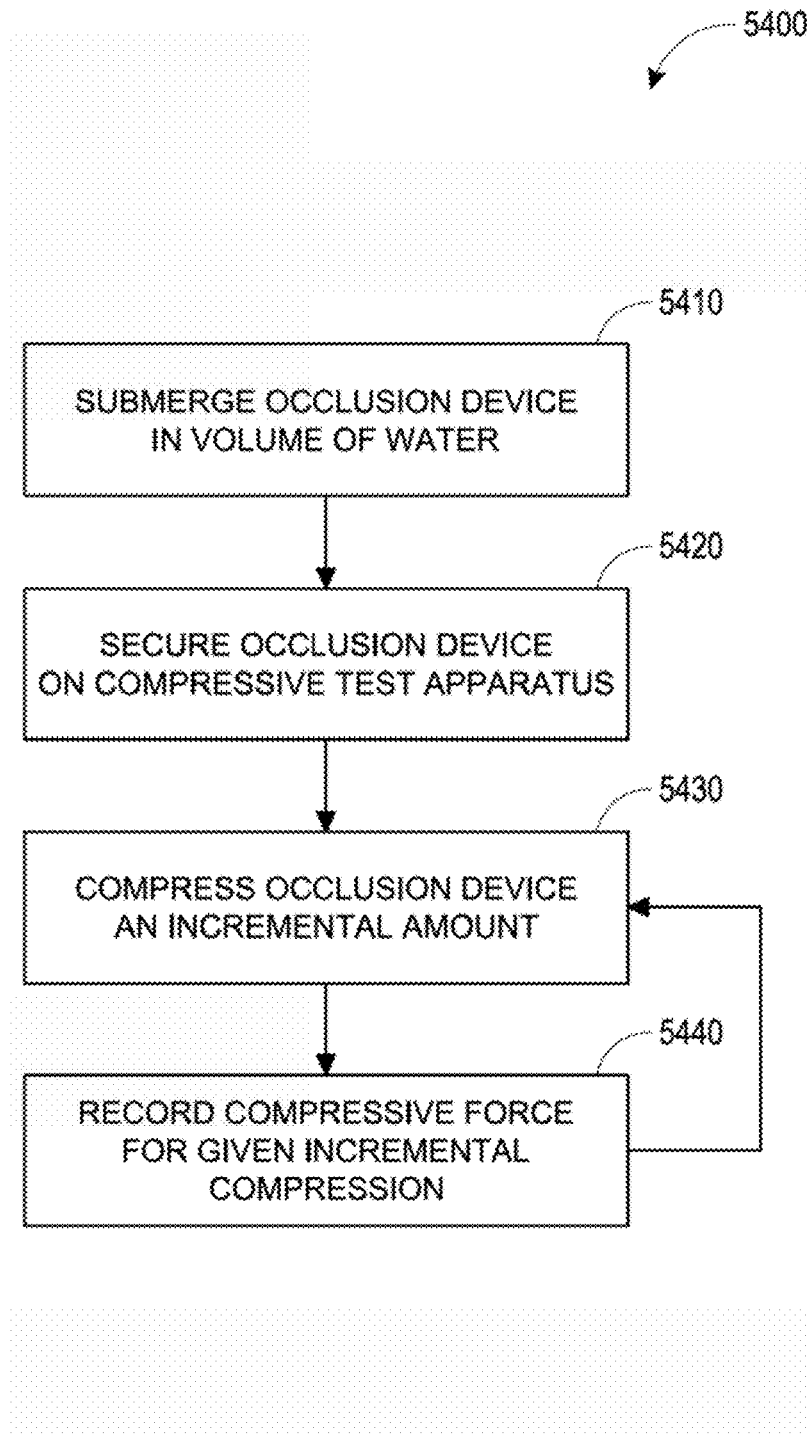


Fig. 102

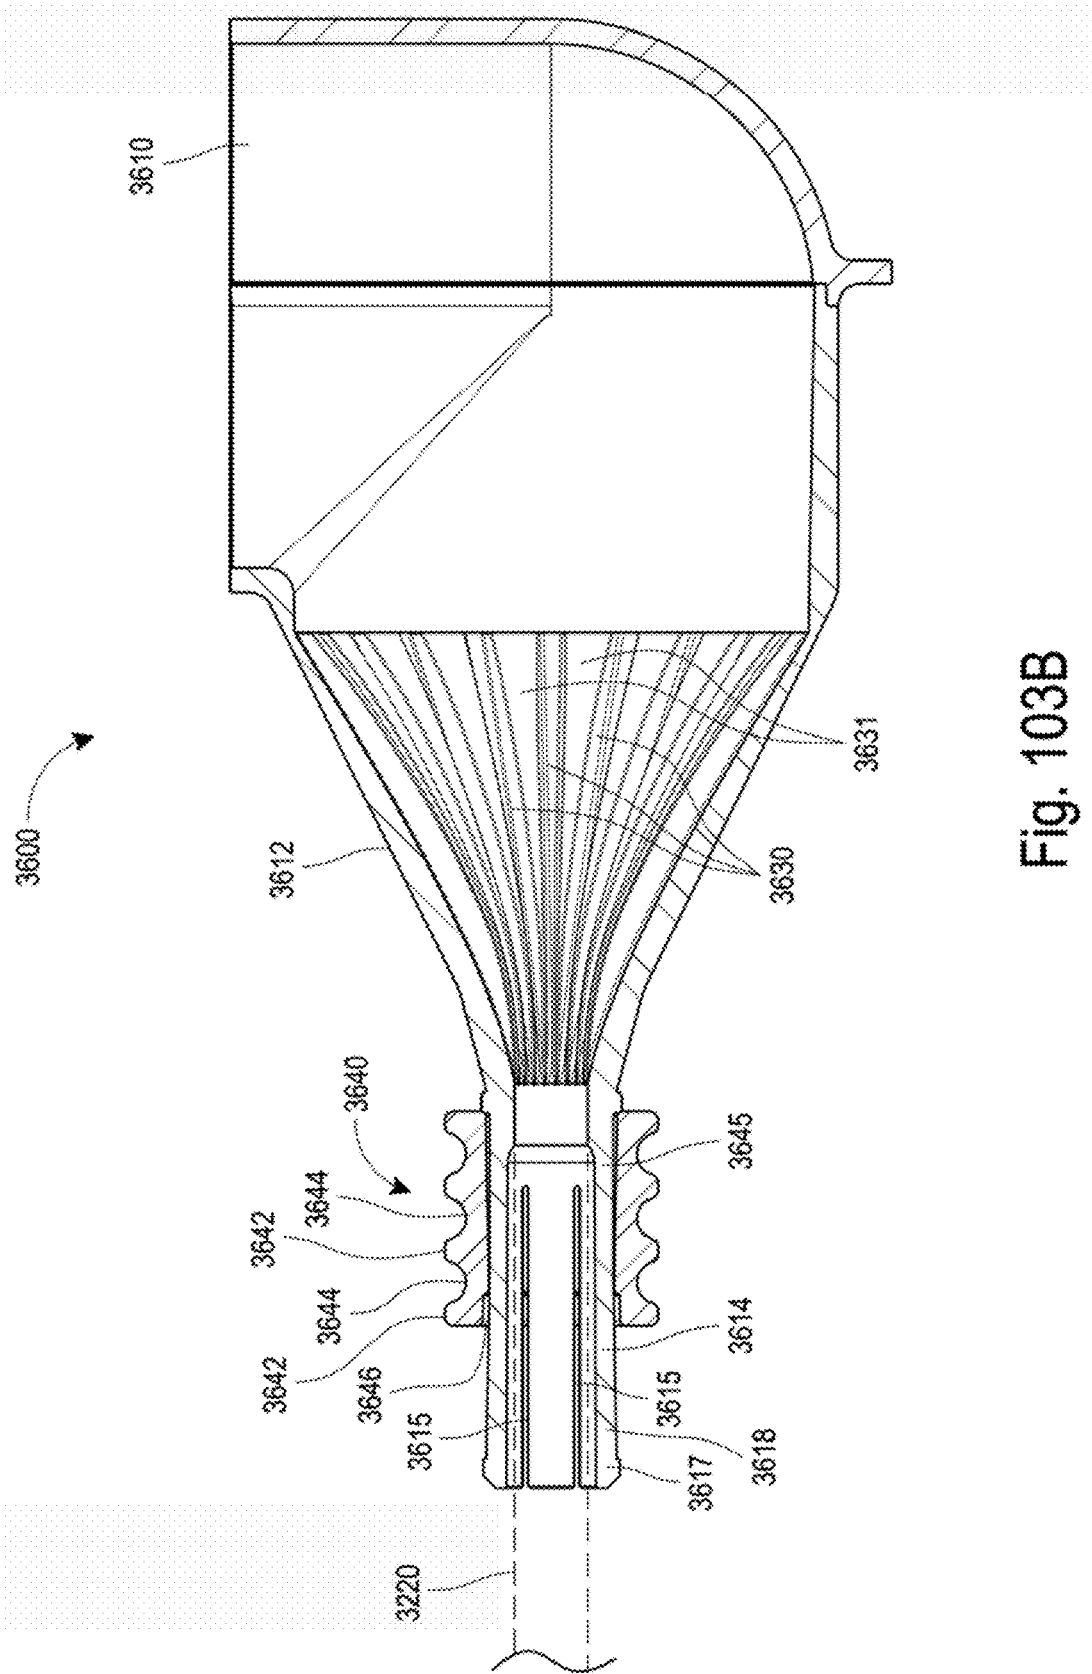
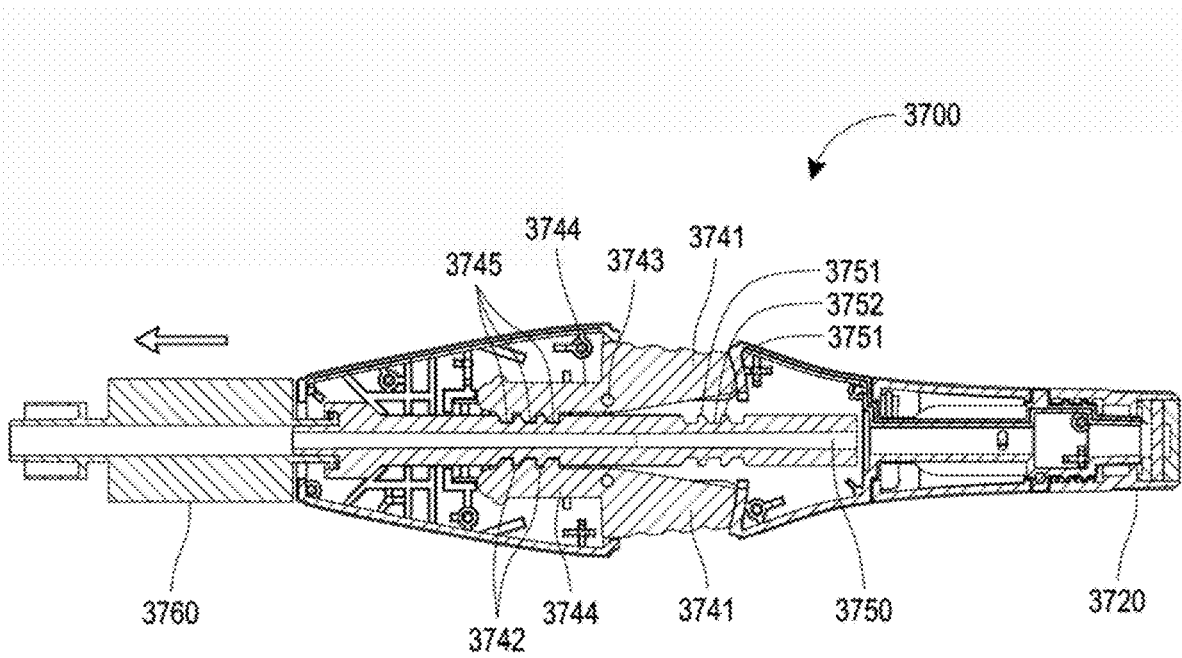
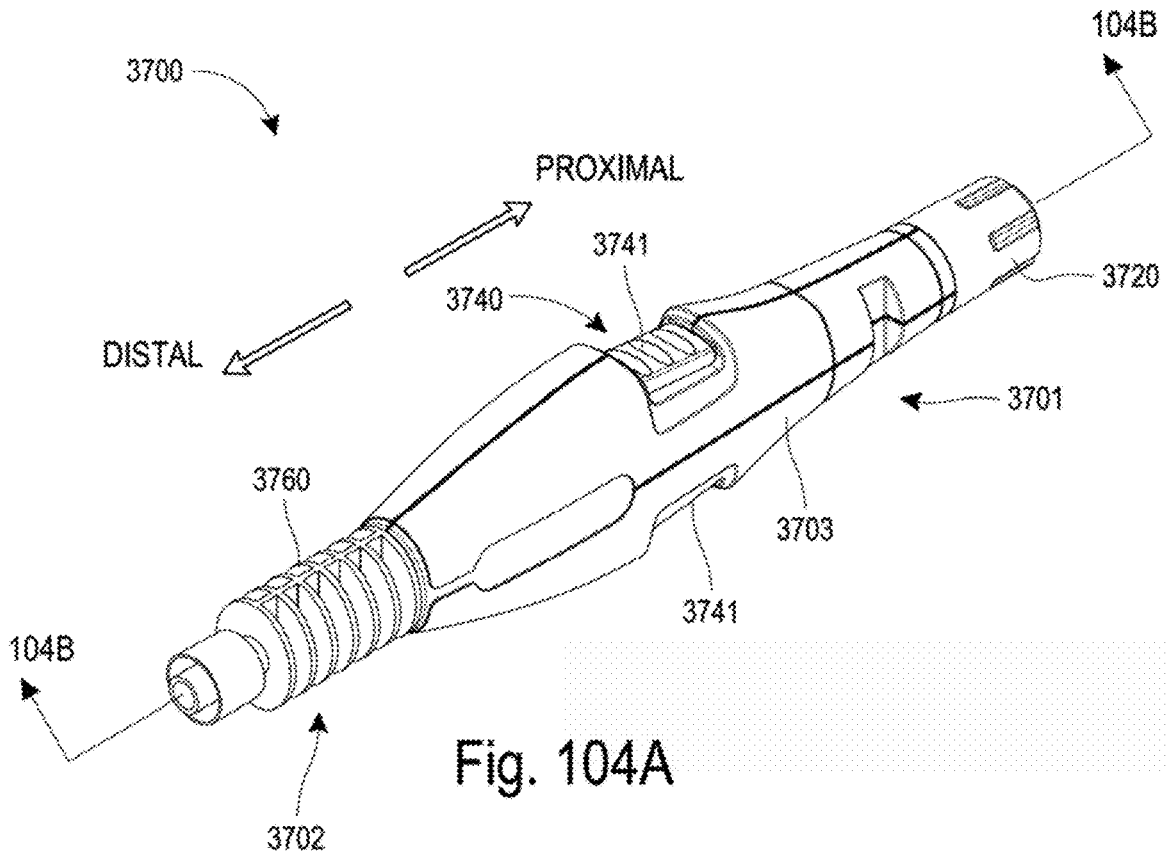


Fig. 103B



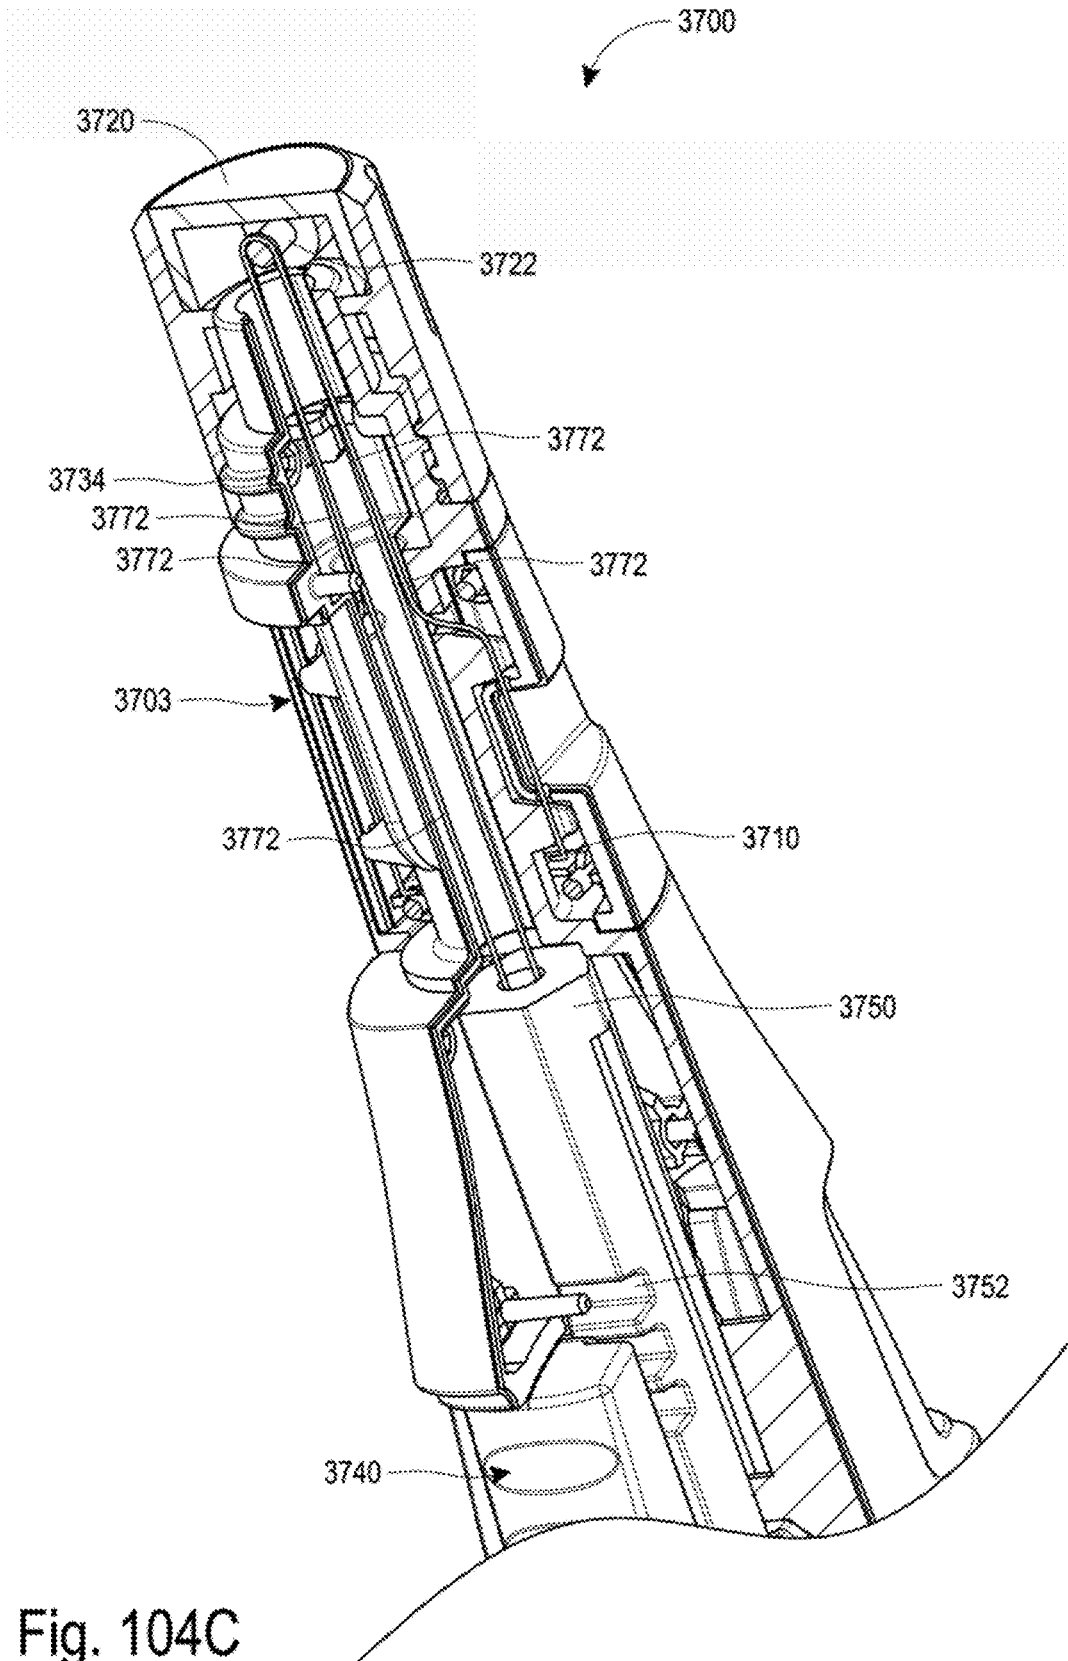


Fig. 104C

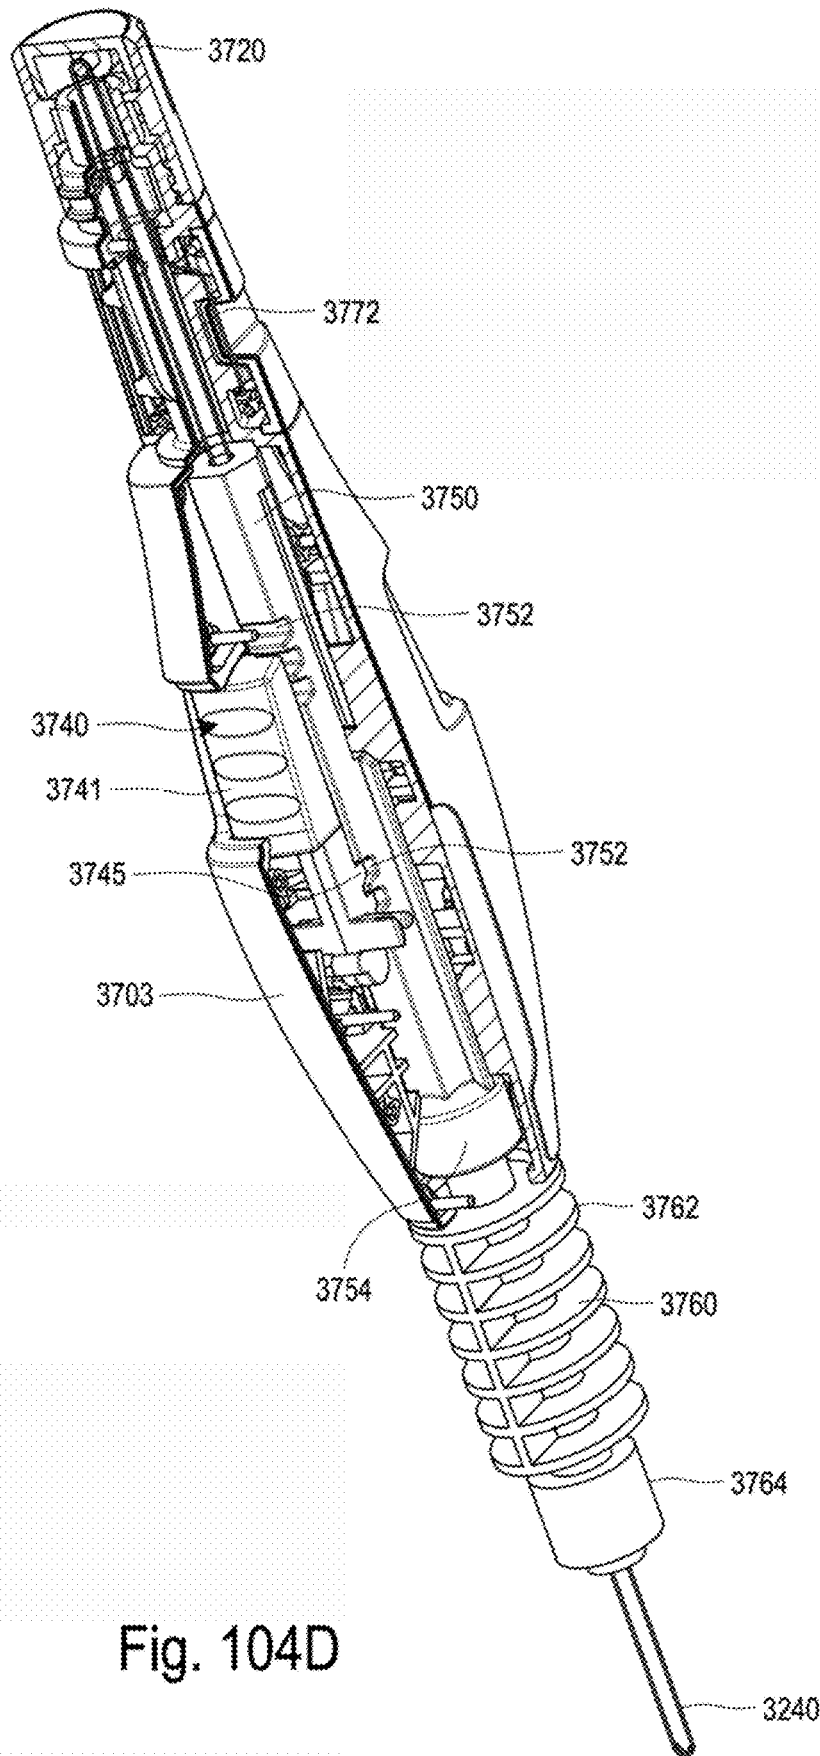


Fig. 104D

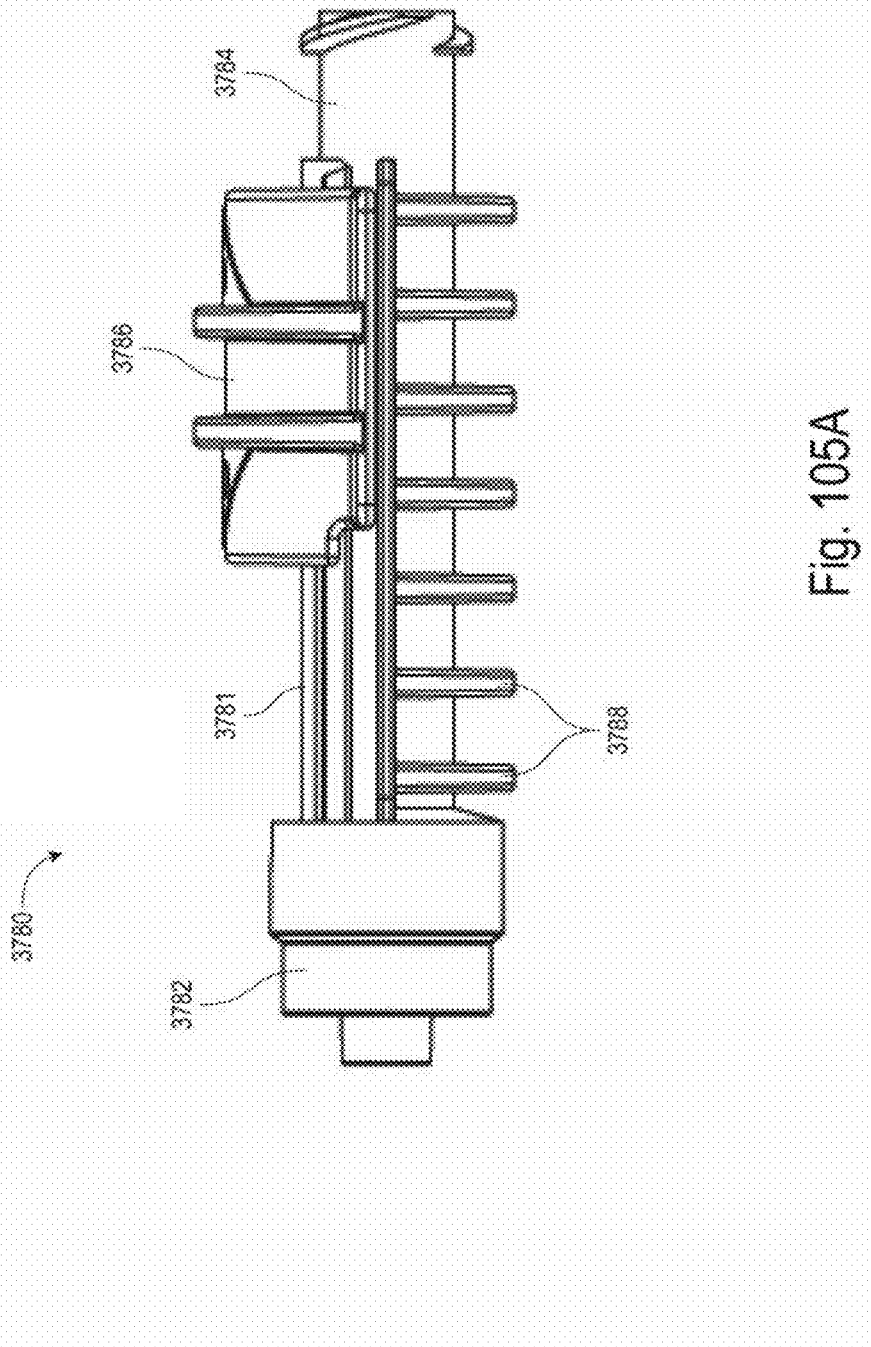


Fig. 105A

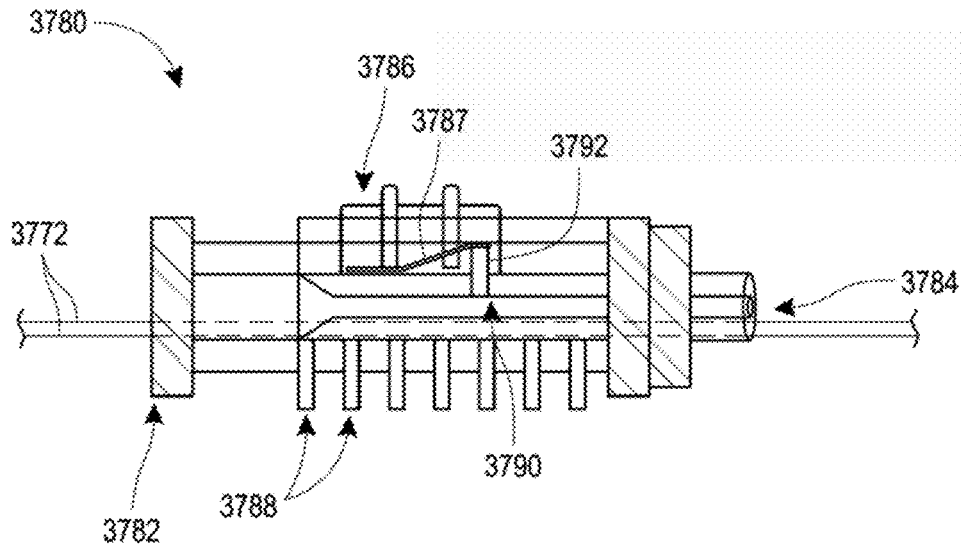


Fig. 105B

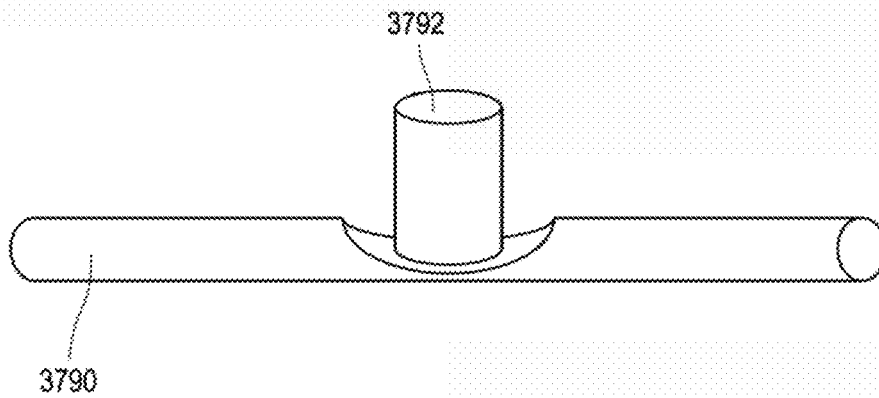


Fig. 105C

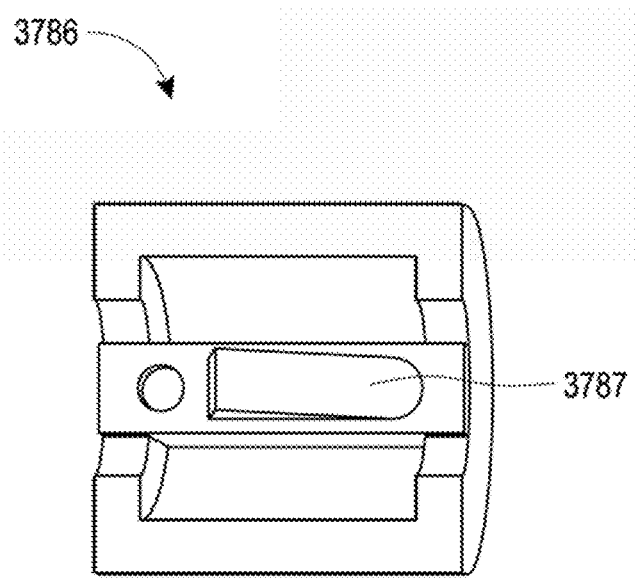


Fig. 105D

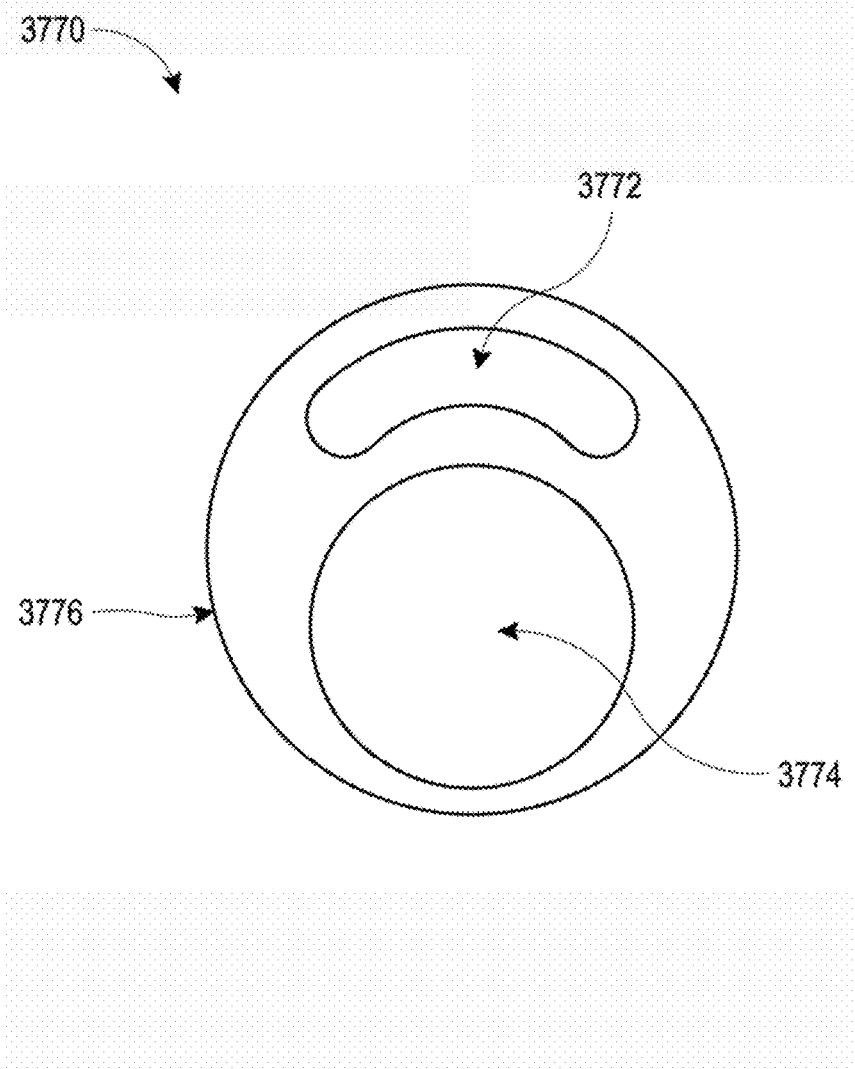


Fig. 106A

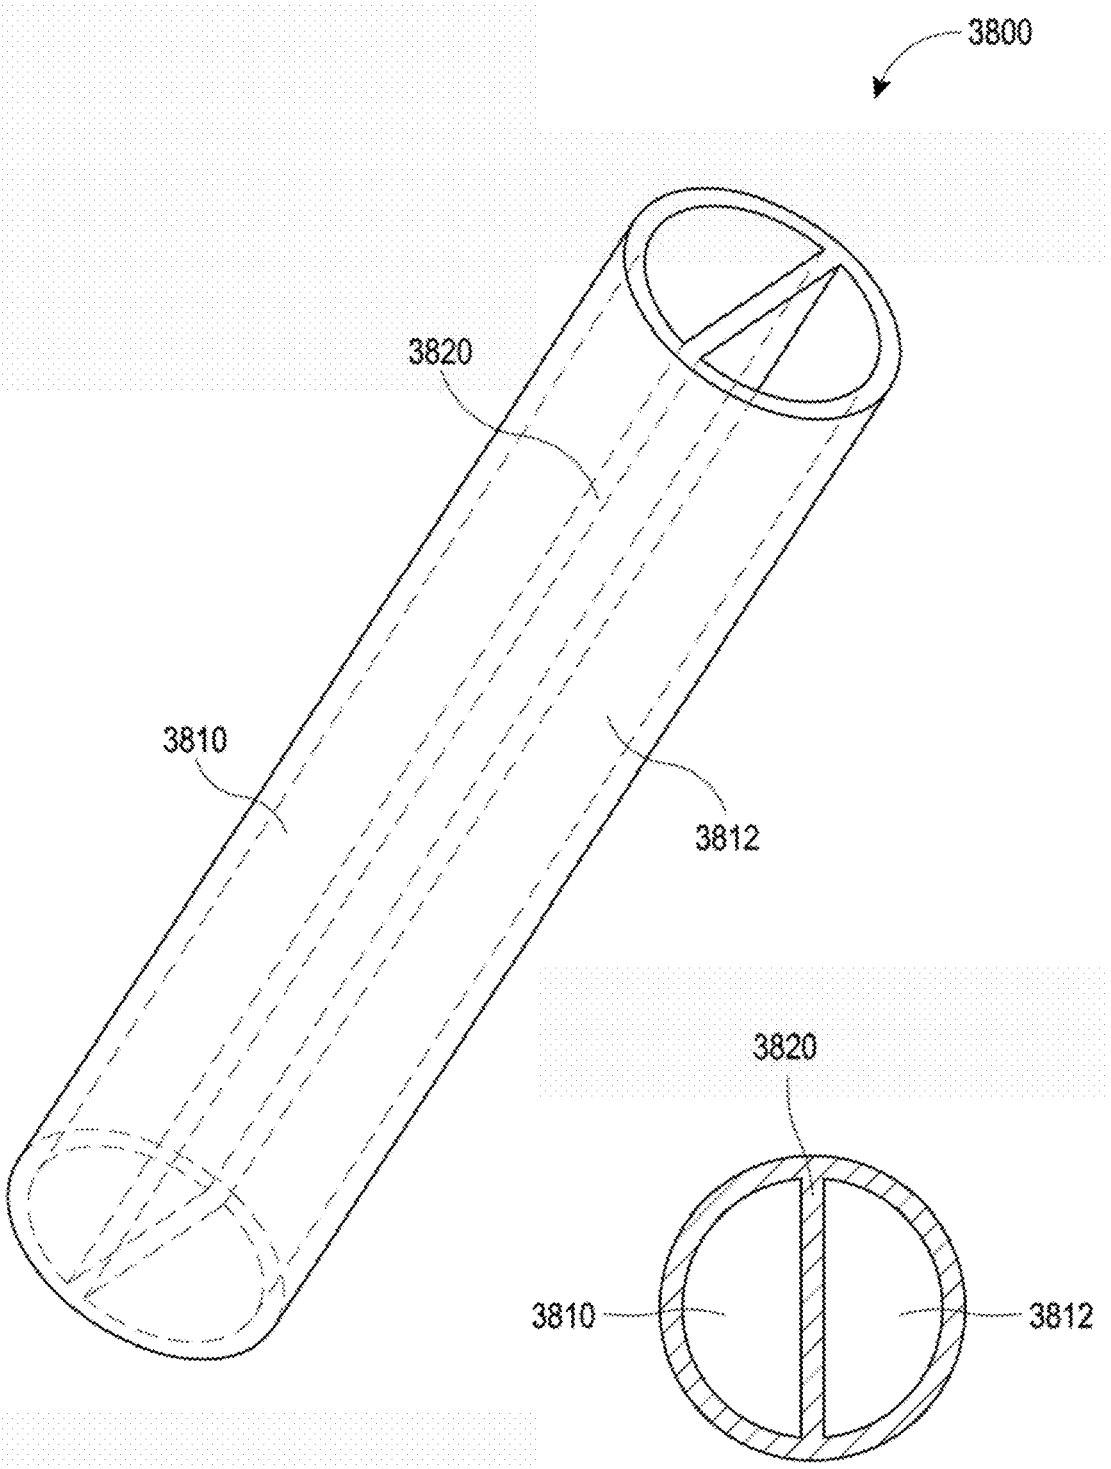


Fig. 106B

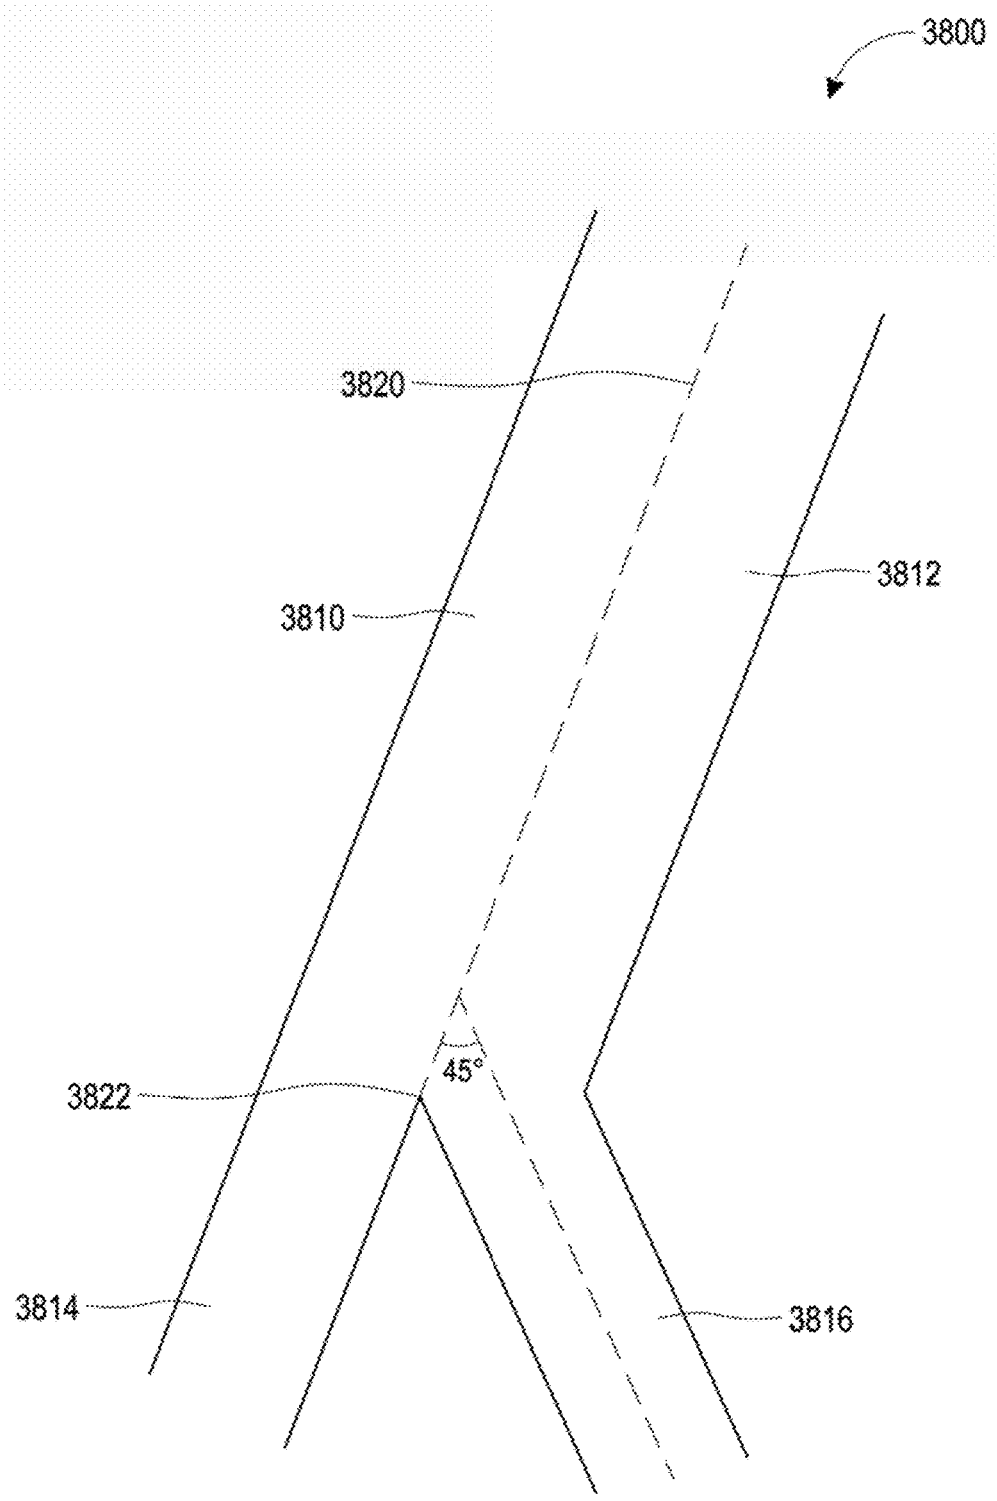


Fig. 106C

DEVICES AND METHODS FOR EXCLUDING THE LEFT ATRIAL APPENDAGE

CROSS-REFERENCE TO RELATED APPLICATIONS

[0001] This application is a continuation of U.S. patent application Ser. No. 16/782,871, filed Feb. 5, 2020, which claims the priority benefit of U.S. Provisional Patent Application No. 62/803,289, filed Feb. 8, 2019, the entire disclosure of which is hereby incorporated by reference herein in its entirety.

BACKGROUND

Field

[0002] This development relates generally to systems, devices and methods for excluding the left atrial appendage (LAA). In particular, systems, devices and methods for excluding the LAA using an expandable foam implant with a deployable and compliant frame are described herein.

Description of the Related Art

[0003] Atrial fibrillation (Afib) is a condition in which the normal beating of the left atrium (LA) is chaotic and ineffective. The left atrial appendage (LAA) is a blind pouch off the LA. In patients with Afib blood stagnates in the LAA facilitating clot formation. These clots (or clot fragments) have a tendency to embolize or leave the LAA and enter the systemic circulation. A stroke occurs when a clot/clot fragment embolizes and occludes one of the arteries perfusing the brain. Anticoagulants, e.g. Coumadin, have been shown to significantly reduce the stroke risk in Afib patients. These drugs reduce clot formation but also increase bleeding complications including hemorrhagic strokes, subdural hematoma, and bleeding in the gastrointestinal tract.

[0004] There are about eight million people in the US and EU with Afib. About 4.6 million of these patients are at a high risk for stroke and would benefit from anticoagulation. A large portion of these patients cannot take anticoagulants due to an increased bleeding risk, leaving their stroke risk unaddressed. The prevalence of Afib increases with age.

[0005] Existing devices for occluding the LAA have drawbacks. Existing devices are offered in many sizes and must be closely matched to the highly variable LAA anatomy. This is difficult to do using fluoroscopy and often requires adjunctive imaging in the form of transesophageal echocardiography (TEE), cardiac CT and MRI, all with three dimensional reconstructions. If the device is significantly oversized, the LAA ostium may become overstretched leading to tearing, resulting in bleeding into the pericardial space. If the device is too small, it will not adequately seal the ostium and may be prone to embolization. Even if sized correctly, the device forces the oval LAA ostium to take the round shape of the device, often resulting in residual leakage at the edges due to poor sealing.

[0006] Existing devices require sufficient spring force or stiffness to seal and anchor to surrounding tissue. If too stiff, these devices may lead to leaking of blood through the tissue into the pericardial space which may lead to cardiac tamponade. Furthermore, the geometry of these devices limits repositioning once the implant is fully expanded. Existing devices also complicate delivery by requiring positioning in the LAA coaxial to the axis of the LAA.

[0007] There is therefore a need for an improved LAA occlusion device.

SUMMARY

[0008] The embodiments disclosed herein each have several aspects no single one of which is solely responsible for the disclosure's desirable attributes. Without limiting the scope of this disclosure, its more prominent features will now be briefly discussed. After considering this discussion, and particularly after reading the section entitled "Detailed Description," one will understand how the features of the embodiments described herein provide advantages over existing systems, devices and methods for left atrial appendage (LAA) occlusion.

[0009] The following disclosure describes non-limiting examples of some embodiments. For instance, other embodiments of the disclosed systems and methods may or may not include the features described herein. Moreover, disclosed advantages and benefits can apply only to certain embodiments and should not be used to limit the disclosure.

[0010] Devices and methods are described for occluding the LAA (LAA) to exclude the LAA from blood flow to prevent blood from clotting within the LAA and subsequently embolizing, particularly in patients with atrial fibrillation. An LAA occlusion device is delivered via transcatheter delivery into the LAA and anchored using a compliant frame and foam body. The device conforms to the oval shape of the LAA with superior sealing effect, does not require an excessive number of sizes and thus negates the need for extensive pre-procedure imaging, and can be delivered off-axis thereby allowing for simpler delivery procedure, among other advantages.

[0011] A foam body, which can be tubular in shape, and a compliant frame inside or within the foam body, are described that are collapsed for delivery and then expand in place within the LAA. The foam body may have a coating at least partially on the outer surface(s) of the foam body. The coating may be a layer of Polytetrafluoroethylene (PTFE). The device is anchored by structural anchors of the frame and/or by tissue ingrowth from the left atrium (LA) and LAA into the foam. Some embodiments are additionally or alternatively anchored by independent or integrated repositionable anchors, by barbs, and/or by distal anchoring elements. For example, anchors extending from a compliant frame are described which deploy through the compressible foam plug. In some embodiments, repositionable atraumatic anchor system embodiments are also disclosed which can be independent structures or integral to the foam plug and/or skin.

[0012] The foam body may be at least partially covered by a proximal end cover. The cover may be an expanded Polytetrafluoroethylene (ePTFE) cover. The cover provides several advantages, such as the following: sufficiently strong to enable handling of the plugs without tearing; allow for repositioning and retrieval of the plugs; provides a thromboresistant surface within the LA which will encourage formation of a neointima; assist in the creation of occlusion zones designed to encourage thromboresistance and endothelialization from the blood and adjacent tissue and anchoring zones designed to promote fast and tenacious tissue ingrowth into the compressible implant from the adjacent non-blood tissue; and can assist in closure at the ostium. The cover, e.g. a layer, jacket or skin, etc., can be independent or can be attached to the foam body, for

example with sutures, adhesives, etc. In some embodiments, retrieval finials can be attached at one or more points to aid in retrieval of an embolized device and to increase radiopacity.

[0013] Some embodiments are tracked over a guidewire and have a guidewire lumen within the foam that is expandable, to allow for placement of the guidewire, and then is self-closing upon removal of the guidewire. Some embodiments do not require a guidewire lumen. Further, some embodiments may be multi-functional and include features for ablation, pressure-sensing, drug-elution, pacing, electrical isolation, etc.

[0014] In one aspect, a left atrial appendage occlusion device comprises a tubular foam body and a cover. The tubular foam body extends axially from a proximal end to a distal end. The cover includes at least a portion that covers the proximal end. The portion that covers the proximal end includes a series of openings therethrough. The foam and cover are configured to allow for a flow rate of water axially through the device of at least four liters per minute, with the water at about sixty-eight degrees Fahrenheit (F) and an upstream pressure of about twenty-five millimeters of Mercury (mmHg).

[0015] Various embodiments of the various aspects may be implemented. In some embodiments, the body may include a compressible side wall extending between the proximal end and the distal end and defines a central cavity. The left atrial appendage occlusion device may further comprise an expandable support coupled with the body and configured to compress the side wall against a wall of a left atrial appendage. The foam body may include a proximal face having an area, and the series of openings in the cover may collectively provide an open area that is at least five percent of the area of the proximal face. The open area may be at least ten percent of the area of the proximal face. The open area may be at least fifteen percent of the area of the proximal face. The flow of water may be along a flow axis, and the tubular foam body may extend axially along a device axis. The device axis may be angled with respect to the flow axis by at least thirty degrees. The device may be configured to allow for an off-axis flow rate of water through the device of at least four liters per minute, with the water at about sixty-eight degrees Fahrenheit (F) and an upstream pressure of about twenty-five millimeters of Mercury (mmHg). The off-axis flow may be at least thirty degrees from the axial flow.

[0016] In another aspect, a left atrial appendage occlusion device comprises a tubular foam body and a cover. The tubular foam body extends axially from a proximal end to a distal end. The cover includes at least a portion that covers the proximal end. The portion that covers the proximal end includes a series of openings therethrough. The foam body includes a proximal face at the proximal end having an area. The series of openings in the cover collectively provide an open area that is at least five percent of the area of the proximal face.

[0017] Various embodiments of the various aspects may be implemented. In some embodiments, the open area may be at least ten percent of the area of the proximal face. The open area may be at least fifteen percent of the area of the proximal face. The foam and cover may be configured to allow for a flow rate of water axially through the device of at least four liters per minute, with the water at about sixty-eight degrees Fahrenheit (F) and an upstream pressure

of about twenty-five millimeters of Mercury (mmHg). The body may include a compressible side wall extending between the proximal end and the distal end and define a central cavity. The left atrial appendage occlusion device may further comprise an expandable support coupled with the body and configured to compress the side wall against a wall of a left atrial appendage.

[0018] In another aspect, a method of loading a left atrial appendage occlusion device into a delivery catheter is described. The method comprises positioning a proximal end of a loading body adjacent a distal end of the delivery catheter, the loading body having a sidewall defining a channel therethrough with a distal opening at a distal end that is larger than a proximal opening at the proximal end. The method further comprises retracting the left atrial appendage occlusion device proximally through the loading body to thereby radially compress the device, the device comprising a foam body, and receiving the device into the distal end of the delivery catheter.

[0019] Various embodiments of the various aspects may be implemented. In some embodiments, the loading body may comprise a frustoconical portion. The loading body may define a central longitudinal axis, and the sidewall may extend at an angle of at least five degrees with respect to the longitudinal axis. The sidewall may extend at an angle of at least ten degrees with respect to the longitudinal axis. The sidewall may extend at an angle at least fifteen degrees with respect to the longitudinal axis. The sidewall may define a total angle of at least ten degrees, at least twenty degrees, or at least thirty degrees. The advancing step may comprise pulling a tether proximally through the delivery catheter. The device may be radially compressed within a delivery catheter having an outer diameter of no more than fifteen French. An inner surface of the loading body may be substantially smooth. The method may comprise radially compressing the device to a radial compressed width within the delivery catheter that is no more than twenty percent of a radially uncompressed width of the device. The radial compressed width within the delivery catheter may be no more than fifteen percent of the radially uncompressed width of the device.

[0020] In another aspect, a left atrial appendage occlusion device comprises a foam body, an expandable support and at least one anchor. The foam body has a tubular sidewall with a radial uncompressed thickness. The expandable support is coupled with the body. The at least one anchor is coupled with the support and extends through the sidewall when the foam of the sidewall is compressed, and where the at least one anchor has a radial height no greater than the radial uncompressed thickness of the sidewall.

[0021] Various embodiments of the various aspects may be implemented. In some embodiments, the device may define a central axis and the at least one anchor may be angled relative to the central axis. The at least one anchor may extend radially outward in a proximal direction at an angle of at least twenty degrees relative to a portion of the central axis that extends proximally to the device. The angle may be at least thirty degrees. The at least one anchor may extend through a radially-compressed portion of the sidewall having a radial thickness less than the radial uncompressed thickness. The left atrial appendage occlusion device may further comprise an attachment that connects the support to the sidewall and radially compresses the sidewall at the radially-compressed portion. The device may further com-

prise a proximal cover that covers at least a portion of a proximal face of the foam body.

[0022] In another aspect, a left atrial appendage occlusion device comprises a foam body, an expandable support and at least one anchor. The foam body has a tubular sidewall comprising at least one first portion having a first radial thickness and at least one second portion having a second radial thickness that is less than the first radial thickness. The expandable support is coupled with the body. The least one anchor is coupled with the support and extends at least partially through the at least one second portion of the sidewall.

[0023] Various embodiments of the various aspects may be implemented. In some embodiments, the device may define a central axis and the at least one anchor may be angled relative to the central axis. The at least one anchor may extend radially outward in a proximal direction at an angle of at least twenty degrees relative to the central axis. The angle may be at least thirty degrees. The at least one anchor may extend through the at least one second portion of the sidewall such that a portion of the at least one anchor extends outwardly beyond an outer surface of the at least one second portion of the sidewall. The at least one anchor may have a length equal to the radial uncompressed thickness of the tubular sidewall. The support may comprise a tubular frame portion configured to expand radially outward to compress the sidewall against a wall of a left atrial appendage after implantation of the device. The device may further comprise a proximal cover that covers at least a portion of a proximal face of the foam body.

[0024] In another aspect, a left atrial appendage occlusion device comprises a tubular foam body and an expandable support coupled with the body. The device is configured to insert into a non-cylindrical opening of a test body having a non-cylindrical profile, expand radially within the non-cylindrical opening, and conform to the non-cylindrical profile at least at the opening of the test body.

[0025] Various embodiments of the various aspects may be implemented. In some embodiments, the device may be configured to conform to the non-cylindrical profile at least at the opening of the test body and leave no radial gaps between the device and the test body opening that are greater than five millimeters. The device may leave no radial gaps that are more than four, three, two and/or one millimeter. The device may be configured to insert into a non-cylindrical opening of a test body having a non-cylindrical profile with a size and shape substantially similar to that of a native left atrial appendage. The device may be configured to insert into a non-cylindrical opening of a test body having a radial stiffness substantially similar to that of a native left atrial appendage and to assume a non-cylindrical profile at least at the opening of the test body after a period of at least thirty days, of at least sixty days, and/or of at least one hundred twenty days. The device may further comprise at least one anchor coupled with the frame and extending at least partially into the tubular foam body.

[0026] In some embodiments, the foam body may include a compressible side wall extending between a proximal end and a distal end and define a central cavity. The left atrial appendage occlusion device may further comprise an expandable support coupled with the foam body and configured to compress the side wall against an inner surface of the test body.

[0027] In another aspect, a left atrial appendage occlusion device comprises a tubular foam body and an expandable support coupled with the body. The device has a radial uncompressed width. The device is configured to compress radially to a radial compressed width that is no more than fifty percent of the radial uncompressed width.

[0028] Various embodiments of the various aspects may be implemented. In some embodiments, the radial compressed width may be no more than forty percent of the radial uncompressed width. The tubular foam body may extend along a longitudinal axis, and the radial uncompressed width may extend along a diameter of the foam body that is perpendicular to the longitudinal axis.

[0029] In another aspect, a left atrial appendage occlusion device comprises a tubular foam body and an expandable support coupled with the body. The device extends axially from a proximal end to a distal end, and the proximal end has a radial uncompressed width. The distal end is configured to compress radially to a radial compressed width that is no more than fifty percent of the radial uncompressed width of the proximal end.

[0030] Various embodiments of the various aspects may be implemented. In some embodiments, the distal end may be configured to compress radially to a radial compressed width that is no more than forty percent of the radial uncompressed width of the proximal end. The radial compressed width may be no more than thirty percent, no more than twenty percent, no more than ten percent, and/or no more than five percent, of the radial uncompressed width of the proximal end.

[0031] In another aspect, a left atrial appendage occlusion device comprises a tubular foam body and an expandable support coupled with the body. The device has an axial uncompressed length. The device is configured to compress axially to an axial compressed length that is no more than fifty percent of the axial uncompressed length.

[0032] Various embodiments of the various aspects may be implemented. In some embodiments, the axial compressed length may be no more than forty percent of the axial uncompressed length. The axial uncompressed length may extend from a proximal end of the foam body to a distal end of the foam body.

[0033] In another aspect, a left atrial appendage occlusion device is described. The device comprises a conformable, tubular foam body, a compressible side wall and an expandable support. The conformable, tubular foam body has a closed proximal end and a distal end. The compressible side wall extends between the proximal end and the distal end, and defines a central cavity. The expandable support is within the body and configured to compress the side wall against a wall of a left atrial appendage.

[0034] In some embodiments, the side wall may have an uncompressed thickness of at least about 0.5 mm. The compressible side wall may have an uncompressed thickness of at least about 1.5 mm. The compressible side wall may have an uncompressed thickness of about 2.5 mm. The compressible side wall may extend in a distal direction beyond a distal end of the support by at least about 2 mm in an unconstrained, expanded state. The compressible side wall may extend in a distal direction beyond a distal end of the support by about 5 mm in an unconstrained, expanded state. The compressible side wall may comprise a foam having a plurality of interconnected reticulations and voids, and further comprising a PTFE coating on at least some of

the interconnected reticulations. The closed proximal end may comprise a foam end wall. The foam end wall may further comprise a cover. The cover may comprise ePTFE. The expandable support may be self-expandable. The expandable support may be in the central cavity. The tubular foam body may be substantially cylindrical in an unconstrained, expanded state.

[0035] In another aspect, a self-expandable, atraumatic occlusion device is described. The device is configured to conform to the side wall of a left atrial appendage. The device comprises a compressible open cell foam body, a self-expandable support and a proximal end wall. The compressible open cell foam body has a tubular foam side wall and a central cavity. The expandable support is within the cavity. The proximal end wall is on the foam body. The proximal end wall is positioned proximally of the proximal end of the support, and the foam side wall extends distally beyond the distal end of the support to form a distal, atraumatic bumper for preventing contact between the support and a wall of the left atrial appendage in an implantation in which a central longitudinal axis of the occlusion device is non-parallel to a primary longitudinal axis of the left atrial appendage.

[0036] In another aspect, a left atrial appendage occlusion device is described. The device comprises an expandable tubular foam cup and an expandable frame. The expandable tubular foam cup has a proximal end, a distal end, a tubular side wall and a proximal end wall. The side wall has a thickness of at least about 1.0 mm and a porosity of at least about 85% open void content. The expandable frame is configured to press the side wall into conforming contact with a wall of the left atrial appendage.

[0037] In some embodiments, the tubular side wall may have a thickness of at least about 2 mm. The tubular side wall may have a void content of at least about 90%. The tubular side wall may have an average pore size of at least about 100 microns. The tubular side wall may have an average pore size of at least about 200 microns. The tubular side wall may be provided with a thromboresistant coating. The thromboresistant coating may comprise PTFE. The proximal end wall may be provided with a thromboresistant cover. The frame may further comprise at least three recapture struts inclining radially inwardly in the proximal direction to a hub. The frame may comprise a plurality of axially extending side wall struts, with adjacent pairs of side wall struts joined at an apex. The frame may comprise at least six proximally facing apexes and at least six distally facing apexes. Each recapture strut may be joined to a unique proximally facing apex on the frame. The recapture struts may be integrally formed with the frame. The device may further comprise a lumen through the hub. The device may further comprise anchors to secure the device to tissue. The anchors may be flexible anchors configured to extend through the foam side wall at an inclined angle.

[0038] In another aspect, a conformable LAA occlusion device is described. The device comprises a compressible tubular foam wall. The wall comprises a reticulated, cross linked matrix having at least about 90% void content, an average cell size within the range of from about 250-500 microns, a wall thickness of at least about 2 mm and a compressive strength of at least about 1 psi. In some embodiments, the compressive strength is within a range of from about 1 psi to about 2 psi. In some embodiments, the

device may have an expandable support configured to compress the side wall against a wall of a left atrial appendage.

[0039] In another aspect, a LAA occlusion device is described. The device includes an open cell foam body and an internal locking system. The body has a proximal end, a distal end and an outer skin. The proximal end is configured to face a left atrium and the distal end is configured to face the LAA following implantation in the LAA. The body can be compressed for delivery within a delivery catheter and can self-expand when removed from the delivery catheter. The internal locking system is coupled with the body and comprises at least one deployable tissue anchor. The deployable anchor is configured to deploy from a constrained configuration within the body to a deployed configuration where a tissue engaging segment of the anchor extends outside the body to secure the body within the LAA. The deployable anchor is configured to deploy to the deployed configuration after the body expands within the LAA. The deployable anchor may be retractable from the deployed configuration to a retracted configuration within the body.

[0040] In some embodiments, the internal locking system further comprises a plurality of the deployable anchors rotatably coupled with the body, wherein the plurality of anchors are configured to rotate to the deployed and retracted configurations. The internal locking system may comprise four of the deployable anchors. In some embodiments, the body further comprises a plurality of axially extending slots corresponding to the plurality of anchors, wherein each of the plurality of anchors is configured to deploy and retract through the corresponding axial slot.

[0041] In some embodiments, the internal locking system further comprises a restraint that restrains the anchor in the constrained configuration, and the anchor is deployed from the constrained configuration to the deployed configuration by removing the restraint from the anchor. The restraint may be a sheath that restrains the anchor in the constrained configuration by covering the anchor, wherein the anchor is deployed from the constrained configuration to the deployed configuration by removing the sheath from covering the anchor. The restraint may be a lasso that restrains the anchor in the constrained configuration by surrounding the anchor, and the anchor is deployed from the constrained configuration to the deployed configuration by removing the lasso from surrounding the anchor.

[0042] In some embodiments, the internal locking system further comprises a moveable mount coupled with an end of the anchor, and the anchor is deployed from the constrained configuration to the deployed configuration by axially moving the mount.

[0043] In some embodiments, the internal locking system further comprises a constraint configured to move over the anchor to cause the anchor to retract. The constraint may be a ring configured to slide over the anchor to cause the anchor to retract.

[0044] In some embodiments, the skin comprises ePTFE.

[0045] In some embodiments, the device further comprises at least one tissue ingrowth surface on a sidewall of the body.

[0046] In some embodiments, the device further comprises a plurality of openings in the skin to permit tissue ingrowth into the open cell foam body. The plurality of openings of the skin may be located in an anchoring region of the device located at least between the proximal and distal ends of the device, and the device may further comprise an

occlusion region located at the proximal end of the device and configured to encourage thromboresistance and endothelialization from the blood and adjacent tissue.

[0047] In another aspect, a LAA closure system is described. The system comprises a delivery catheter and a LAA occlusion device. The delivery catheter comprises an elongate flexible tubular body, having a proximal end and a distal end and at least one lumen extending therethrough. The LAA occlusion device is configured to be compressed within the delivery catheter and to self-expand upon deployment from the delivery catheter. The device comprises a self-expandable open cell foam body coupled with an internal locking system. The internal locking system comprises a deployable anchor configured to deploy from a constrained configuration to a deployed configuration after the body expands within the LAA and is configured to retract from the deployed configuration to a retracted position within the body.

[0048] In some embodiments, the system further comprises an axially movable deployment control extending through a lumen of the body, for deploying the deployable anchor. The system may further comprise an axially movable deployment control extending through a lumen of the body, for deploying the foam body from the distal end of the closure system. The internal locking system may further comprise a restraint that restrains the anchor in the constrained configuration, and the anchor is actively deployed from the constrained configuration to the deployed configuration by removing the restraint from the anchor using an axially movable deployment control extending through a lumen of the body. The internal locking system may further comprise a moveable mount coupled with an end of the anchor, and the anchor is actively deployed from the constrained configuration to the deployed configuration by axially moving the mount using an axially movable deployment control extending through a lumen of the body.

[0049] In another aspect, a method of excluding a LAA is described. The method comprises advancing a guidewire into the LAA, advancing a distal end of a delivery catheter over the guidewire and into the LAA, and deploying a LAA occlusion device from the distal end of the delivery catheter. The device comprises an expandable foam body coupled with an internal locking system having a deployable anchor, and the body expands within the LAA upon deploying from the distal end of the delivery catheter. The method further comprises actively deploying the deployable anchor after the body expands within the LAA. The deployable anchor is configured to retract from the deployed configuration to a retracted position within the body. In some embodiments, the method further comprises retracting the deployable anchor from the deployed configuration to the retracted position.

[0050] In another aspect, a LAA occlusion device is described. The device comprises an expandable foam body and an internal locking system. The body can be compressed for delivery within a delivery catheter and can self-expand when removed from the delivery catheter. The internal locking system is coupled with the body and comprises a deployable anchor configured to deploy from a constrained configuration within the body to a deployed configuration where the anchor extends outside the body to secure the body within the LAA. The body is configured to expand

upon removal from the delivery catheter, and the deployable anchor is configured to deploy to the deployed configuration after the body expands.

[0051] In another aspect, a LAA occlusion device is described. The device comprises an expandable foam body and an internal locking system. The body can be compressed for delivery within a delivery catheter and can self-expand when removed from the delivery catheter. The internal locking system is coupled with the body and comprises a deployable anchor configured to deploy from a constrained configuration within the body to a deployed configuration where the anchor extends outside the body to secure the body within the LAA. The deployable anchor is configured to retract from the deployed configuration to a retracted configuration within the body such that the body can be repositioned within the LAA.

[0052] In another aspect, a LAA occlusion device is described. The device comprises an expandable tubular frame, an expandable tubular foam layer and a tissue scaffold. The expandable tubular frame has a proximal end, a distal end and a central lumen. The expandable tubular foam layer is carried by the frame and has a thickness of at least about 0.5 mm. The emboli retention layer is carried by the frame and encloses the lumen at the proximal end.

[0053] In some embodiments, the foam layer may have a thickness of at least about 1 mm. The foam layer may have a thickness of at least about 2.5 mm. The foam layer may have a void content of at least about 80%. The foam layer may have a void content of at least about 90%. The foam layer may have an average pore size of at least about 100 microns. The foam layer may have an average pore size of at least about 200 microns. The foam layer may extend across the proximal end of the frame to form the tissue scaffold. The tissue scaffold may be provided with a thromboresistant coating. The tissue scaffold may be provided with a thromboresistant layer. The thromboresistant coating or layer may comprise PTFE. The thromboresistant coating or layer may comprise ePTFE. The frame may further comprise at least three recapture struts inclining radially inwardly in the proximal direction to a hub.

[0054] In some embodiments, the foam layer extends across the proximal end of the frame to form the tissue scaffold, and the frame may comprise a plurality of axially extending side wall struts, with adjacent pairs of side wall struts joined at an apex. The device may comprise at least six proximally facing apexes and at least six distally facing apexes. The device may comprise at least three recapture struts joined at a proximal hub, where each recapture strut has a distal end joined to the frame. Each recapture strut may be joined to a unique proximally facing apex on the frame. The recapture struts may be integrally formed with the frame. The device may further comprise a lumen through the hub.

[0055] In some embodiments, the device may comprise anchors to secure the device to tissue. The anchors may be static anchors that are configured to deploy upon deployment of the device from a delivery catheter. The anchors may be constrained anchors that are configured to be controllably released into a deployed configuration after expansion of the foam. The anchors may be dynamic anchors that are configured to be deployed from a contracted configuration to a deployed configuration and are further configured to be retracted from the deployed configuration back to a

retracted configuration. The anchors may be further configured to be retracted from the deployed configuration back to the contracted configuration.

[0056] In another aspect, a delivery system for deploying an implant is described. The system comprises an elongate flexible pusher, an implant, a hand piece, a tether, and a control. The elongate, flexible pusher has a proximal end, a distal end and at least one lumen extending therethrough. The implant is releasably carried on the distal end. The hand piece is on the proximal end. The tether extends from the hand piece through the lumen and is detachably connected to the implant. The control is on the hand piece for moving between a first, transvascular navigation configuration in which the implant is held by the tether in close proximity to the distal end of the pusher, and a second, test configuration in which the distal end of the pusher may be moved a distance away from the implant without changing the orientation of the implant, while the tether is still attached to the implant.

[0057] Various embodiments of the various aspects may be implemented. The distance may be at least about 5 mm. The distance may be at least about 1 cm. The tether may extend from the hand piece distally through the lumen, around a retainer in the implant and proximally back through the lumen to the hand piece. The retainer may be a pin, and the tether may be slidable around the pin. The tether may have a first end anchored to the hand piece, and a second end attached to a retraction mechanism. There may be a window on the hand piece where the tether is exposed. The implant may be a left atrial appendage occlusion device. There may be a second lumen extending axially through the pusher, between an open proximal end and an open distal end. A stiffening mandrel may be removably extending through the second lumen. An ICE catheter may be removably extending through the second lumen. The hand piece may comprise an inner body and an outer body, and the control may be configured to engage and disengage the inner and outer bodies.

[0058] In another aspect, a tether retraction system for releasing an implant from an implant pusher is described. The tether retraction system comprises an elongate, flexible pusher, an implant, a hand piece, a tether and a pulley. The elongate, flexible pusher has a proximal end, a distal end and at least one lumen extending therethrough. The implant is releasably carried on the distal end. The hand piece is on the proximal end. The tether has a first portion extending from an attachment point in the hand piece distally through the lumen, around a retainer in the implant and a second portion extending proximally back through the lumen to the hand piece. The pulley is in the hand piece. Severing the tether in the first portion to provide a severed end and proximally retracting a control on the hand piece by a distance causes the severed end to advance distally by at least about twice the distance.

[0059] In another aspect, a loader for loading an expandable implant into a deployment catheter is described. The loader comprises a housing, a reservoir, and a connector. The housing defines a tapered chamber having a small diameter proximal end and a large diameter distal end. The reservoir is in communication with the large diameter distal end, and has a floor, an annular side wall and an open top. The connector is on the proximal end, and is configured for connection to a distal end of a deployment catheter.

[0060] Various embodiments of the various aspects may be implemented. The loader may further comprise a plurality of ribs on a side wall of the tapered chamber. The connector may comprise a proximally extending tubular extension configured to insert into the distal end of the deployment catheter. The tubular extension may comprise a plurality of axially extending slots. The loader may further comprise an axially slidable tubular collar carried concentrically over the tubular extension. The tubular collar may be spaced apart radially from the tubular extension to form an annular space configured to receive the delivery catheter.

BRIEF DESCRIPTION OF THE DRAWINGS

[0061] The foregoing and other features of the present disclosure will become more fully apparent from the following description and appended claims, taken in conjunction with the accompanying drawings. Understanding that these drawings depict only several embodiments in accordance with the disclosure and are not to be considered limiting of its scope, the disclosure will be described with additional specificity and detail through use of the accompanying drawings. In the following detailed description, reference is made to the accompanying drawings, which form a part hereof. In the drawings, similar symbols typically identify similar components, unless context dictates otherwise. The illustrative embodiments described in the detailed description, drawings, and claims are not meant to be limiting. Other embodiments may be utilized, and other changes may be made, without departing from the spirit or scope of the subject matter presented here. It will be readily understood that the aspects of the present disclosure, as generally described herein, and illustrated in the drawing, can be arranged, substituted, combined, and designed in a wide variety of different configurations, all of which are explicitly contemplated and make part of this disclosure.

[0062] FIG. 1 shows the anatomy of the left atrium (LA) and left atrial appendage (LAA).

[0063] FIG. 2 shows an LAA with an embodiment of an LAA occlusion device implanted in the LAA and that uses adhesive.

[0064] FIG. 3 shows an x-ray image of an embodiment of an LAA occlusion device.

[0065] FIG. 4 shows an LAA with an embodiment of an LAA occlusion device and distal anchor implanted in the LA.

[0066] FIG. 5 shows an embodiment of a screw anchor that may be used with the various LAA occlusion devices described herein.

[0067] FIG. 6 shows a longitudinal cross section of an embodiment of an LAA occlusion device.

[0068] FIGS. 7-15 are sequential schematic cross section views of an embodiment of an LAA and delivery system showing delivery and anchoring techniques that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0069] FIG. 16 is a side cross section view of an embodiment of an LAA occlusion device having a foam body, frame and proximal cover.

[0070] FIG. 17 is a side cross section view of an embodiment of an LAA occlusion device having metal coils and foam.

[0071] FIG. 18 is a side view of an embodiment of an LAA occlusion device having a single metal coil.

[0072] FIG. 19 is a side view of an embodiment of an LAA occlusion device having a dilating distal tip.

[0073] FIG. 20 is a side cross section view of an embodiment of an LAA occlusion device having proximal and distal caps.

[0074] FIG. 21 is a schematic of an embodiment of an implant delivery system that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0075] FIG. 22 is a schematic of an embodiment of a delivery of an expanding foam system that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0076] FIG. 23 is a side view of a plug with barbs that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0077] FIG. 24 shows an embodiment of an LAA occlusion device having a retrieval suture attachment that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0078] FIGS. 25A-26 show embodiments of distal anchoring systems that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0079] FIGS. 27A-27G are various views of an embodiment of an LAA occlusion device with an internal locking system that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0080] FIGS. 28A-28D are various views of an embodiment of an internal locking system that may be used the device of FIGS. 27A-27G.

[0081] FIGS. 29A-29B are sequential side views of an unlocking mechanism that may be used with the device of FIGS. 27A-27G.

[0082] FIG. 30 is a side view of an embodiment of an LAA occlusion device having flexible anchors that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0083] FIGS. 31-32 are side views of an embodiment of an LAA occlusion device having flexible anchors and stiffening tubular members configuration that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0084] FIG. 33 is a side view of an embodiment of an LAA occlusion device having discrete attachments of an outer skin to an internal foam that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0085] FIG. 34 is a side view of the device of FIG. 34 including an outer rim.

[0086] FIG. 35 is a side view of an embodiment an LAA occlusion device having anchors with deployed V-tips that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0087] FIG. 36 is a side view of an embodiment an LAA occlusion device having deployed anchors with V-tips that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0088] FIGS. 37A-37C are side views of various embodiments of anchors that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0089] FIG. 38 is a side view of an embodiment of an LAA occlusion device implanted inside an LAA.

[0090] FIGS. 39A-39B are perspective views of an embodiment of a deployable anchor that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0091] FIGS. 40A-40B are perspective views of an embodiment of a deployable anchor that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0092] FIGS. 41A-41B are perspective views of an embodiment of a deployable anchor that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0093] FIGS. 42A-42D are various views of embodiments external deployable anchors that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0094] FIGS. 43A-43C are sequential side views of an embodiment of a deployment constraint that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0095] FIGS. 44A-44C are side views of an embodiment of an adjustable two stage anchor system that may be used with the various LAA occlusion devices described herein, including but not limited to the devices of FIGS. 85A-90D.

[0096] FIG. 45A is a cross-sectional view of an embodiment of an LAA occlusion device shown in an expanded configuration and having a foam cup body, proximal cover, and a deployable frame that includes a hub, recapture struts and a tubular body.

[0097] FIGS. 45B and 45C are, respectively, a distal end view and a proximal perspective view of the device of FIG. 45A.

[0098] FIG. 46 is a distal end view of the LAA occlusion device of FIG. 45A.

[0099] FIGS. 47A-47B are perspective and side views respectively of the LAA occlusion device of FIG. 45A having a single piece internal frame.

[0100] FIG. 48 is a perspective view of the device of FIG. 45A.

[0101] FIGS. 49-50 are side views of the device of FIG. 45A as attached to a delivery catheter shown, respectively, in embodiments of an expanded configuration and a partially collapsed configuration.

[0102] FIGS. 51-55 are schematics showing various embodiments of static barbs that may be used with the various occlusion devices described herein, such as the devices of FIG. 45A or 85A.

[0103] FIGS. 56-58 are schematics showing various embodiments of constrained barbs that may be used with the various occlusion devices described herein, such as the devices of FIG. 45A or 85A.

[0104] FIGS. 59-65 are schematics showing various embodiments of dynamic barbs that may be used with the various occlusion devices described herein, such as the devices of FIG. 45A or 85A.

[0105] FIGS. 66A-66C are side views of the implant of FIG. 45A having a proximal cover.

[0106] FIG. 67 shows side and end views of an embodiment of an implant having grappling hook anchors.

[0107] FIGS. 68A-68B are side and end views respectively of an embodiment of an implant having a thicker distal bumper.

[0108] FIG. 69 is a side view of an embodiment of an implant having a constrained anchor deployed in a secondary step.

[0109] FIGS. 70-72 depict embodiments of an implant having distal anchors and proximal speed bumps.

[0110] FIGS. 73-75 depict embodiments of an implant having distal loops.

[0111] FIGS. 76-77 depict embodiments of an implant having perfusion elements.

[0112] FIG. 78 is a side view of an embodiment of an LAA occlusion device having ablative features that may be incorporated with the various LAA occlusion devices described herein.

[0113] FIG. 79 is a side view of an embodiment of an LAA occlusion device having pressure-sensing features that may be incorporated with the various LAA occlusion devices described herein.

[0114] FIG. 80 is a side view of an embodiment of an LAA occlusion device having drug elution features that may be incorporated with the various LAA occlusion devices described herein.

[0115] FIG. 81 is a side view of an embodiment of an LAA occlusion device having pacing/defibrillatory features that may be incorporated with the various LAA occlusion devices described herein.

[0116] FIGS. 82-84 depict various systems and methods for electrically isolating the LAA that may be used with the various LAA occlusion devices described herein.

[0117] FIGS. 85A-85C are proximal, distal and side views, respectively, of an embodiment of an LAA occlusion device having a compressible foam body, an expandable frame, and a proximal cover.

[0118] FIG. 85D is a distal view of the embodiment of the LAA occlusion device of FIGS. 85A-85C additionally having an interior cover and proximal markers.

[0119] FIGS. 86A-86B are side and cross-section views, respectively, of the compressible foam body of FIGS. 85A-85C.

[0120] FIG. 86C is a cross-section view of the foam body of FIGS. 85A-85C with the expandable frame.

[0121] FIGS. 87A-87C are top perspective, side, and cross-section views of another embodiment of an LAA occlusion device.

[0122] FIGS. 87D-87E are side cross-section views of various embodiments of the LAA occlusion device of FIG. 85D.

[0123] FIG. 88A is a top view of an embodiment of a proximal cover shown in a flat configuration that may be used with the various LAA occlusion devices described herein.

[0124] FIGS. 88B-88C are top views of another embodiment of a proximal cover shown, respectively, in a flat configuration and assembled with an LAA occlusion device.

[0125] FIGS. 88D-88E are side and perspective views, respectively, of another embodiment of a proximal cover shown assembled with an LAA occlusion device.

[0126] FIGS. 89A and 89B are side perspective and proximal perspective views, respectively, of the frame of FIGS. 85B and 86C shown in a deployed configuration.

[0127] FIGS. 90A-90C are sequential proximal perspective views of an embodiment of a frame showing assembly of a cap and pin with the frame that may be used with the LAA occlusion devices of FIGS. 85A-88E.

[0128] FIG. 90D is a distal perspective view of the cap of FIGS. 90A-90C.

[0129] FIG. 91 is a side view of an embodiment of a loading system for loading the device of FIGS. 85A-88E into a delivery catheter.

[0130] FIG. 92A is a side view of a schematic of a transcatheter delivery system for delivering the device of FIGS. 85A-88E via an artery or vein.

[0131] FIGS. 92B-92C are proximal and distal perspective views, respectively, of the delivery system of FIG. 92A, showing an associated tether release mechanism and method.

[0132] FIGS. 93A and 93B are proximal and distal perspective views respectively of another embodiment of a tether release system that may be used with the device of FIGS. 85A-88E.

[0133] FIGS. 94A-94C depict various embodiments of an anchor/foam interface that may be used with the LAA occlusion devices of FIGS. 85A-88E.

[0134] FIG. 95A is a schematic showing an embodiment of a profile of an ostium and an LAA.

[0135] FIG. 95B is a schematic of the LAA occlusion devices of FIGS. 85A-88E as implanted in the ostium and LAA of FIG. 95A, illustrating the conforming capabilities of the devices.

[0136] FIG. 96A is a schematic of an LAA occlusion device illustrating the radial compression capabilities of the devices of FIGS. 85A-88E.

[0137] FIG. 96B is a schematic of an LAA occlusion device illustrating the axial compression capabilities of the device of FIGS. 85A-88E.

[0138] FIG. 97 is a plan view of an embodiment a laser cut tube frame shown in a flat configuration that may be used as the frame for the LAA occlusion devices of FIGS. 85A-88E.

[0139] FIGS. 98A-98C are various detail views of the frame of FIGS. 89A-90C indicating some of the structural aspects contributing to the LAA occlusion device's conformable capabilities.

[0140] FIGS. 99A-99B are top views of the device of FIGS. 85A-88E shown, respectively, in an uncompressed configuration and a compressed configuration.

[0141] FIGS. 100A-100C are data plots of test results showing various structural characteristics for certain embodiments of the device of FIGS. 85A-88E.

[0142] FIG. 101 is a schematic of an embodiment of a test setup that may be used to perform a flat plate test to characterize the stiffness and other structural attributes of the device of FIGS. 85A-88E.

[0143] FIG. 102 is a flow chart depicting an embodiment of a flat plate test method that may be performed with the test setup of FIG. 101 and the device of FIGS. 85A-88E.

[0144] FIGS. 103A and 103B are perspective and cross-section views, respectively, of an embodiment of a loading tool having guides, a locking connection for securing a catheter, and configured to hold fluid.

[0145] FIGS. 104A-104D are various views of an embodiment of a delivery catheter handle that may be used with the LAA implant and associated devices and systems described herein.

[0146] FIGS. 105A-105D are various views of an embodiment of a tether control switch or components thereof that may be used with the various LAA implant delivery handles, such as the handle of FIGS. 104A-104D, and associated devices and systems, described herein.

[0147] FIGS. 106A-106C show various views of various embodiments of dual lumen delivery catheter pushers that may be used with the various delivery systems and implants described herein.

[0148] While the above-identified drawings set forth presently disclosed embodiments, other embodiments are also contemplated, as noted in the discussion. This disclosure presents illustrative embodiments by way of representation and not limitation. Numerous other modifications and embodiments can be devised by those skilled in the art which fall within the scope and spirit of the principles of the presently disclosed embodiments.

DETAILED DESCRIPTION

[0149] The following detailed description is directed to certain specific embodiments of the development. In this description, reference is made to the drawings wherein like parts or steps may be designated with like numerals throughout for clarity. Reference in this specification to “one embodiment,” “an embodiment,” or “in some embodiments” means that a particular feature, structure, or characteristic described in connection with the embodiment is included in at least one embodiment of the invention. The appearances of the phrases “one embodiment,” “an embodiment,” or “in some embodiments” in various places in the specification are not necessarily all referring to the same embodiment, nor are separate or alternative embodiments necessarily mutually exclusive of other embodiments. Moreover, various features are described which may be exhibited by some embodiments and not by others. Similarly, various requirements are described which may be requirements for some embodiments but may not be requirements for other embodiments. Reference will now be made in detail to embodiments of the invention, examples of which are illustrated in the accompanying drawings. Wherever possible, the same reference numbers will be used throughout the drawings to refer to the same or like parts.

[0150] The devices and related methods are described herein in connection with use in occluding, i.e. excluding, a LAA (LAA). The various figures show various embodiments of LAA occlusion devices, systems and methods for delivery of the LAA occlusion devices, and/or methods of using the device to occlude a LAA. The various systems, devices and methods described herein may include the same or similar features and/or functionalities as other LAA occlusion systems, devices and methods as described, for example, in U.S. application Ser. No. 14/203,187 entitled “DEVICES AND METHODS FOR EXCLUDING THE LAA” and filed on Mar. 10, 2014, and/or as described in U.S. Provisional Application No. 62/240,124 entitled “DEVICES AND METHODS FOR EXCLUDING THE LAA” and filed on Oct. 12, 2015, the entire disclosure of each of which is incorporated herein by reference for all purposes and forms a part of this specification.

[0151] Some embodiments of an LAA occlusion device 3000 include a foam body 3002, a deployable and compliant frame 3040, and a proximal cover 3100, as primarily shown and described for example with respect to FIGS. 85A-90D.

Other features and functionalities that the device 3000 may include and employ are shown and described with respect to FIGS. 1-84 and 91-93B.

[0152] The heart 100 is shown in FIG. 1 with the left atrial appendage (LAA) 102, which is a cavity emanating from the left atrium (LA) 104. The LAA 102 is quite variable in shape in all dimensions. If the heart is not beating normally, a condition called atrial fibrillation, blood within the LAA becomes stagnant which promotes clot formation. If blood clots within the LAA, the clots may pass from the LAA 102 to the LA 104, to the left ventricle 106 and out of the heart 100 into the aorta. Vessels that bring blood to the brain branch off the aorta. If the clot passes to the brain via these vessels, it may get stuck and occlude a small vessel in the brain which then causes an ischemic stroke. Strokes have severe morbidities associated with them. The opening of the LAA 102 to the LA 104 is called an ostium 110. The ostium 110 is oval, highly variable and dependent on loading conditions, i.e., left atrial pressure. An object of the LAA occlusion devices described herein is to occlude the ostium 110 thereby sealing off the LA 104 from the LAA 102.

[0153] One embodiment of an LAA occlusion device is shown in FIG. 2. The occlusion device or plug 204 is placed within the LAA 200 at its opening to the LA 202. It is understood that the “plugs” described herein, such as the plug 204, may have the same or similar features as other implantable “devices” or “implants” described herein, such as the device 10, device 1020, device 3000, foam body 3002, etc., and vice versa. The plug 204 comprises an expandable media such as an open cell foam which enables collapse and expansion of the plug 204 and also to enhance ingrowth of tissue into the foam. The foam plug 204 is at least partially encapsulated within a thin strong layer 206 such as ePTFE (expanded polytetrafluoroethylene), polyolefin or polyester. The layer 206 may be referred to herein as a “skin” or “cover” and the like. Alternatively, bioabsorbable materials could be utilized such as PLA, PGA, PCL, PHA, or collagen. This thin encapsulating layer 206 can be oriented or otherwise modified to be elastomeric in at least one direction, such as radially. The layer 206 may have the same or similar features and/or functionalities as the cover 3100, and vice versa.

[0154] The plug 204 may be made of polyurethane, polyolefin, PVA, collagen foams or blends thereof. One suitable material is a polycarbonate-polyurethane urea foam with a pore size of 100 μm -250 μm or 250 μm -500 μm and 90-95% void content. The foam could be non-degradable or use a degradable material such as PLA, PGA, PCL, PHA, and/or collagen. If degradable, the tissue from the LAA will grow into the foam plug and replace the foam over time. The plug 204 may be cylindrical in shape in an unconstrained expansion, but it may also be conical for example with its distal end smaller than the proximal end or reversed. It could also be oval in cross section to better match the opening of the LAA.

[0155] The foam plug 204 is oversized radially in an unconstrained expansion to fit snugly into the LAA and may be 5-50 mm in diameter depending on the diameter of the target LAA. In a free, unconstrained state, the axial length “L” of the plug is less than its outer diameter “D” such that the L/D ratio is less than 1.0. In some embodiments, this ratio may be greater than 1.0. The compliance of the foam material is designed such that it pushes on the walls of the LAA with sufficient force to maintain the plug 204 in

place but without overly stretching the LAA wall. The foam and/or skin also conforms to the irregular surfaces of the LAA as it expands, to provide a complementary surface structure to the native LAA wall to further enhance anchoring and promote sealing. Thus, the expandable foam implant described herein conforms to the native configuration of the LAA. In one embodiment, the structure of the foam may be fabricated such that squeezing axially on the opposing ends of the foam causes the foam to increase in diameter.

[0156] The ePTFE or foam material may be provided with one or two or more radiopaque markers such as radiopaque threads **210** or be filled with or impregnated with a radiopaque filler such as barium sulfate, bismuth subcarbonate, or tungsten which permit the operator to see under x-ray the plug for proper positioning in the anatomy. An x-ray image is shown in FIG. 3 where one cannot see a foam plug **300** but can clearly see threads **302** and a crimp **304** (discussed below). This thread **302** or ribbon may be made from a radiopaque metallic wire or tube such as platinum, platinum-iridium or tungsten or a polymer with a radiopaque filler such as barium, bismuth, tantalum, tungsten, titanium or platinum.

[0157] An outer ePTFE layer may be formed from a tube with a diameter about the same diameter of the foam plug and a wall thickness between about 0.0001" and about 0.001" thick and serves to allow one to collapse and pull on the plug **204** without tearing the foam material. The ePTFE material also serves as the blood contacting surface facing the LA **206** and has pores or nodes such that blood components coagulate on the surface and an intimal or neointimal covering of tissue grows across it and anchors tightly to the material. Pore sizes within the range of from about 4 μ to about 110 μ , ideally 5-35 μ are useful for formation and adherence of a neointima.

[0158] The outer covering **206** may be constructed of materials other than ePTFE such as woven fabrics, meshes or perforated films made of FEP, polypropylene, polyethylene, polyester or nylon. The covering **206** should have a low compliance (non-elastic), at least longitudinally, be sufficiently strong as to permit removal of the plug, a low coefficient of friction, and be thromboresistant. The outer covering **206** serves as a matrix to permit plug removal as most foams are not sufficiently strong to resist tearing when pulled. The plug **204** can also be coated with or contain materials, such as PTFE. Such materials may enhance the plug's **204** ultrasonic echogenic profile, thromboresistance, and/or lubricity. The plug **204** can also be coated with or contain materials to facilitate echocardiographic visualization, promote cellular ingrowth and coverage.

[0159] The outer covering **206** has holes in it to permit contact of the LAA tissue with the foam plug **204** to encourage ingrowth of tissue into the foam plug pores and/or allow blood flow therethrough. These holes may be 1 to 5 mm in diameter or may also be oval with their long axis aligned with the axis of the foam plug, the length of which may be 80% of the length of the foam plug and the width may be 1-5 mm. The holes may be as large as possible such that the outer covering maintains sufficient strength to transmit the tensile forces required for removal. The holes may be preferentially placed along the device. In one embodiment, holes are placed distally to enhance tissue ingrowth from the LAA wall.

[0160] In one implementation, the implant is provided with proximal and/or distal end caps of ePTFE, joined

together by two or three or four or more axially extending strips of ePTFE. The axially extending strips are spaced apart from each other circumferentially, to provide at least two or three or four or more laterally facing windows through which the open cell foam body will be in direct contact with the tissue wall of the LAA. This outer covering could be a mesh or netting as well. As shown in FIG. 20, the covering **2004** is only on the proximal and distal faces of the plug **2000**. They may be glued to the foam plug and then crimped to the center tube **2002**.

[0161] The implantable plug **204** or devices **10**, **1020**, **3000** (as described below) may be anchored and secured in place in the LAA by tissue ingrowth and/or with additional anchoring features. In some embodiments, the plug **204** or devices **10**, **1020**, **3000** may be anchored by tissue ingrowth alone.

[0162] In some embodiments, other anchoring means may be implemented. One means of adhering the foam plug in place within the LAA is to use an adhesive, such as a low viscosity cyanoacrylate (1-200 cps). The adhesive is injected into place along the sidewall near the distal end of the foam plug **208**. Holes in the ePTFE covering permit the adhesive to interact between the foam plug **204** and the LAA wall **200**. Injection of the adhesive may be accomplished with several means, one of which is to inject through the catheter into the center lumen **212**. Passages **214** serve to guide the adhesive to the correct location. The distal end of the foam plug may be restricted at that time to prevent the adhesive from exiting the distal crimp **216**. Alternatively, FIG. 21 shows tubes **2104** that are pre-placed through the guide catheter **2102**, through the center lumen of the plug **2106** and bend backwards in the LAA to the distal end of the plug **2100**. These tubes **2104** pass all the way to the proximal end of the guide catheter **2102** where a fitting is attached to permit injection of the adhesive which then exits the small tubes **2104** at the desired location of the plug. These tubes are made of polyethylene, polypropylene or FEP so that the adhesive will not adhere to the tubes. The tubes **2104** are withdrawn after injection through the guide catheter out of the patient.

[0163] Other one part adhesives including aqueous cross linking adhesives, polyurethane, PEG, PGA, PLA, polycaprolactone or a lycine-derived urethane may be used. In addition, these adhesives may be made in two components such that one component is adherent to the foam and the second injected in vivo. Also, these two component adhesives may be injected simultaneously to mix in vivo to prevent fouling of injection tubes.

[0164] An alternative anchoring means for plug **400** or device **3000**, etc. is one or two or more distal anchors as shown in FIG. 4. A wire **404** is passed through a center lumen **410** into the LAA and attached to the distal wall of the LAA. In this case, a screw wire **408** is threaded into the wall of the LAA **406**. A closer detail of this is seen in FIG. 5 as screw **502** is shown embedded into the LAA wall **504** but not all the way through the epicardial surface **506**.

[0165] Additional means of anchoring include the use of a plurality of hooks or barbs or graspers to grab the distal wall and baskets, malecots, distal foam plugs and Nitinol wire birds nests that open within the LAA and push outward on the wall or engage the protrusions of the LAA. It may be desirable to place the plug then engage the anchor as a secondary step. One such embodiment could include a multitude of nitinol wires with a ball or catch welded

proximal to the anchor tip. These could be gathered with the delivery catheter then released when the ideal plug position has been confirmed.

[0166] A cross section of one embodiment is shown in FIG. 6 with foam plug 600 and the LA face 602 and the LAA face 610. The ePTFE material 604 encapsulates the foam plug 600 and its open ends are connected with an attachment structure such as a wire, suture or tubular crimp 606 over an inner tube 608. The inner tube 608 may be made of an implant grade stainless steel such as 304 or 316 grades or a cobalt-chromium alloy such as MP35n and the crimp 606 may be made of annealed 304 or 316 stainless steel or a cobalt-chromium alloy such as MP35n. This crimp also serves as an element which can be snared should the device need to be removed.

[0167] Referring to FIG. 6, the tubular ePTFE layer 604 extends along an inner layer 612 which lines the guidewire lumen, and everts out around the left atrial face 602 to form outer layer 614. In some embodiments, the layer 604 may cover the entire proximal face and/or part of the sidewall, such as the cover 3100 or the cover over proximal face 1064', as further described herein. As further shown in FIG. 6, a first end 616 of inner layer 612 is disposed concentrically within a second end 618 of outer layer 614. The first end 616 and second end 618 are clamped between inner tube 608 and outer crimp 606. In this manner, the implant can be encapsulated in a manner that presents a seamless left atrial face 602, and preserves the integrity of the guidewire lumen with inner tube 608.

[0168] An embodiment of a technique for placement of an LAA occlusion device is shown in FIGS. 7 through 15. To close the LAA, the LA is first accessed from the venous system. One approach is to use a Brockenbrough-style needle to puncture the atrial septum to access the LA from the right atrium (RA). The basic needle-puncture technique is performed obtaining venous access typically via the right femoral vein. A Mullins sheath and dilator are then tracked over a 0.025" or 0.032" guidewire previously placed in the superior vena cava (SVC). Fluoroscopic and echocardiographic imaging, such as transesophageal echo (TEE) or intracardiac echo (ICE), are typically utilized. If echo is not utilized, it is common to also place a pigtail catheter in the aortic root to define the location of the aortic valve, a step not necessary when using echo.

[0169] Once the Mullins sheath and dilator are in the SVC, the guidewire is removed and a trans-septal needle is placed through the dilator. The needle contains a stylette to prevent skiving off of polymeric material from the dilator lumen as it traverses to the tip. Once the needle is near the dilator tip, the stylette is removed and the needle is connected to a manifold and flushed. The Mullins sheath/dilator set and the needle (positioned within the dilator tip) are retracted into the SVC toward the RA as a unit. As the system is withdrawn down the wall of the SVC into the RA and positioned in the fossa ovale, the preferred puncture location.

[0170] Once proper position in the fossa ovale is observed, the needle is advanced across the fossa ovale into the LA. Successful trans-septal puncture can be confirmed by echo, pressure measurement, O₂ saturation and contrast injection. Once the needle position is confirmed to be positioned in the LA, the sheath and dilator can be advanced over it into the LA. In some cases, the user will first pass a guidewire through the needle into the LA and into an upper pulmonary vein (typically the left) prior to crossing. Alternative options

include the use of radiofrequency trans-septal needles, which are useful for crossing very thick or hypertrophic septa, or the use of a safety wire placed through the needle and utilized for the initial puncture.

[0171] Referring to FIGS. 8 through 15, a guide catheter 802 is placed through the femoral vein into the right atrium of the heart and across the intra-atrial septum into the LA as described above and positioned near the LAA ostium 804. A guidewire 902 usually of 0.035" diameter is placed through guide catheter 900 and into the LAA 904. This guidewire 1002 may have attached to its distal end a balloon 1006 which is inflated in the LAA and serves as a bumper to prevent guide catheter 1100 from perforating the wall of the LAA. The guide catheter 1100 is then advanced over the guidewire 1108 into the LAA 1104. A radiopaque marker 1102 is used to guide catheter placement under fluoroscopy.

[0172] The foam plug 1204 is then pushed through the guide catheter 1200 with pusher 1202 and is shown exiting the guide catheter 1300 slowly in FIG. 13 until it is fully deployed as shown in FIG. 14. The foam plug 1404 position may then be adjusted in place using the distal balloon 1408 and the guide catheter 1400, sliding the foam plug proximally by pulling on the balloon 1408 through shaft 1412 or sliding it distally by pushing guide catheter 1400 distally. The guidewire may also contain a pressure sensor within it such that sealing of the LAA is monitored and confirmation of a sufficient seal is made. Once the placement is satisfactory, the adhesive 1514 may be injected and/or mechanical anchors be deployed anchoring the plug 1404 to the wall. The guidewire balloon 1508 is deflated, after which the guidewire is removed. In an alternative embodiment, a binary adhesive system can be used where one component of the binary system is bonded to the outer surface of the skin covering the foam plug. The second component can be injected at the interface between foam plug and the wall of the LAA such that bonding happens only at the interface minimizing the risk of adhesive embolization. In some embodiments, adhesives and balloons may or may not be used, for example with the device 3000 further described herein.

[0173] An alternative to pushing the plug through the entire length of the guide catheter is that the plug 1204 may be initially located at the distal end of the guide catheter 1200 as shown in FIG. 12. The guidewire 1210 passes through the center of the plug 1204 and in this mode, the pusher 1202 only needs to push the plug a short ways to deploy it into the LAA.

[0174] For alternative anchors, they may be deployed, the shafts disconnected and removed. Disconnection mechanisms may be any of several types, such as threaded, electrolytic detachment, or others known in the art. In some embodiments, a suture attachment may be implemented, for example as described with respect to FIG. 24.

[0175] As shown in FIG. 16, in some embodiments, a foam body 1600 and metal frame such as stent 1602 may be included. The foam body 1600 and stent 1602 may have the same or similar features and/or functionalities as respectively the foam body 3002 and tubular body 3080 (see FIGS. 85A-90D), and vice versa. The foam 1600 is designed to provide ingrowth of tissue and also to provide a cushion of the metal stent 1602 onto the tissue of the LAA. The proximal face 1604' of the plug is covered in ePTFE,

polyester or another thromboresistant tissue scaffold material to facilitate sealing with the desired pore size to encourage overgrowth.

[0176] The stent **1602** may be made of Nitinol to enable it to pack into a 10, 12, 14, 16, 18 or 20 F delivery catheter and expand to its desired diameter. The stent **1602** may be braided, laser cut or wire formed. Any of a variety of stent wall patterns may be utilized, depending upon the desired performance. The stent **1602** may be a balloon expandable stent, or self-expandable stent. In the illustrated embodiment, the self-expandable stent **1602** comprises a plurality of proximal apices **1608** and distal apices **1610** connected by a plurality of zig zag struts **1612**. A hole **1606** allows passage of the guidewire for delivery. This design may be advantageous in that the expansion force exerted by the plug on the LAA can be controlled separately from the foam characteristics. Also, it may be easier to pack this concept into a smaller geometry. For example, the plug can be packed into a smaller geometry by reducing the amount of foam that must be compressed into the delivery catheter while maintaining sufficient dilation force.

[0177] Alternatively, the foam plug may be constructed of two foams. One denser core to provide force, for example radial force, and an outer softer foam to engage the tissue irregularities. The softer foam could also be located on the proximal and/or distal ends to facilitate retrieval.

[0178] Another means of adding stiffness to the foam plug is shown in FIG. 17 where a cavity **1704** in the foam plug **1700** is made and a coil of wire **1702** may be advanced from the guide catheter at the proximal end **1706** into the cavity **1704**. As the wire enters the cavity, it expands to its predetermined size and exerts force on the foam radially outwards. The type and amount of wire may be determined in vivo using x-ray guidance to examine the radial expansion of the foam into the LAA.

[0179] Instead of wires as shown in FIG. 17, a balloon may be passed into the foam and inflated to provide radial force while the outer foam serves to engage the tissue irregularities and tissue ingrowth. Following inflation, the balloon may be detached from a deployment catheter and the deployment catheter withdrawn. The balloon is preferably provided with a valve, to prevent the escape of inflation media. Inflation media may be any of a variety of media which is convertible between a first, flowable state and a second, hardened state such as by cross linking or polymerization in situ.

[0180] Another LAA plug is shown in FIG. 18 as a spring like implant wire **1800** that is covered with foam **1802** to encourage ingrowth. The proximal face of the implant is covered with a sheet of ePTFE or other tissue scaffolding material. This implant may be stretched out for delivery and released in place.

[0181] Rather than using a foam, a low porosity outer bag without perforations could be placed in the LAA and then filled with a substance to provide the radial expansion. This substance may be a hydrogel, cellulose or polyvinylacetate.

[0182] Rather than requiring the use of a separate dilation device to cross the septum, the distal crimp element **1902** may be formed in a tapered manner such that it extends from the distal end of the catheter **1200** and serves as a dilating tip to dilate the opening in the septum as the catheter is advanced. See FIG. 19.

[0183] An alternative plug design uses a foam such as cellulose sponge material that is compacted and dehydrated

such that it can be packed into the guide catheter. This foam material **2202** may be packed into the guide catheter as shown in FIG. 22. The foam plug **2202** is then advanced from the distal end of the guide catheter **2204** with a plunger **2206** into the LAA. The plug exits the guide catheter and opens to a disc shape **2210**. As the foam absorbs fluid in the blood, its length expands to form a cylinder **2220** filling the LAA. Expansion ratios for compressed cellulose materials may be as high as 17:1, expanded to compressed length.

[0184] It may be advantageous to use small barbs **2302** in FIG. 23 to further engage the plug **2204** into the LAA. Barbs may be unidirectional or bidirectional to resist movement in either the proximal or distal direction. These barbs are embedded into the foam plug and may be 0.1 to 1 mm in height. It may be desirable to place the plug then engage the barbs as a secondary step. One such embodiment could include a multitude of nitinol barb wires with a ball or catch welded proximal to the barb tip. These could be gathered with the delivery catheter within a sleeve or suture then released when the ideal plug position has been confirmed.

[0185] One means of removing a device that is not functioning properly is to releasably attach a retrieval suture **2400** to the implant, such as to the proximal cap **2402** which also passes proximally throughout the entire length of the guide catheter **2404** in FIG. 24. If the device is to be removed, pulling on both ends of the suture **2400** will pull the outer covering into the guide catheter **2404** which can then be removed from the patient. If the device is properly placed, the suture **2400** may be cut and removed leaving the plug in place.

[0186] Deployment of the occlusion device has been discussed primarily in the context of a transvascular access. However, the implants may alternatively be deployed via direct surgical access, or various minimally invasive access pathways (e.g. jugular vein). For example, the area overlying the xiphoid and adjacent costal cartilage may be prepared and draped using standard techniques. A local anesthetic may be administered and skin incision may be made, typically about 2 cm in length. The percutaneous penetration passes beneath the costal cartilage, and a sheath may be introduced into the pericardial space. The pericardial space may be irrigated with saline, preferably with a saline-lidocaine solution to provide additional anesthesia and reduce the risk of irritating the heart. The occlusion device may thereafter be introduced through the sheath, and through an access pathway created through the wall of the LAA. Closure of the wall and access pathway may thereafter be accomplished using techniques understood in the art.

[0187] Depending upon the desired clinical performance, any of the LAA occlusion devices described herein may be provided with a drug or other bioactive agent, which may be injected via the deployment catheter, or impregnated within the open cell foam or coated on the implant. The bioactive agent may be eluted or otherwise released from the implant into the adjacent tissue over a delivery time period appropriate for the particular agent as is understood in the art. Useful bioactive agents can include those that modulate thrombosis, those that encourage cellular ingrowth, through-growth, and endothelialization, and potentially those that resist infection. For example, agents that may promote endothelial, smooth muscle, fibroblast, and/or other cellular growth into the implant including collagen (Type I or II), heparin, a combination of collagen and heparin, extracellular matrix (ECM), fibronectin, laminin, vitronectin, peptides or

other biological molecules that serve as chemoattractants, molecules MCP-1, VEGF, FGF-2 and TGF-beta, recombinant human growth factors, and/or plasma treatment with various gases.

[0188] Anti-thrombotics can typically be separated into anti-coagulants and anti-platelet agents. Anti-Coagulants include inhibitors of factor(s) within the coagulation cascade an include heparin, heparin fragments and fractions as well as inhibitors of thrombin including hirudin, hirudin derivatives, dabigatran, argatroban and bivalrudin and Factor X inhibitors such as low molecular weight heparin, rivaroxaban, apixaban.

[0189] Antiplatelet agents include GP 2b/3a inhibitors such as epifibitide, and abciximab, ADP Receptor agonists (P2/Y12) including thienopyridines such as ticlopidine, clopidogrel, prasugrel and tacagrelor and aspirin. Other agents include lytic agents, including urokinase and streptokinase, their homologs, analogs, fragments, derivatives and pharmaceutical salts thereof and prostaglandin inhibitors.

[0190] Antibiotic agents can include, but are not limited to penicillins, cephalosporins, vancomycins, aminoglycosides, quinolones, polymyxins, erythromycins, tetracyclines, chloramphenicols, clindamycins, lincomycins, sulfonamides, their homologs, analogs, derivatives, pharmaceutical salts and combinations thereof.

[0191] Biologic agents as outlined above maybe be added to the implant 204 and may be injected through the delivery catheter into the space between the proximal cap 206 and the foam plug 204. This may serve as a reservoir to minimize thrombus formation during the initial implantation and reduce the need for systemic anticoagulation following device implantation.

[0192] An electronic pressure sensor may be embedded into the proximal end of the foam plug which may be used to transmit LA pressure to a remote receiver outside the body for the monitoring of LA pressure which is useful to monitor cardiac function. In addition, a cardiac pacer or defibrillator may be embedded into the foam plug and attached electrically to the distal anchor. A drug delivery reservoir may be embedded with connection to the LA for controlled delivery of biologic agents as outlined above.

[0193] Another means of anchoring is shown in FIG. 25A where the foam plug 2500 is placed in the LAA. The distal screw lead 2502 is advanced and screwed into the LAA wall. Guide 2506 is pulled proximally as shown in FIG. 25B. When this guide 2506 is pulled back, the screw lead wire, made of Nitinol, bunches up into a "birds nest" 2508 or forms a coil inside the foam plug 2500. The screw lead wire 2502 is pushed distally from the guide catheter 2504 with a pusher 2510 and continues to bunch up into the foam. The catheter system 2504, 2506 and 2510 are then removed.

[0194] Another means of anchoring the distal anchor element to the foam is shown in FIG. 26. Two barbed leads 2604 are attached to anchor 2602 such that when advanced into place in the foam plug 2600, the barbs 2604 dig into the foam plug.

[0195] FIGS. 27A-27G are various views of an embodiment of a device 10 for occlusion of the LAA (LAA). The device 10 may include the same or similar features as other devices for occlusion of the LAA described herein, such as the plug 204, device 1020, device 3000, etc., and vice versa. The device 10 includes an internal locking system 101 for securing the device 10 within the LAA. In some embodi-

ments, the device 10 may not include the internal locking system 101 or other anchoring features, for example the device 10 may be anchored by tissue ingrowth alone. The occlusion device 10 comprises an expandable media such as an open cell foam body 15, for example a plug. The body 15 enables collapse and expansion of the device 10 and also enhances ingrowth of tissue into the foam.

[0196] The body 15 of the device 10 shown in FIG. 27A through FIG. 27F is in its expanded configuration. The body 15 is in a compressed configuration in FIG. 27G. The device 10 includes the foam body 15, a skin 20, a central lumen 25, a finial 30, and a dynamic internal locking system 101 which anchors the device 10 within the LAA. FIG. 27A is a side cross-section view of the device 10 showing the body 15 and the internal locking system 101 in a deployed configuration. FIG. 27B is an end view of the proximal end of the device 10 showing the body 15 and the internal locking system 101 in a deployed configuration. FIG. 27C is a side view of the device 10 showing the body 15 and the internal locking system 101 in a deployed configuration. FIG. 27D is a side cross-section view of the device 10 showing the body 15 in a deployed configuration and the internal locking system 101 in a constrained configuration. FIG. 27E is an end view of the distal end of the device 10 showing the body 15 and the internal locking system 101 in a deployed configuration. FIG. 27F is a cross-section view of the device 10 taken along the line 1F-1F as shown in FIG. 27C. FIG. 27G shows the body 15 and internal locking system 101 loaded and compressed within a delivery sheath 1. The device 10 may be delivered via a delivery catheter in the configuration shown in FIG. 27G. The body 15 of the device 10 may then expand with the internal locking system 101 still constrained, as shown in FIG. 27D. The internal locking system 101 may then deploy into the deployed configuration as shown in FIG. 27A.

[0197] FIG. 27G shows the body 15 and internal locking system 101 loaded and compressed within an embodiment of a delivery sheath 1. In some embodiments, the delivery sheath 1 may be an outer delivery catheter. The body 15 and internal locking system 101 are loaded and compressed within a delivery catheter 5. The device 10 may be entirely or partially inside the delivery catheter 5. In some embodiments, the delivery catheter 5 may be an inner delivery catheter. The device 10 may be loaded and compressed with the delivery catheter 5 inside of the delivery sheath 1. Removing the delivery sheath 1, for example by retracting the delivery sheath 1 in the proximal direction, may allow the body 15 of the device 10 to expand. The body 15 expands while the internal locking system 101 is still constrained, for example by the delivery catheter 5. FIG. 27D shows the body 15 in its deployed state, with the internal locking system 101 in a constrained configuration within the delivery catheter 5. This demonstrates the first step in the deployment process, specifically placement of the device 10 within the LAA where the body 15 is expanded and the internal locking system 101 is constrained and thus the anchors are not deployed. The second step of the deployment process is shown in FIG. 27A where the internal locking system 101 has been deployed through the body 15. In some embodiments, this second step is reversible to retract the anchors, for example if placement of the device 10 within the LAA is unacceptable. The internal locking system 101, for example an anchoring component or system as further described herein, is deployed from within the body

15 to deploy at least one and in some implementations at least 2 or 4 or 6 or more anchors of the internal locking system **101** outside the body **15** to engage adjacent anatomy of the LAA.

[0198] The internal locking system **101** may be controllably deployed a period of time after the body **15** expands. For instance, the location, orientation, etc. of the device **10** may be verified with various imaging techniques such as by fluoroscopy with injection of contrast media via the central lumen before the internal locking system **101** is deployed and the anchors secure the device **10** within the LAA. In some embodiments, even after deployment of the internal locking system **101** and anchors thereof, the anchors may be retracted to a position within the body **15** for repositioning, and/or retrieval of the device **10** from, within the LAA.

[0199] FIG. 27F shows an embodiment of the device having slots **17**. The slots **17** are formed within the foam body **15**. For instance, material of the foam body **15** may be removed to facilitate deployment of the internal locking system **101**, such as outward expansion of anchors to engage the tissue.

[0200] The device **10** may have any or all of the same or similar features and/or functionalities as the other plugs described herein, for example the plug **204**, etc. For example, the device **10** is at least partially encapsulated within the skin **20**. In some embodiments, the skin **20** may cover the proximal end of the body **15**. The skin **20** may be a thin, strong outer layer. The skin **20** may be a thin, encapsulating layer. The skin **20** may be fabricated from ePTFE (expanded polytetrafluoroethylene), polyolefin, polyester, other suitable materials, or combinations thereof. In some embodiments, the skin **20** may be fabricated from bioabsorbable materials, for example polylactic acid (PLA), Polyglycolic acid (PGA), polycaprolactone (PCL), PHA, collagen, other suitable bioabsorbable materials, or combinations thereof. The skin **20** can be oriented or otherwise modified to be elastomeric in at least one direction, such as radially.

[0201] The body **15** may be made of polyurethane, polyolefin, PVA, collagen foams or blends thereof. One suitable material is a polycarbonate-polyurethane urea foam with a pore size of 100-250 μm and 90-95% void content. The body **15** may be non-degradable or use a degradable material such as PLA, PGA, PCL, PHA, and/or collagen. If degradable, the tissue from the LAA will grow into the foam body **15** and replace the foam over time. The body **15** may be cylindrical in shape in an unconstrained expansion, but it may also be conical with its distal end smaller than the proximal end, or vice versa. The body **15** may also be oval in cross section to better match the opening of the LAA.

[0202] The device **10** is oversized radially in an unconstrained expansion to fit snugly into the LAA. The device **10** may be 5-50 millimeters (mm) and generally at least about 10 mm or 15 mm in diameter in its unconstrained configuration, for example depending on the diameter of the target LAA. The length "L" of the device **10** may be less than, similar to or greater than its diameter "D" such that the L/D ratio is less than 1.0, about or greater than about 1.0, greater than about 1.5, or greater than about 2.0. The L/D ratio may be greater than 1.0 to maximize its stability. However, in some embodiments, the L/D ratio may be less than 1.0, for example, from about 0.2 to about 0.9, or from about 0.3 to about 0.8, or from about 0.4 to about 0.6. The compliance of the material of the device **10** is designed such

that it pushes on the walls of the LAA with sufficient force to maintain the plug in place but without overly stretching the LAA wall. The foam body **15** and/or skin **20** also conforms to the irregular surfaces of the LAA as it expands, to provide a complementary surface structure to the native LAA wall to further enhance anchoring and promote sealing. Thus, the expandable foam body **15** conforms to the native irregular configuration of the LAA. In some embodiments, the structure of the foam body **15** may be fabricated such that axial compression on the opposing ends of the body **15** such as by proximal retraction of a pull wire or inner concentric tube causes the foam to increase in diameter.

[0203] The body **15** and/or skin **20**, for example the foam material and/or ePTFE, may be provided with one, two or more radiopaque markers, such as radiopaque threads **210** (see FIG. 2) or filled with or impregnated with a radiopaque filler such as barium sulfate, bismuth subcarbonate, or tungsten, which permit the operator to visualize under x-ray the device **10** for proper positioning in the anatomy. Visualization of the device **10** may be used to verify the position of the device **10** before deployment of anchors to secure the device **10** in place.

[0204] The skin **20**, such as an outer ePTFE layer, may have a thickness between about 0.0001 inches and about 0.0030 inches. In some embodiments, the thickness of the skin **20** may be between about 0.0003 inches and about 0.0020 inches. In some embodiments, the thickness of the skin **20** may be between about 0.0005 inches and about 0.0015 inches. The thickness of the skin **20** may be uniform, for example the same or approximately the same no matter where the thickness is measured. In some embodiments, the thickness of the skin **20** may be non-uniform, for example the thickness may be different in different portions of the skin **20**.

[0205] The skin **20**, such as an outer ePTFE layer, may also serve as the blood contacting surface on the proximal end of the device **10** facing the LA. The skin **20** may have pores or nodes such that blood components coagulate on the surface and an intimal or neointimal covering of tissue grows across it and anchors tightly to the skin material. Pore sizes may be within the range of from about 4 μm to about 110 μm . In some embodiments, the pore sizes are within the range of from about 30 μm to about 90 μm . In some embodiments, the pore sizes are within the range of from about 30 μm to about 60 μm . Such ranges of pore sizes are useful for formation and adherence of a neointima. In some embodiments, the skin **20**, such as an outer ePTFE layer, may be formed from a tube with a diameter about the same diameter of the foam body **15**. and allows one to collapse and pull on the body **15** without tearing the foam material.

[0206] The skin **20** may be constructed of materials other than ePTFE such as woven fabrics, meshes or perforated films made of FEP, polypropylene, polyethylene, polyester or nylon. The skin **20** may have a low compliance (e.g. non-elastic), for instance a low compliance longitudinally, may be sufficiently strong as to permit removal of the plug, may have a low coefficient of friction, and/or may be thromboresistant. The skin **20** serves as a matrix to permit plug removal as most foams are not sufficiently strong to resist tearing when pulled. The body **15** can also be coated with or contain materials to enhance its ultrasonic echogenic profile, thromboresistance, lubricity, and/or to facilitate echocardiographic visualization, promote cellular ingrowth and coverage.

[0207] The skin 20 may include holes to permit contact of the LAA tissue with the foam body 15. Exposure of the foam body 15 to the LAA or other tissue has benefits for example encouraging ingrowth of tissue into the foam plug pores and/or increasing friction to hold the body 15 in place. These holes may be 1 to 5 mm in diameter or may also be oval with their long axis aligned with the axis of the foam plug, the length of which may be 80% of the length of the foam plug and the width may be 1-5 mm. The holes may be as large as possible such that the outer covering maintains sufficient strength to transmit the tensile forces required for removal. The holes may be preferentially placed along the device 10. In some embodiments, the holes are placed distally to enhance tissue ingrowth from the distal LAA wall.

[0208] In some embodiments, the device 10 includes an occlusion region and anchoring region. The proximal portion of the device 10 facing the LA after the device is implanted in the LAA may include the occlusion region. The occlusion region may be a blood contacting surface on the proximal end of the device 10 that is thromboresistant while promoting formation of a neointima at the occlusion region. The occlusion zone encourages thromboresistance and endothelialization from the blood and adjacent tissue. The anchoring zone promotes fast and tenacious tissue ingrowth into the device 10 from the adjacent non-blood tissue. The anchoring zone may be lateral surfaces of the device 10 that interface with tissue adjacent and/or within the LAA. The anchoring zone can also include the distal end of the device 10 that faces the distal wall of the LAA after implantation.

[0209] FIGS. 28A-28D are various views of an embodiment of an internal locking system 101 that may be used with the device 10. In some embodiments, multiple internal locking systems 101 may be used with the device 10. FIG. 28A is a side view of the internal locking system shown in a deployed configuration. FIG. 28B is an end view of a distal end of the internal locking system 101 in a deployed configuration. FIG. 28C is a side view of the internal locking system 201101 in a constrained configuration. FIG. 28D is a side view of an embodiment of an anchor 120 of the internal locking system 101.

[0210] Any of a variety of structures may be utilized as the dynamic internal locking system 101 with the device 10. In general, at least about two or four or six or more tissue anchors 120 may be actively or passively advanced from the implantable device 10 into adjacent tissue surrounding the implantation site. Following deployment of the device 10 and expansion of the body 15, a tissue engaging segment 121 of the tissue anchor 120 will extend beyond the skin by at least about one, and in some implementations at least about two or four 4 mm or more. The tissue engaging segment 121 is carried by a support segment 122 of the tissue anchor 120 which extends through the foam body 15, and may be attached to a deployment control such as a pull wire, push wire, tubular support or other control structure depending upon the desired configuration.

[0211] The locking system 101 discussed primarily herein is a passive deployment construction. Removal of a constraint allows the tissue anchors 120 to laterally self-expand to deploy into adjacent tissue. Self-expansion may be accomplished by constructing the tissue anchor 120 using nitinol, Elgiloy, stainless steel or other shape memory or spring bias materials. The constraint may be removed by proximal retraction or distal advance until the tissue anchors

120 are no longer engaged by the constraint, depending upon the construction of the locking system 101.

[0212] Alternatively, tissue anchors 120 may be deployed actively such as by distal advance, proximal retraction or rotation of a control, or inflation of a balloon positioned within the device 10 to actively drive the anchors 120 through the skin 20 or corresponding apertures on the skin 20 and into tissue. For example, a plurality of support segment 122, such as struts, may be joined at a distal end to a central hub 111, and incline radially outwardly in the proximal direction. Proximal retraction of the hub 111 will cause the tissue engaging segment 121 to advance along its axis beyond the skin 20 and into the adjacent tissue. The inclination angle of the support segment 122, for example the struts, may be reversed, in another construction, such that distal advance of the hub 111 will deploy the tissue engaging segments 121 beyond the skin 20. Proximal or distal advance of the hub 111 may be accomplished by proximal or distal advance of a control such as a control wire or inner tube releasably engaged with the hub 111.

[0213] Depending upon the desired clinical performance, the tissue anchors 120 may be retractable, such as by axial distal or proximal movement of the control depending upon the inclination angle of the anchors 120. In the embodiment primarily illustrated herein, re-sheathing the anchors 120 may be accomplished by advancing the tubular constraint along the ramped surface of the tissue anchor 120 to move the anchor 120 radially inwardly towards the central longitudinal axis of the device 10. In the case of an anchor 120 which deploys by advance along its own longitudinal axis, the anchor 120 may be retracted by advancing the control in the opposite direction from the direction advanced to deploy the anchors 120.

[0214] Referring to FIGS. 28A-28D, the internal locking system 101 includes a central tubular element or hub 111 and anchors 120. The anchors 120 may be arms, segments, or other members extending from the hub 111. Each anchor 120 may comprise a tissue engaging segment 121 and a support segment 122 which extends to the hub 111 or other control. The internal locking system 101 has a single central tubular hub 111 and a multitude of the anchors 120. As shown, there are four anchors 120. There may be two, three, four, five, six, seven, eight, or more anchors 120. The anchor 120 may be rotatably, hingedly, or otherwise moveably coupled with the hub 111. The anchor 120 may thus move relative to the hub 111, for example after being released from a restraint holding the anchor 120 in a constrained configuration to deploy into a deployed configuration. As further example, the anchor 120 may move from the deployed configuration to a retracted position, as further described herein. The anchor 120 may be curvilinear as shown, for example to allow the anchor 120 to take the geometry shown in FIG. 28A when unconstrained.

[0215] The illustrated anchor 120 may have a distal region 130, a hinge region 135, and/or a proximal region 125. The distal region 130 interacts with the hub element 111. The hinge region 135 and the curvilinear geometry as shown allow the end of the proximal region 125 to extend beyond the body 15, for example beyond a sidewall of the body 15. The proximal region 125 includes a tissue engaging segment 121 configured to engage adjacent tissue. The tissue engaging segment 121 may be the entire proximal region 125 or a portion thereof, for example the tip, etc. The proximal region 125 may thus include a sharpened tissue engaging

segment 121, a shaped tissue engaging segment 121, an angled tissue engaging segment 121, a thickness configured for tissue engagement, and/or other suitable features. In some embodiments, the proximal region 125 may retract back within the body 15, as further described herein. In the embodiment shown, the anchor 120 and central tube 111 are distinct elements which are affixed to one another as shown. In other embodiments, the anchor 120 and tube 111 are a single, integral unit.

[0216] The internal locking system 101 is made from biocompatible metallic wire such as Nitinol, implant grade stainless steel such as 304 or 316, or cobalt-chromium based alloys such as MP35N or Elgiloy. In some embodiments, the internal locking system 101 may be cut from a single tubular piece of metal fabricated via machining or laser cutting followed by a secondary forming or annealing step using similar materials.

[0217] The internal locking system 101 may be in a constrained configuration as the device 10 is placed in position in the LAA and the body 15 expands therein. Then, in a secondary step, the internal locking system 101 locks or otherwise secures the device 10 in the LAA by engaging the anchors 120. If the position is not considered optimal, or if the device 10 otherwise needs to be repositioned within and/or removed from the LAA, the internal locking system 101 and anchors 120 thereof can be unlocked and the device 10 repositioned and/or removed.

[0218] FIGS. 29A-29B are sequential side views of an axially movable loop type unlocking mechanism that may be used with the device 10 to release the tissue anchors. FIG. 29A is a side cross-section view of the device 10 showing the tissue anchors of internal locking system 101 in a deployed configuration. FIG. 29B is a side cross-section view of the device 10 showing the tissue anchors in a retracted configuration. An embodiment of an unlocking system 140 is shown. The unlocking system 140 includes a ring 145. The ring 145 may be moved over the anchors 120 to move the anchors 120 to retracted configurations. The ring 145 may be moved by a pull rod 147. The ring 145 may be releasably attached to the pull rod 147. The pull rod 147 may extend through a catheter to engage the ring 145. The unlocking system 140 may be utilized if, after the internal locking system 101 is deployed, it is desirable to unlock the device 10 from within the LAA in order to reposition and/or remove the device 10.

[0219] In the illustrated construction, deployment of the tissue anchors by distal advance of the restraint enables reversible deployment, so that subsequent proximal retraction of the restraint will retract the tissue anchors. Alternatively, proximal retraction of the restraint to release the tissue anchors will irreversibly release the tissue anchors.

[0220] FIG. 30 is a side view of an embodiment of the device 10 having flexible anchors 401. The device 10 shown in FIG. 30 may have the same or similar features and/or functionalities as the other devices for excluding the LAA described herein, and vice versa. The device 10 may be in the configuration shown in FIG. 30 adjacent to or within an LA 201. The device 10 in FIG. 30 includes the expandable body 15, such as an open cell foam body, which enables collapse and expansion of the device 10, and at least partially encased within the skin 20, which may be a thin, strong layer fabricated from ePTFE (expanded polytetrafluoroethylene), polyolefin, or polyester which assists with healing, anchoring, and retrieval. The device 10 may also be

deployed, and, if desired, repositioned and/or retrieved, or the device 10 may be permanently fixated within the LAA by engaging an anchoring system, such as the internal locking system 101, as described herein. The anchors 401, which may be metallic, may be fabricated from Nitinol. The anchors 401 may be small diameter Nitinol wire approximately 0.001 inches to approximately 0.010 inches in diameter. In some embodiments, the anchors 401 may be approximately 0.0005 inches to approximately 0.020 inches in diameter. The anchors 401 may be deployed upon expansion of the body 15. For example, the anchors 401 may self-deploy upon deployment of the device 10 from a delivery catheter. The anchors 401 may be relatively short and extremely flexible. The anchors 401 may be unable to penetrate the tissue or cause any anchoring immediately after deployment of the device 10.

[0221] FIG. 31 is a side view of an embodiment of a device 10 for occlusion of the LAA having anchors 401 with tubes 500. The device 10 may be positioned adjacent to or within the LA 201. The anchors 401 may be flexible anchors, or in some embodiments the anchors 410 may be relatively stiffer, as further described. The tubes 500 may be stationary or moveable tubes, as further described. In some embodiments the tubes 500 are hypotubes. The tubes 500 may be stainless steel, polyamide, or other suitable materials. The tubes 500 may surround a corresponding anchor 401, as further described.

[0222] In some embodiments, the anchors 401 may be fixed such that they do not move axially. For example, the anchors 401 may have a portion, such as a tissue engaging segment 121, of a fixed length extending outside the body 15. The portion of the anchors 401 extending outside the body 15 may be bent when compressed within a delivery catheter and/or sheath, and these portions of the anchors 401 may then straighten out to the configuration shown in FIGS. 31 and 32 after deployment of the body 15. The fixed length portion of the anchors 401 extending beyond the body 15 may be from about 1 mm to about 5 mm, or from about 1.5 mm to about 4 mm, or from about 2 mm to about 3 mm. This length of exposed anchor 401 outside the body 15 may be effectively shortened by deployment of a corresponding tube 500, as further described. Deployment of the corresponding tube 500 about the corresponding anchor 400 may shorten the effective length of exposed anchor 401, i.e. the length of the anchor 401 extending beyond the end of the tube 500 after deployment of the tube 500, from about 0.5 mm to about 1 mm. These are merely examples of different lengths of the anchor 401 and other suitable lengths may be implemented.

[0223] In some embodiments, the anchors 401 may be moveable axially. For example, the anchors 401 may not deploy or otherwise extend outside the body 15 immediately upon expansion of the body 15. Following acceptable positioning of the device 10 within the LAA, the flexible anchors 401 may then be advanced through a corresponding tube 500. The anchors 401 may move axially in any suitable manner, including those described elsewhere herein. The anchor 401 may be moved through the tube 500 either before or after the tube 500 has been moved and deployed outside the body 15, as described below.

[0224] In some embodiments, the tubes 500 are moveable and deploy outside the body 15. The tubes 500 may be moveable in embodiments having either fixed or moveable anchors 401. The tubes 500 may be pre-loaded over corre-

sponding wire anchors 401 as shown in FIG. 31, for example one tube 500 per anchor 401. The tube 500 may then be moved over the corresponding anchor 401 as shown in FIG. 32. The tube 500 may straighten the anchor 401 and add mechanical integrity. The tube 500 may also act as a perforation protector to prevent the anchor 401 from puncturing through the wall of the LAA. Movement of the tube 500 over the corresponding anchor 401 may shorten the exposed length of the anchor 401, as described. This may provide for a stiffer tissue engaging segment of the anchor 401 due to the shortened exposed length.

[0225] In some embodiments, the tubes 500 extend from the delivery catheter to or near the outer surface of the body 15 but do not extend outside the body 15. Instead, the tubes 500 just guide the anchor 401, for example around the curve, and support the wire 401 right up to tissue penetration. The tubes 500 may set the launch angle so the anchor 401 does not buckle and hits the tissue at the right angle. In this embodiment, the anchor 401 may have relatively more stiffness than in the embodiments where the anchors 401 are relatively flexible, in order to provide a more secure anchoring of the device 10 to the tissue. It is understood the tube 500 may provide this guiding function to the corresponding anchor in any of the embodiments described herein having moveable anchors, such as the moveable anchors 401, the anchors 120, etc.

[0226] The flexible anchors 401 and/or the external stiffening tube 500 may be made from biocompatible metallic materials such as Nitinol, implant grade stainless steel such as 304V or 316LVM, cobalt-chromium based alloys such as MP35N or Elgiloy, other suitable materials, or combinations thereof. The anchor 401 length can vary from 0.1 mm to 5 mm in length with an external stiffening tube 500 that covers from 10% to 90% of the exposed length of the anchor 401.

[0227] The skin 20 at least partially surrounds the body 15 and portions of the skin 20 may or may not be attached to the body 15. The various devices 10 described herein may have the body 15 at least partially encased within the skin 20, which may be fabricated from a material such as ePTFE (expanded polytetrafluoroethylene), polyolefin, or polyester which assists with healing, anchoring, and retrieval. FIG. 33 is a side view of an embodiment of a device 10 for occlusion of the LAA having discrete points of attachment 700 of the skin 20 to the internal foam body 15. For clarity, the points of attachment 700 are shown as dots in the figures. It is understood the points of attachment 700 may not be visible from outside the device 10, for example the skin 20 may be bonded to the body 15 at the points of attachment 700, etc. In some embodiments, in addition or alternatively to bonding, the skin 20 may be secured for example with sutures to the body 15 at the points of attachment 700, and thus some or all of the points of attachment 700 may be visible from outside the device 10. The device 10 may be in the configuration shown in FIG. 33 adjacent to or within the LA 201. The skin 20 may be attached to the body 15 at the various separate points of attachment 700. As shown in FIG. 33, the skin 20 can be partially attached, with portions thereof not attached at all, to the body 15. This may allow, for example, the skin 20 to move during expansion of the body 15 that occurs after deployment of the device 10 from the delivery catheter. The skin 20 may, in some embodiments, be attached at points of attachment 700 located near the proximal side of the device 10, for example to help promote closure of the ostium of the LAA, such as with a

rim 800 as described below. The skin 20 may, for example, be tacked in place in one or more points of attachment 700 near the proximal face so that any bunching of the skin 20 that occurs during implantation occurs near the ostium but within the LAA. This can be achieved using sutures, adhesive bonding, heat bonding, other suitable approaches, or combinations thereof.

[0228] The selective location of the points of attachment 700 may facilitate with formation of a circumferential rim 800 of the skin 20. The rim 800 is shown schematically in FIG. 34 as a triangular rim for clarity. It is understood the rim 800 may be a variety of different shapes depending on the configuration of the device 10, the shape of the LAA, etc. Further, the rim 800 may extend completely or partially around the device 10. The rim 800 may surround the ostium of the LAA. The formation of the rim 800 may help to completely seal the entrance to the LAA around the device 10 and thereby prevent leakage. The attachment points 700 between the skin 20 and the body 15 can prevent irregular bunching of the fabric and instead guide any excess material to form the sealing rim 800 around or near the proximal face of the device 10, as shown in FIG. 34. The rim 800 may form upon expansion of the body 15 after deployment from the delivery catheter, as described herein. Alternatively the attachment points 700 can be designed so as to prevent any bunching at all of the fabric and provide a smooth surface, such as a smooth proximal surface.

[0229] FIGS. 35-36 are side views of embodiments of the device 10 having anchors 120 with V-tips 901 shown in the deployed configuration. The V-tips may be located in the proximal region 125 and/or may form all or part of the tissue engaging segment 121 of the anchor 120, as described herein. The V-tips 901 form a V-shaped point. The V-tips 901 are generally in the shape of a "V" or an otherwise angled, segmented shape. The V-tips 901 may be sharp barbs or hooks. The V-tips 901 may be formed from wire or laser-cut tubing or other suitable methods. As shown in FIG. 35, one or more of the V-tips 901 are attached to the body 15 encased in the skin 20. The V-tips 901 can be attached to the body 15 and/or to the skin 20. In some embodiments, the V-tips 901 are ends of anchors 1000. For example, the V-tips 901 may be part of the anchors 1000 that are within the body 15 and skin 20, as shown in FIG. 36. The distal ends of the V-tips 901 may be free to slide along and collapse or expand. The distal ends of the V-tips 901 may be attached to the body 15, skin 20, and/or the anchors 1000 to allow the V-tips 901 to collapse and retract. During retrieval into a catheter or sheath, the V-tips 901 can flatten out when engaging the inner diameter of the catheter or sheath. The V-tips 901 can be formed from Nitinol, implant grade stainless steel such as 304 or 316, cobalt-chromium based alloys such as MP35N or Elgiloy, other suitable materials, or combinations thereof. The V-tips 901 may then recover their pre-set shape after deployment or re-deployment.

[0230] FIGS. 37A-37C are side views of various embodiments of V-tips that may be used with the anchors described herein. FIG. 37A is a side view of an embodiment of the V-tip 901. The V-tip 901 includes two angled segments. The segments may form the angle in a free state. The angle may be various angular amounts. In some embodiments, the angle formed by the V-tip 901 is no more than about 170°, 160°, 150°, 140°, 130°, 120°, 110°, 100°, 90°, 80°, 70°, 60°, or any smaller, greater or intermediate angular amount. FIG. 37B is a side view of an embodiment of a wave V-tip 1101.

The wave V-tip **1101** may include a curved segment and an angled straight segment. FIG. **37C** is a side view of an embodiment of a two-wave V-tip **1103**. The two-wave V-tip **1103** may include two curved segments. The curved segments may promote engagement of the tip with the inner wall of the LAA. The end of the various V-tips may be smooth and rounded or sharp to promote tissue penetration. In some embodiments, all of the V-tips may have the same shape. In some embodiments, some of the V-tips may have a first shape and other V-tips may have a second shape different from the first shape. In some embodiments, some of the V-tips may be attached to the skin **20** and or body **15**. In some embodiments, some of the V-tips may be attached to the anchors **1000**.

[**0231**] FIG. **38** is a side view of another embodiment of the device **10** for occlusion of the LAA implanted inside an LAA **1201**. The device **10** includes a body **15** with a skin **20** and finial **30** placed within the LAA **1201**. The LAA includes a thicker proximal portion **1203** closer to the ostium. The internal locking system **101**, for example anchors thereof, may be configured to engage with the thicker proximal portion **1203** of the LAA. The various anchors, V-tips etc. described herein for the various embodiments of the device **10** may be used to secure the anchors in the thicker proximal portion **1203**. In some embodiments, the device **10** may be deployed from the catheter such that the body **15** expands. The location, orientation, etc. of the expanded body **15** within the LAA may be verified, for example by imaging, as described herein. The location, orientation, etc. of the expanded body **15** within the LAA may be verified to ensure engagement of the internal locking system **101**, for example anchors thereof, with the thicker proximal portion **1203**. Then, the internal locking system **101**, for example anchors thereof, may be deployed to engage the thicker proximal portion **1203**. If after deployment of the internal locking system **101**, for example anchors thereof, it is determined that the anchors did not engage with the thicker proximal portion **1203**, the anchors may be retracted, as described herein, in order to reposition and/or retrieve the device **10**.

[**0232**] In some embodiments, the internal locking system **101**, for example anchors thereof, may be preloaded surface elements releasably constrained or otherwise locked down in a collapsed or constrained position or configuration. The internal locking system **101**, for example anchors thereof, may be constrained using a restraint. The restraint may be a dissolvable polymer, a lasso, or wires that can be retracted to release the anchors. The restraint may be similar to a deadbolt. Other anchoring concepts include Velcro integral to the ePTFE, electrically orientable/ratcheting anchoring elements, unidirectional Gecko tape, or wires pre-attached to the finial **30**. In some embodiments, the body **15** with skin **20** may be secured within the LAA by texturing the body **15** and exposing the body **15** to the tissue through holes in the skin **20** to increase the friction with the cardiac surface to a high enough level to prevent implant migration.

[**0233**] FIGS. **39A-39B** are perspective views of an embodiment of a deployable anchor **1302** activated by a pull wire **1301** and shown, respectively, in the constrained and deployed configuration, that may be used with the various devices **10**, **1020**, **3000** etc. for occlusion of the LAA described herein. A two-stage anchoring system allows deployment of the anchors **1302** after implantation and expansion of the body **15**. This embodiment incorporates one or more hinged anchors **1302**. The anchors **1302**, which

be a barb or other anchoring element, may lie flat during delivery and during deployment of the body **15**. Next, when pulled or pushed, the anchors **1302** bend at a hinge **1306** and extend outward from the surface of the body **15** and into the LAA tissue. The anchors **1302** may bend at the hinge **1306** using a hollow constraining element **1304** which can be a thin, metallic, round or rectangular box such as a round or rectangular shaped tube, and the pull wire **1301**, for example a sliding element, which can be a wire or suture. The pull wire **1301** is attached to the proximal end of the anchor **1302** and extends back through the delivery catheter or sheath. When the pull wire **1301** is retracted, the anchor **1302** slides back through a slot **1308** in the tube **1304** and bends at the preformed hinge **1306**. A portion of the anchor **1302** then extends out through the slot **1308**.

[**0234**] FIGS. **40A-40B** are perspective views of an embodiment of a deployable anchor **1405** activated by a lock wire **1401** and shown, respectively, in the constrained and deployed configuration, that may be used with the various devices **10**, **1020**, **3000** etc. for occlusion of the LAA described herein. The anchor **1405**, which be a barb or other anchoring element, may be formed from wire or a flat sheet of Nitinol or other shape memory material and heat set to be in an expanded configuration. One or more of the anchors **1405** can be placed along the skin **20** or otherwise along an external surface of the body **15**. One or more corresponding guides **1402**, such as loops, may be located along the skin **20** or the body **15**. The guides **1402** may be located on both sides of the anchor **1405**, as shown. The guides **1402** on a first side of the anchor **1405** may fix the anchors **1405** in place. The guides **1402** on a second, opposite side of the anchor **1405** may act as a guide for the lock wire **1401**, which may be a restraining wire, suture, etc. The lock wire **1401** may be used to constrain the anchors **1405** in a constrained configuration, for example in the flat position as shown in FIG. **40A**. When the lock wire **1401** is retracted, the anchors **1405** deploy, as shown in FIG. **40B**. The anchors **1405** may extend perpendicular to the body **15**, or at an angle.

[**0235**] FIGS. **41A-41B** are perspective views of an embodiment of a deployable anchor **1506** activated by a sheath **1502** and shown, respectively, in the constrained and deployed configuration, that may be used with the various devices **10**, **1020**, **3000** etc. for occlusion of the LAA described herein. The anchor **1506**, which be a barb or other anchoring element, may be formed from wire or a flat sheet of Nitinol or other shape memory material and heat set to be in an expanded configuration.

[**0236**] One or more of the anchors **1506** may be placed along the skin **20** or otherwise along an external surface of the body **15**. One or more corresponding guides **1500** and locking loops **1504** may be located along the skin **20** or the body **15**. The guides **1500** may be located on a first side of the anchor **1506** and the locking loops **1504** may be located on a second, opposite side of the anchor **1506**, as shown. The anchors **1506** are held in the constrained or restrained configuration or position by a sheath cover **1502**. The sheath cover **1502** may be tubular or rectangular in shape. The sheath cover **1502** constrains the anchors **1506**. The sheath cover **1502** may constrain the anchors **1506** in a flat position as shown in FIG. **41A**. When the sheath cover **1502** is retracted, the anchors **1506** deploy, as shown in FIG. **41B**. The anchors **1506** may extend at an angle to the body **15**, or perpendicularly.

[0237] FIGS. 42A-42D are various views of embodiments of the device 10 for occlusion of the LAA having external deployable anchors 1601, 1604 which can be collapsed and expanded by retraction into or out of a sheath or outer catheter. FIG. 42A is a side view of the device 10 having anchors 1601 constrained by a delivery sheath 1603. FIG. 42B is a side view of the device 10 unconstrained by the delivery sheath 1603 with the anchors 1601 deployed. FIG. 42C is a side view of the device 10 having anchors 1604 constrained by the delivery sheath 1603. FIG. 42D is a side view of the device 10 unconstrained by the delivery sheath 1603 with the anchors 1604 deployed. The body 15 with skin 20 can contain the anchors 1601 or 1604 which are fixed to the surface of the skin 20 and are unconstrained and therefore expanded in a free state, as shown in FIGS. 42B and 42D. The delivery sheath 1603, such as a catheter, may be used to constrain the anchors 1601 or 1604. The anchors 1601 or 1604 may then expand when the body 15 is unconstrained by the delivery sheath 1603, for example when the body 15 is released from the delivery sheath 1603. The anchors 1601 may deploy into a curved shape as shown in FIG. 42B. The anchors 1604 may deploy into an angled shape as shown in FIG. 42D. The anchors 1603 or 1604 after deployment may point toward either the proximal or distal side of the body 15.

[0238] FIGS. 43A-43C are sequential side views of an embodiment of the device 10 for occlusion of the LAA shown, respectively, constrained by a lasso 1707, deployed, and adjusted with a mount 1705. One or more anchors 1709 may be pre-mounted within the body 15 and attached distally to the mount 1705. The mount 1705 may be a ring-like member having an opening extending there-through. The mount 1705 is positioned over a rod 1701 with end 1711. The mount 1705 can move, for example slide, over the rod 1701 in the proximal direction. In some embodiments, the mount 1705 may be pulled proximally, for example by a pull wire. In some embodiments, the mount 1705 may move when the rod 1701 is rotated. In some embodiments, the mount 1705 and/or end 1711 of the rod 1701 may be threaded. Movement of the mount 1705 causes the anchor 1705 to move. The device may include a tapered cone 1708. The cone 1708 may be attached to the end of the rod 1701. The mount 1705 may be moved toward the cone 1708 to adjust the height of the anchors 1709. Thus, the anchors 1709 are angled more in FIG. 17C relative to FIG. 17B. The anchor 1709 may move through the body 15 and into the tissue. The anchors 1709 may be adjusted to increase or decrease the amount of tissue penetration, for example by moving the mount 1705 as described. For retrieval, this process can be reversed. In some embodiments, the lasso 1707, attached to a wire 1703, may extend, for example thread, through the threaded rod 1701 and be placed around the anchors 1709 to retract the anchors 1709 back into the body 15. In some embodiments, the lasso 1707 may be used to initially constrain the anchors 1709 and then retract to allow the anchors 1709 to deploy.

[0239] FIGS. 44A-44C are side views of an embodiment of the device 10 for occlusion of the LAA having an adjustable two stage anchor system with anchors 1801 activated by moving a mount 1803 along a rod 1804. The anchors 1801 may be internal grappling hook type structures placed within the body 15 and skin 20. The anchors 1801 may be introduced through a central lumen 1003 that extends through the body 15, as shown in FIG. 43A. The

anchors 1801 may then travel through the body 15 and skin 20 to engage tissue, as shown in FIG. 43B. The anchors 1801 may be adjusted to increase or decrease the amount of tissue penetration. The anchors 1801 are attached at distal ends to the moveable mount 1803. The mount 1803 is prevented from rotating, for example the mount 1803 may be notched to prevent rotation of the mount 1803 within the finial 30, as shown in FIG. 43C. The mount 1803 is threaded onto the threaded rod 1804 that can be rotated clockwise or counter clockwise to change the linear position of the mount 1803. The distal end of the rod 1804 may couple with a cap 1807. The cap 1807 may rotate with the rotation of the rod 1804. The mount 1803 may move proximally causing the anchors 1801 to extend past the surface of the body 15 and skin 20 as shown in FIG. 43B. The mount 1803 may move distally to pull the anchors 1801 back within or under the surface of the skin 20. The depth of penetration of the anchors 1801 may be controlled, for example to account for the non-circular cross-section of the LAA. In some embodiments, the anchors 1801 may be deployed individually. Another option is to deploy the anchors 1801 distal to the body 15 with skin 20 and control the stiffness of the anchors 1801 such that they apply a reasonably uniform penetrating force to the tissue at contact.

[0240] Various features for LAA (LAA) occlusion may be included, such as those described, for example, in U.S. patent application Ser. No. 15/290,692, filed Oct. 11, 2016 and titled DEVICES AND METHODS FOR EXCLUDING THE LAA (Attorney Docket: CNFRM.001P1), in U.S. patent application Ser. No. 14/203,187, filed Mar. 10, 2014 and titled DEVICES AND METHODS FOR EXCLUDING THE LAA (Attorney Docket: CNFRM.001A), in European Patent Application no. EP 14779640.3, filed Aug. 24, 2015 and titled DEVICES AND METHODS FOR EXCLUDING THE LAA (Attorney Docket: CNFRM.001EP), and in PCT Patent Application no. PCT/US2014/022865, filed Mar. 10, 2014 and titled DEVICES AND METHODS FOR EXCLUDING THE LAA (Attorney Docket: CNFRM.001WO), the entire disclosure of each of which is hereby expressly incorporated by reference for all purposes and forms a part of this specification. Further additions and improvements to these and other concepts are described below. The embodiments described in the sections below may include the same or similar features and/or functionalities as the embodiments described above, and vice versa, except as otherwise noted or indicated by context.

A. Basic Plug Design Components and Improvements

[0241] Various occlusion devices and associated features are described with respect to FIG. 45A to FIG. 77. The same or similar features and/or functionalities of the various devices as shown and described with respect to FIG. 45A to FIG. 77 may be present in the various devices as shown and described with respect to FIGS. 1-44C and 78-93B, and vice versa.

[0242] As shown in FIGS. 45A-45C, the device 1020 (sometimes referred to herein as “implant”) may utilize a cored-out foam “cup.” In some embodiments, this may be similar to the foam 1600 design shown in and described with respect to FIG. 16 and/or the foam body 3002 described with respect to FIGS. 85A-93B. The “cup” design may be contrasted with a solid or generally solid tubular foam plug, such as those described and shown in FIGS. 2 and 6. Regarding the cup design of FIGS. 45A-45C, the approxi-

mate thickness of the foam may be about 2.5 mm but can range from about 0.25 mm to about 10 mm. Note that the thickness may be significantly thicker than the typical stent coating or covering as utilized in other applications (e.g. coronary stents, peripheral stents, AAA liners, etc.). In this application, where we are occluding, the thickness of the foam adds some desired structure between the gaps of the internal support structure **1032**, such as a stent. In some embodiments, the thickness may be at least about 0.25 mm; in some embodiments at least about 0.50 mm, 0.75 mm, 1.0 mm or 2.0 mm or greater in an unconstrained state, and in one implementation about 2.5 mm, with thickness selected depending upon the desired performance.

[0243] FIG. 45A is a cross-sectional view of the preferred embodiment showing the components of the implant **1020** having a proximal (atrial) end **1022**, a distal (LAA) end **1024** and an interior cavity **1026** in the expanded configuration. An expandable tubular wall **1028** defines the interior cavity **1026**, which may be enclosed at its proximal end **1022** by a tissue scaffold **1030** or other barrier configured to span the ostium and isolate the LAA from the atrium post deployment. The proximal edge of the tubular wall **1030** may be provided with a ramped reentry or recapture surface such as an annular chamfer **1031** extending circumferentially or otherwise around the proximal edge of the implant **1020**, preferably continuously, to facilitate proximal retraction of the implant into the deployment sheath to permit repositioning or removal if desired. A distal extension **1029** of the tubular wall **1028** extends distally beyond the internal support (discussed below) to form an atraumatic leading edge.

[0244] The tissue scaffold **1030** may be integrally formed with the tubular wall **1028** or may be bonded thereto. The tissue scaffold **1030** and the tubular wall **1028** may have approximately the same thickness and pore characteristics, discussed below. Alternatively the tissue scaffold may comprise a different material such as ePTFE, PTFE, Dacron, or others known in the art, configured to support tissue ingrowth and isolate the LAA, but thinner than the tubular wall **1028**.

[0245] An expandable, internal support structure **1032** such as a wave stent **1034** or other frame may be provided. The illustrated wave stent **1034** comprises a plurality of struts **1038**, adjacent pairs of struts joining to form a plurality of proximal apexes **1041** and distal apexes **1042**. The stent **1034** may be laser cut from tube stock as is known in the art. Each of at least three, and preferably at least 4 or 6 or 8 or more of the proximally facing apexes **1040** is provided with a reentry or recapture strut **1044**, which incline radially inwardly in the proximal direction to a central hub **1046**. Recapture struts may be cut from the same tube stock as the stent. Hub **1046** may be provided with a central lumen, such as for delivery over a guidewire, or for releasable engagement with a deployment device (not illustrated). Alternatively, the hub **1046** may be provided with an attachment such as an eyelet **1048** for receiving a suture loop. A suture or other retention element may extend distally from the deployment catheter, through the tissue scaffold **1028**, through the eyelet **1048** and proximally back through the tissue scaffold **1028** and into the deployment catheter. Following satisfactory positioning of the implant **1020**, the suture may be removed, releasing the implant **1020** from the deployment catheter leaving a homogeneous tissue scaffold **1030** as resilience of the material closes the suture tracks. In one preferred implementation the implant **1020** is deployed

from the delivery catheter without advancing over the wire and the hub lacks a central lumen. In one embodiment, the implant is secured to the delivery system using any of a variety of means known in the art including screw mechanisms or ball in socket attachment mechanism, which can also pivot.

[0246] The tubular wall **1028** may be attached to the stent **1034** by adhesives, sutures or other bonding techniques known in the art. In the illustrated embodiment, the tubular wall **1028** is sutured to the stent **1034** and the tissue scaffold **1030** is sutured to the recapture struts **1044**, with the support structure **1032** carried within the cavity **1026**. Alternatively, at least a portion of the support structure **1032** may be carried on the outside surface of the tubular wall **1028** or tissue scaffold **1030**. The wave stent may be embedded within the tubular wall **1028** such as by sandwiching the stent between inner and outer layers of foam which are then bonded together. Similarly the recapture struts may be enclosed between inner and outer polymer layers. The polymeric material can also be foamed around the stent so that a secondary attachment process is not required.

[0247] FIG. 45B is a distal end view of an embodiment of the implant **1020** showing the internal metallic structure having a central hub **1046** and eight recapture struts **1044** inclining radially inwardly to the hub **1046**. A plurality of suture retainers such as apertures **1050** are attached to or formed in the struts **1044** to receive the sutures used to secure the tissue scaffold **1030**. This reduces the tendency of material of the tissue scaffold **1030** to slide distally along the struts **1044** if the implant **1020** is proximally retracted into the deployment catheter.

[0248] The frame may be expandable from a contracted delivery configuration to an expanded deployed configuration. The frame may be retractable from an expanded deployed configuration to a contracted delivery configuration. The frame may be generally tubular, e.g. circular, rounded, segmented, polygonal, other shapes, or combinations thereof in the unconstrained, expanded configuration, and preferably presses the foam into conformance with the shape of the inside surface of the LAA. This permits the deployed implant to minimize leaks, the largest of which is no more than about 4 mm or 3 mm or 2 mm or less and in some deployments essentially no leaks as viewed on color Doppler.

[0249] FIG. 45C is a proximal end perspective view of the outside of an embodiment of the implant **1020** having a unitary foam shell and showing the proximal chamfer **1028**, in an unconstrained expansion. Anchors deployed near the distal end of the frame are discussed in further detail below.

[0250] Some advantages of the cored-out foam “cup”, as compared to a solid foam plug, are as follows: it still behaves like a full foam plug with respect to conformability and sealing; it allows incorporation of an internal metallic frame which can be optimized to provide the desired amount of expansion for sealing and anchoring by providing an optimal radial force and an attachment point for the anchors, and a front face inside the proximal face to aid in collapse of the foam for retrieval; by sizing the metallic frame so that it is shorter in length than the foam cup, an atraumatic distal bumper is formed which is entirely foam and can be extruded from the sheath tip as the tip is advanced within the LAA; and the reduced overall volume of material aids with the following: it significantly reduces the delivery profile, it is easier to flush to remove air prior to delivery into the

vascular system, and it makes the plug more porous to blood so that if embolized within the cardiovascular system, it allows more blood to flow through it.

[0251] In an embodiment, the proximally facing edges of the foam plug **1040** are chamfered to aid in loading and retrieval. Also, while there can still be a central location to allow tracking of the implant **1020** over a guidewire-type device, in some embodiments there is no lumen or there is just a slit in the foam plug **1040**, as it is not desirable to have a significant residual central hole which may cause thrombus formation or allow leakage. The slit can be a single slit, double cross-shaped slit, or multiple slits. The objective is to still allow tracking over a guidewire but to be sure the hole closes completely once the guidewire is removed. In the case of a solid face, the implant **1020** may not be tracked over a guidewire and may instead, for example, be delivered through a long transeptal sheath.

[0252] Please note that the term “guidewire”, as utilized above, can mean an actual medical device sold as a guidewire or it can be a catheter, such as a pigtail catheter, which is initially placed in the LAA over which the LAAC (LAA Closure) implant **1020** is tracked.

[0253] Diameters: The LAA may vary in diameter from about 15 mm to about 33 mm and as such, the implant **1020** diameter must be able to accommodate this variation in sizes. The more the implant **1020** may accommodate various large ranges of diameters, the fewer predetermined sizes are needed, thereby simplifying the procedure for implantation. The construct of this implant **1020** is such that it may accommodate diameters less than 50% of the fully expanded diameter. The preferred plug **1040** diameters may be about 27 mm, 33 mm, and 35 mm. Ideally, only 1-2 sizes would be needed to close a large range of LAA diameters. This is a key advantage of the foam plug **1040** concept as compared to metal cage type devices with fabric tissue scaffolds.

[0254] Depth: The preferred plug **1040** length (the depth of the occluder within the LAA generally along a proximal-distal direction) is 20 mm and is independent of the diameter of the implant **1020**. This allows for good implant **1020** stability while still accommodating the majority of anatomies. The distal tip of the foam plug **1040** is very soft, providing an atraumatic tip as it enters the LAA when the distal tip of the implant **1020** is allowed to protrude past the distal dip of the delivery catheter or sheath. The short depth makes placement of the plug **1040** more robust, as there is less need to align delivery catheters with the LAA, as is needed with longer devices.

[0255] Foam and Porosity: The average pore size of the foam is 250-500 microns. The foam has a very high void content (90-95%) to promote quick and thorough tissue ingrowth. The open cell foam permits blood to flow through it. If the plug **1040** should embolize, it will be open enough to allow enough blood flow to be safe until it can be retrieved. Additionally, the large void content should be beneficial for proper flushing of the implant **1020** to prevent air introduction into the vascular system. The porosity and cell size may be as described with respect to the foam body **3002** of the device **3000**, shown and described for example with respect to FIGS. **85A-90D**.

[0256] The compliance and thickness of the foam are designed to provide a good seal against the tissue with minimal compression. While other devices require significant oversizing to obtain a seal, this implant **1020** may require only ≤ 1 mm of oversizing.

[0257] LA Facing Surface: ePTFE (expanded Polytetrafluoroethylene) or PTFE as the skin/layer for the implant **1020** such as over or partially over the plug **1040**, as described above, may be ideal for supporting neointimal formation without thrombus formation. While embodiments may be described with respect to ePTFE, it is understood that PTFE may also be used. It may, however, reduce safety due to the inability or reduced ability to allow blood flow through the surface of an embolized implant **1020** due to the low porosity of the ePTFE, even though blood flow may be enabled around the outer surfaces of the cup. ePTFE porosity is much lower than that of the open cell foam, so blood flow across the membrane may be negligible. It is, however, hydrophobic which is beneficial for thromboresistance. One option, to maintain the desired open porosity of the foam structure while adding the thromboresistance of ePTFE and/or PTFE, is to add a PTFE coating via vapor deposition to the foam. The thromboresistant coating may contain ePTFE or PTFE. This creates a highly porous surface that simulates the ePTFE morphology. Methods of attachment could include vapor deposition, as mentioned above or elastomeric glue (although this may eliminate porosity at the attachment points). If ePTFE is preferred, that could be attached by encasing the metallic frame in ePTFE then wrapping through the center, around the OD, and attaching via sutures.

[0258] It may be desirable to reduce the pore size of the foam to between about 30-200 μm , as further described herein.

[0259] Barbs/Anchors: There are several options or types of barb designs that may be implemented for anchoring the implant **1020** within the LAA. The following are some examples: 1) Static: always engages tissue when the plug is deployed. This makes re-sheathing and repositioning of the implant **1020** more difficult. 2) Constrained: the implant **1020** can be deployed with barbs constrained. The implant **1020** can then be repositioned, as needed. The barbs are then released when the plug **1040** is in its final position. 3) Dynamic: barbs can be deployed or retracted as desired without dislodging plug. Dynamic barbs may allow for deployment and retraction, for example to reposition and/or remove the implant **1020**.

[0260] In some embodiments, the implant **1020** may have different features from other implants described herein. In some embodiments, the implant **1020** may include any or all of the following features: does not have a central lumen; has a spiked element against the proximal face inside the cup in addition to the wave stent; has anchors/barbs that can preferably be activated as a secondary step following placement of the plug itself; has a layer on the proximal face, which may be similar to the proximal face **1604'** shown in FIG. **16** or the layer **3100** shown in FIG. **85A**, although in some embodiments the PTFE may be applied via vapor deposition coating as opposed to expanded PTFE (ePTFE) attached as a secondary material.

B. Endoskeleton System with Proximal Spokes

[0261] The implant **1020** may include a foam plug **1040** with a central endoskeleton that includes a proximal spoke face **1080** with several radial struts. This configuration improves the ability to retrieve (re-sheath) the foam implant **1020**. The stent version depicted in FIG. **45A** and FIG. **45B** may be laser cut from a superelastic nitinol tube, however, numerous other biocompatible metallic materials can be utilized such as shape memory Nitinol, stainless steel,

MP35N, or Elgiloy. While this embodiment is self-expandable, a balloon-expandable design could be utilized. Additionally the frame could be fabricated from drawn wire as opposed to being laser cut from a tube. Loops can be provided along each strut to allow for attachment to the foam via sutures, although other attachment processes could be utilized, such as adhesive bonding. The loops located mid strut can be oval in shape and staggered, to allow easier loading into the delivery catheter and ease of fabrication. Additionally, as shown in FIG. 46, there may be no loops. While the embodiment shown in FIG. 45A has 8 struts, anywhere from 4 to 32 struts may be utilized. In general, it is preferred that the foam be attached to the frame at numerous points including the center. This promotes retrieval without damage to the foam and the suture loops are beneficial for this. In other embodiments, the foam could be formed around the endoskeleton so that it is within the foam, eliminating the need for a secondary attachment step. As shown in FIG. 45A, it is preferable that the proximal foam face have a chamfer at the edges to minimize the bulk of the material in this area to aid in re-sheathing.

[0262] FIGS. 47A-47B are perspective and side views respectively of an embodiment of the LAA occlusion device 1020 having an internal frame 1032, which may be a single piece. While the design shown in FIG. 45B is fabricated from two separate pieces—the proximal spoke face 1080 with eight struts and a wave stent—in some embodiments there may be a single piece unit frame 1032, such as that shown in FIGS. 47A and 47B. In some embodiments the proximal spoke face 1080 may support re-sheathing, the eight crown wave cage stent 1060 supports the foam cylinder plug 1040, and the eight to sixteen, or fewer or more, barbs or anchors 1100 located within the cylinder provide anchoring to resist embolization. The anchors 1100 can be located proximal, distal, and/or centrally along the length of the cylinder. The anchors 1100 can preferably range in size, when fabricated from a Nitinol tube, from about 0.003" to about 0.009" in thickness and from about 0.007" to about 0.015" in width. In some embodiments the anchors 1100 may extend about 1 mm from the surface of the implant 1020 but can range from extending about 0.5 mm to about 2 mm, or less or more, from the surface of the implant 1020. The anchors 1100 may be in a single location along the length of the cylinder or staggered, as shown in FIG. 48. In vitro anchoring dislodgement resistance with these designs may be in the 0.5 lb to 1.5 lb force range. There may be a single row of anchors 1100 as shown. There may be multiple

[0263] FIG. 49 depicts the implant 1020 with central endoskeleton that includes a proximal spoke face 1080 in its fully expanded configuration as attached to the delivery catheter. FIG. 50 depicts the implant 1020 in an embodiment of its collapsed configuration. Variations include an outer sheath component of the delivery catheter that can be stretchable or slit at the tip, aiding in tapering collapse. A reduced coefficient of friction on the foam face may reduce the forces required to collapse the implant into the catheter. This may be done, for example, by applying a layer of PTFE via vapor deposition or other processes to the foam, or by a layer of expanded PTFE (ePTFE) attached to the proximal face using adhesives or mechanical methods such as suturing. Secure attachment of the foam face to the spoked system may be obtained by suture attachment or other methods including adhesive bonding, which will prevent the foam from bunching up during retrieval which can result in

increasing forces and potentially tearing of the foam. If not securely attached with distributed forces, the metallic spoked element may pull through the foam during re-sheathing, destroying the implant.

C. Proximal (Blood-Contacting) Surface of the Foam

[0264] The foam implant 1020 may be comprised of porous open cell foam. The foam can be any of a variety of currently available materials including polyurethane-based biomaterials such as polyurethane or polycarbonate-polyurethane, or polyvinyl acetal (PVA) (Ivalon®). The foam can also be reticulated, such as a net. An embodiment utilizes a non-resorbable reticulated polyurethane-based biomaterial. Additionally, resorbable foams could also be utilized including a polyhydroxyalkanoate (PHA) such as poly-4-hydroxybutyrate (P4HB) or cross-linked resorbable polyester urethane-urea scaffolds.

[0265] Pore sizes in the material may be from about 50 micron to about 800 micron, preferably from about 250 micron to about 500 micron. Such a high void content (e.g. from about 90% to about 95%) material promotes quick and tenacious tissue ingrowth and effectively mimics the extracellular matrix. While such a high void content material is desirable for tissue ingrowth, it may not be ideal for thromboresistance, which is required for the left atrial (LA) surface. A thromboresistant surface is desired on the face that faces the LA. If modifications are made to the LA facing surface to promote blood compatibility, those modifications may be extended from about 1 mm to about 20 mm, preferably from about 1 mm to about 5 mm, onto the sides of the implant 1020 to assure thromboresistance in the event the implant 1020 is deployed with a portion of the implant's 1020 side surface projecting outside the LAA and into the blood environment. If there is a hole within the proximal face, such as a guidewire lumen, the thromboresistant surface may extend at least partially within that lumen. Additionally, this thromboresistant layer should promote tissue ingrowth and endothelialization.

[0266] Various methods may be used to create a thromboresistant proximal face of the implant 1020, including but not limited to the following. For example, an expanded PTFE (ePTFE) skin or layer may be applied to the outside surface of the foam implant as described elsewhere herein. It could be attached by encasing the metallic frame in ePTFE then wrapping through the center, around the OD, and attaching to the frame. This can be done using numerous methods including suturing or adhesive bonding, including the use of elastomeric glue (although this may eliminate porosity at the attachment points). This ePTFE layer can extend into the guidewire lumen, if there is one. In addition to ePTFE, electrospun, melt blown, non-woven, knitted or woven fibers of PTFE, polyester, PGA, PLA, poly-4-hydroxybutyrate (P4HB) or other biocompatible fiber materials can be utilized to create a porous biocompatible surface.

[0267] In some embodiments, a coating of a hydrophobic material such as PTFE is applied over the proximal face using any of numerous processes known to one skilled in the art including vapor deposition coating. Ideally this coated layer would also extend partially onto the sides of the implant. While some embodiments may not include a guidewire lumen, if a central lumen is present, the coating would preferably extend at least partially (e.g. about 1 mm) into it. To promote thromboresistance, this coated layer would decrease the porosity of the blood-contacting face to a

porosity from about 30 microns to about 200 microns, preferably from about 100 microns to about 150 microns. Materials which could be utilized for this include conformal coatings such as PTFE applied in a thickness of about 50-100 microns, polyurethane spray or dip coatings, albumin, polyethylene glycol (PEG), or poly(ethylene oxide) (PEO), all with or without the incorporation of heparin or nitric oxide. The PEG or PEO would ideally be attached via a grafting process. In the preferred embodiment, the outer layer would also be lubricious to assist in re-sheathing of the implant. This can be achieved with both hydrophobic materials, such as ePTFE and PTFE, and hydrophilic ones, such as PEO and PEG. In order to produce a desirable combination of porosity and blood compatibility, a two-step process may be utilized where the foam is first coated with a base layer, such as a polyurethane-based biomaterial, then in a second step a more thromboresistant and lubricious surface is created utilizing PTFE, PEG, or PEO. Heparin or other anticoagulants may be added to the final blood-contacting surface.

[0268] Another option to create smaller pore sizes with an ePTFE-like material would be to attach an electrospun layer of PTFE to the face of the foam using suturing. A very thin layer (<1 mm) can be made and attached via suturing or adhesive bonding.

[0269] Another desired property of the foam of the plug 1040 is to provide echogenicity of the implant 1020, which allows for visualization by echocardiography. To promote echogenicity, a porous surface may be adequate; however, in certain cases a hydrophilic surface may be beneficial. To promote blood compatibility and a hydrophilic surface, the preferred embodiment would be a foam implant which has a surface grafted with PEO or PEG.

D. Static Barb (Anchor) Designs

[0270] Static barbs engage tissue when the plug 1040 is deployed, e.g. expanded. While this simplifies fabrication, it makes re-sheathing and repositioning of the implant more difficult.

[0271] In some embodiments, as shown in FIG. 51, a barb 2000 may be fabricated from wire and crimped onto the stent 1034, in this example a wave stent. The barb may be made from Nitinol wire of any diameter, with a preferred range of about 0.005" to about 0.012". The tip can be sharpened for ease of penetration into the tissue. It can be attached to the stent frame using a crimp sleeve made from stainless steel, Nitinol, or titanium tubing. It may require filler wires inside the crimp tube to prevent rotation of the barb. It could also be attached by welding, using a laser or other energy source.

[0272] Referring to FIG. 52, in some embodiments a laser cut double barb 2000 system can be utilized. This can be fabricated from a Nitinol tube 2002 cut to allow two crimp ends with one barb 2000 near each crimp 2004 with a continuous Nitinol connection that follows the curvature of the stent 1034, in this example a wave form. An advantage of this embodiment is that it takes less labor to fabricate and shape the barbs, is easier to create sharp tips, and the curvature of the tube wall results in stiffening the barbs. FIG. 53 shows an embodiment of the laser cut part of FIG. 52 prior to forming the crown curvature.

[0273] Referring to FIG. 54, in some embodiments the wire form follows the curvature of the wave support cage 1034 (stent), terminating in two barbs 2000. It can be crimped to the wave cage or can be sewn with sutures,

welded, or glued in place on the wave cage (stent). The advantage is that crimping is not required to prevent barb rotation.

[0274] Referring to FIG. 55, in some static barb embodiments, a laser-cut wave support cage (stent) can be fabricated with integrated barbs 2000. The advantage of this concept is that no secondary attachment step is required to attach the barbs to the cage. It may also be easier to add more barbs. A limitation is that it may be difficult to have 8 crowns (waves) with barbs on every strut as there may not be enough material available, therefore 6 crowns may be preferable.

E. Constrained Barb (Anchor) Designs

[0275] With constrained barbs 2010, the implant 1020 can be deployed in the LAA with the barbs 2010 constrained and can therefore be repositioned, as needed, prior to barb release. The barbs 2010 are released when the implant 1020 is in its final position.

[0276] In one embodiment, as shown in FIG. 56, a lasso-style constraint system can be added to static barbs to create constrained, deployable barbs 2010. A suture material can be tucked between the barbs 2010 and struts to prevent spinning upon deployment. Removal of the lasso can release multiple barbs in a circular array.

[0277] As shown in FIG. 57, barbs can be formed with a loop approximately midway along the barb 2010 which allows suture or thread to be placed through the loop, forming a lasso. This prevents full expansion of the barbs 2010 until the body of the implant is in its final desired position within the LAA.

[0278] A flipping-barb option is shown in FIG. 58. In this embodiment, barbs 2010 can be elongated designs that are folded back inside a cored-out foam opening prior to loading into the delivery system. This may require drawstrings or other locking elements to hold the barbs in a constrained configuration. Once the implant 1020 is in its final desired location, the constraint is removed and the barbs are no longer constrained and flip into position, engaging the tissue.

F. Dynamic Barb (Anchor) Designs

[0279] Dynamic barbs 2020 can be deployed or retracted as desired without dislodging the implant. Dynamic barbs 2020 may be the preferred option for some procedures, for example for recapture of the implant 102 into the delivery catheter and/or sheath.

[0280] One embodiment is a tube within a tube. In this embodiment, as shown in FIG. 59, a laser cut tube 1030 may be utilized to construct a one-piece front spoked face 1080 and wave stent 1032 from a single piece of preferably superelastic Nitinol tubing. Other materials, including shape memory Nitinol, stainless steel, MP35N, or Elgiloy, could be utilized. A second smaller laser cut tube 1040, as shown in FIG. 60, may be utilized to form an inner spoked barb array.

[0281] As shown in FIG. 61, during deployment of the foam implant, the front spoked face and wave stent may be deployed while the spoked barb array remains in a constrained position. The implant 1020 can be repositioned, as needed, then distal motion of the inner tube 1040 with respect to the outer tube 1030 allows the barbs 2020 to expand and engage, as shown in FIG. 62. The inner spoked

barb array can be re-constrained and re-released repeatedly until disconnected from the delivery catheter transmission lines.

[0282] In another embodiment, as shown in FIG. 63, a dynamic barb 2020 design which can preferably be fabricated from a single component is illustrated. This embodiment can be cut from a laser cut tube 1045, preferably superelastic Nitinol, where half of the front spokes connect to wave points of the stent cage 1032 to support re-sheathing while the other half of the spokes are formed into the barbs 2020.

[0283] Recapture or re-sheathing of the implant 1020 may initiate the barb retraction by collapsing the front spoke face, as shown in FIG. 64, thereby simultaneously retracting the barbs 2020 from the tissue. This allows for safe repositioning of the implant 1020 with a minimal amount of re-sheathing required (limiting the length of implant required to be fully retracted into the sheath).

[0284] In another embodiment, as shown in FIG. 65, a dynamic hinged barb system is illustrated. This is a laser cut wave form integrated barb 2020 with a living hinge and constraint. When the constrained end is heat-set, it may curl inward to ride over or under the wave strut. When positioned over the wave strut, its sharp barb end may point to the inner diameter of the assembly. When popped into position under the strut, the opposing barb end may see-saw upwards to engage tissue. Activation of the hinged barbs 2020 can be accomplished through the use of a lasso threaded in a circular array between each barb and the corresponding strut. Cinching inward on the lasso can pop the retention constraint from above the strut to below the strut, causing the opposing barb end to be raised above the surface of the strut where it can engage a tissue surface.

G. Embodiments with Foam Cup, Wave Stent, and ePTFE Layer

[0285] As shown in FIGS. 66A-66C, the foam cup plug 1040 with internal wave or zig-zag anchor (for example, as shown in and described with respect to FIG. 16) can be modified to be completely covered on the outer surface by an ePTFE layer 2060. This layer 2060 can attach to the distal end 1024 of the foam via suture or adhesive bonding as opposed to just the proximal face 1022. It can wrap over the entire external surface and into the central lumen on the proximal face, attaching to the proximal portion of the wave stent by lamination or adhesive bonding. Other biomaterials or coatings could be utilized including, but not limited to, PTFE or polyurethane.

H. Dynamic and Static Anchor Concepts

[0286] The embodiment of an implant 2300 shown in side cross-section view and end view in FIG. 67, respectively, includes anchors 2310 that can be tied, welded, or crimped together at their proximal ends. The anchors 2310 may be made of Nitinol wire to permit loading into the delivery system without taking a set. There could be 8-16 wires formed in the curve. The anchors may act like a “grappling hook”. The assembly is loaded into the delivery catheter in a straightened position. As they are pushed out of the delivery catheter, they take the shape shown in FIG. 67 and pierce into the tissue through the foam 2320. The foam 2320 is cored out as shown to reduce the volume of foam needed to compress into the delivery system and yet maintain sufficient radial force to seal the tissue.

[0287] The embodiment of the implant 2350 shown in FIGS. 68A and 68B includes a wave stent internal anchor with barbs within a foam plug which has been cored out to be thicker on the distal end to create a larger atraumatic foam tip bumper 2360 when collapsed within but partially deployed from the delivery catheter. The proximal face 2363 can have an internal lumen 2365 as shown in FIG. 68A, but may not include an internal lumen as shown in FIG. 68B.

I. Constrained Anchor Deployed in Secondary Step

[0288] The embodiment of an implant 2370 shown in FIG. 69 has barbs/anchors 2371 pre-attached to a wave stent 2372 inside the foam 2374. A suture 2375 is looped around the distal end of the wave stent 2372 to compress the stent 2372 and pull the barbs 2371 inward. The suture 2375 is tied with a slip knot. After delivery of the device 2370 into place, one end of the suture 2375 is pulled and the knot comes free and the suture is removed, allowing the stent 2372 to open radially and the barbs 2371 to engage the tissue. The barbs 2371 can be located distal to the foam 2374 as shown, or pre-engaged with the foam 2374 and penetrating through the foam 2374.

J. Internal Stent with Increased Embolization Resistance

[0289] A metallic stent-like frame 2380 with distal static barbs 2381 and a proximal “speed bump” 2382 is disclosed as shown in FIGS. 70-72. It could be a zig-zag stent (as shown) or a wave stent or other similar expandable embodiment. The bumps 2382 placed on the external portion of the metallic stent frame 2380 can be rounded or pointed in design. Their purpose is to provide added resistance and stability for the implant when deployed in the LAA, to prevent embolization. In the preferred embodiment, the foam “cup” 2384 could be shaped as depicted in FIG. 71 to provide added material 2385 on the distal end for an atraumatic bumper when the distal end of the implant is partially deployed from the delivery catheter. It may or may not have an internal lumen for a guidewire.

K. Constrained Atraumatic Anchor

[0290] As shown in FIGS. 73 and 74, a wave or zig-zag or other stent 2390 may be fabricated with distally located loops 2391 which engage the tissue in the LAA to anchor the implant in place and prevent dislodgement resistance. Because they are round and not sharp, this limits the risk of perforation, however, if a totally rounded loop does not provide adequate dislodgement resistance, the tips can be modified to incorporate a sharp feature. Loop anchors 2391 can be placed on each stent end or on just a few, so anywhere from 4-16 anchors can be placed.

[0291] During delivery of the implant through the vascular system and into the heart and LAA, the loops 2391 are folded toward the center of the constrained stent and are lined up next to each other, as shown in FIG. 75. The inner catheter is placed through the loops 2391 to keep them constrained. When the system is in the LAA, the outer catheter/sheath is retracted, deploying the proximal portion of the implant. If positioning appears acceptable, the inner catheter can be removed, allowing the distal portion of the implant to fully expand and the loop anchors to engage the LAA tissue.

L. Perfusion Element & Barb Options

[0292] In the event of the implant being dislodged after deployment in the LAA, it is anticipated that the device

would travel into the LA, across the mitral valve and into the left ventricle, then out the left ventricular outflow track, across the aortic valve and into the aorta and distal circulation. In this journey, it is possible that the device may get lodged in any of the above structures, interrupting flow and causing distal ischemia and possible hemodynamic collapse. It therefore would be desirable for an implant 2392 to have design features which would allow for distal perfusion, for example as shown in FIGS. 76 and 77.

[0293] FIG. 76 is a top view of an embodiment of the implant showing the left atrial surface. Within the surface is seen a valve, which in the shown embodiment is a simple cut (A) which would open up when sufficient pressure was applied, allowing for flow through the device 2392. This flow could be bi-directional or uni-directional and depending on the specific conditions allowing for flow rates from 10 ml/min to 5 L/min. In the embodiment as shown, this would be accomplished without loss of structural integrity, the loading conditions would result in the device 2392 separating into a multiple sub sections each of which would be retrievable using standard technique. A specific device could have a single valvular element or an array (as shown).

[0294] As shown in FIG. 77, in some embodiments, a series of side ports (B) may be cut in the side wall of the foam 2393 of the implant 2392 to allow for blood flow in the case of dislodgement and distal embolization. These can vary in size and number from 1-20 ports of about 0.1 mm to about 5 mm in diameter. They can also vary in shape including but not limited to circular, oval, and rectangular.

[0295] Regarding barb designs, such as those described herein, in addition to having an array of barbs deployed at different distances from the LA surface, barbs can be incorporated which penetrate into the tissue to different depths. In one embodiment, the barbs placed most proximal on the implant can be longer so they penetrate deeper into the thicker proximal LAA tissue whereas those placed most distal on the implant are shorter, so they penetrate less deep into the delicate distal tissue, to maximize embolization resistance while minimizing the risk of perforation. In another embodiment the proximal and distal barbs can be the same length but can be fabricated from different diameters of wire or can be cut at different thicknesses from tubing material, so that the barbs that engage the more delicate distal LAA tissue are more flexible, or they are designed to primarily engage the internal trabeculations within the LAA, whereas the proximally located barbs penetrate the tissue. Alternatively, two barbs can be placed at each crown point of the stent, as opposed to one.

M. Multi-Functional Occlusion Devices

[0296] FIGS. 78-84 depict various features that may be used, either alone or in combination, with any of the LAA occlusion devices and methods described herein. In some embodiments, the features of FIGS. 78-84 may be incorporated into the device 3000 and associated features and methods shown and described with respect to FIGS. 85A-94B.

[0297] FIG. 78 is a side view of an embodiment of the LAA occlusion device 3000 with ablative features. The LAA occlusion device 3000 has an array of ablative elements 3005. The ablative elements 3005 deliver energy to the tissue in and around the LAA ostium to electrically isolate the LAA. In the shown embodiment, the array of ablative elements 3005 is positioned at the proximal end 3004 of the

body 3002. The ablative elements 3005 may be electrically connected through a deployment catheter to an energy source. Energy may be provided via radiofrequency, ultrasonic, electrical, or other suitable methods. An inner lumen 3003 extends through the body 3002. In some embodiments, there may not be the lumen 3003.

[0298] FIG. 79 is a side view of an embodiment of the LAA occlusion device 3000 with pressure sensing features. The device 3000 has a pressure sensor 3007 on its proximal surface 3008. In some embodiments, the sensor 3007 may be on the proximal surface 3102 of the proximal cover 3100 (see FIG. 85A). In some embodiment, the sensor 3007 does not protrude into the LAA, such as a flat sensor on the proximal surface 3008 or 3102. The sensor 3007 is electrically connected via a wire 3009 to an electronic element 3011. The electronic element 3011 has the capability of transducing and storing the signal generated by the sensor 3007. This information may be transmitted with a signal 3013 remotely. The electronic element 3011 may be powered remotely or by an internal battery.

[0299] FIG. 80 is a side view of an embodiment of the LAA occlusion device 3000 with drug elution features. The device 3000 has a sensor 3007 on its proximal surface 3008. The sensor 3007 may be on the proximal surface 3102 of the proximal cover 3100 (see FIG. 85A). The sensor 3007 is electrically connected via a first wire 3009 to an electronic element 3011. The electronic element 3011 is electrically connected via a second wire 3015 to a drug reservoir 3017 which is fluidly connected via a conduit 3019 to a drug exit port 3021. This allows for drug to be delivered into the LA, as well as for monitoring concentration of specific chemical (s) and or states and to deliver agents in response, e.g., blood sugar level driving insulin delivery. The sensor 3007 may detect the level of various chemicals and the reservoir 3017 may be controlled, for example by the electronic element 3011, to elute drug via the port 3021 in response.

[0300] FIG. 81 is a side view of an embodiment of the LAA occlusion device 3000 with pacing/defibrillatory features. The device 3000 has an electrical pacing element 3025, such as an electrode. The pacing element 3025 extends circumferentially about the body 3002. The pacing element 3025 may be in other configurations. The pacing element 3025 is connected by a wire 3027 to a pace generator 3029. The generator 3029 is attached by a wire 3031 to a battery 3033. This pacing system may pace the atrium and defibrillate the atrium when in atrial fibrillation. The generator 3029 and/or battery 3033 may include components for controls, communications, commands, etc.

[0301] In some embodiments, the LAA may be electrically isolated. The LAA may be electrically isolated with an occlusion device that incorporates one or more ablative elements, such as those shown and described with respect to FIGS. 78-81, conduct the ablation to electrically isolate the LAA, then disengage the occlusion device 3000 leaving it in place within the heart. In some embodiments, the LAA may first be electrically isolated and then the device 3000 implanted, as described herein, for example with respect to FIGS. 82-84. In some embodiments, conformable circumferential ablation via a foam plug with ablation elements may be incorporated.

[0302] FIGS. 82-84 depict various systems and methods for electrically isolating the LAA that may be used with the device 3000. In some embodiments, the LAA may be electrically isolated followed by LAA closure. For example,

the systems and methods shown in FIGS. 82-84 may be used to conduct the isolation, followed by LAA occlusion using the various LAA occlusion devices described herein, such as the device 3000.

[0303] FIG. 82 is a side view of an embodiment of over the wire circumferential ablation balloon system. An over-the-wire balloon catheter 3035 is placed over a guidewire 3037 and into the LAA (LAA). The balloon 3039 can have one or more circumferential ablative elements 3041, such as apposed radiofrequency (RF) elements, to electrically isolate the LAA using RF to treat atrial fibrillation. The ablative element 3041 extends circumferentially about the balloon 3039. The ablative element 3041 may be in other configurations. This guidewire 3037 may have attached to its distal end a balloon 3043 which is inflated in the LAA and serves as a bumper to prevent guide catheter 1100 from perforating the wall of the LAA. These features may be similar to those described with respect to FIGS. 8-11.

[0304] FIG. 83 is a side view of an embodiment of over the wire circumferential ablation ultrasound balloon system. An over-the-wire balloon catheter 3035 is placed over a guidewire 3037 and into the LAA (LAA). A balloon 3045, such as a circumferential ablation ultrasound balloon, is used to electrically isolate the LAA using ultrasound (US) to treat atrial fibrillation. The guidewire 3037 may have attached to its distal end the balloon 3043, as described with respect to FIG. 82.

[0305] FIG. 84 is a side view of an embodiment of an over-the-wire circumferential ablation helical wire system with ablation elements. An over-the-wire circumferential ablation helical wire 3047 with one or more ablation elements is placed into the LAA (LAA). The wire 3047 can be used to electrically isolate the LAA using radiofrequency to treat atrial fibrillation.

N. Embodiments with Compressible Foam Body, Proximal Cover, and Compliant Frame Having Proximal Recapture Struts and Distal Tubular Body

[0306] FIGS. 85A-93B show another embodiment of an LAA occlusion device 3000. The device 3000 described herein may have the same or similar features and/or functionalities as other LAA occlusion devices described herein, and vice versa. Any of the features of the device 3000 described with respect to FIGS. 85A-93B may therefore apply to features of the devices described with respect to FIGS. 1-84, such as the implant 1020, and vice versa.

[0307] FIGS. 85A-85C show the LAA occlusion device 3000 having a foam body 3002, an expandable support or frame 3040, and a proximal cover 3100. FIG. 85D shows the LAA occlusion device 3000 additionally having an interior cover 3101 and proximal markers 3023A. FIGS. 86A-86C show the foam body 3002, with the body 3002 shown in cross-section in FIGS. 86B and 86C. FIG. 86C additionally includes the full view (i.e. non-cross section) of the frame 3040. The device 3000 is shown in an expanded configuration in these figures. The device 3000 has a longitudinal axis as shown, which may be defined by the foam body 3002, as further described.

[0308] 1. Compressible Foam Body

[0309] The body 3002 is formed from a compressible material, such as foam. The body 3002 may be a foam formed from reticulated (e.g. net-like) polycarbonate polyurethane-urea. The body 3002 may be cut, formed or assembled into a cup shape, as further described. The body 3002 may have a thickness and compressibility sufficient to

engage the surrounding tissue and conform to the anatomic irregularities under radial force applied by the inner frame, as further described. The use of a compressible material such as foam for the body 3002 provides a complete seal of the LAA and superior performance for LAA occlusion over existing devices, as further described. The structure of the foam of the body 3002 comprises a three dimensional network of interconnected reticulations, spaced apart to form a network of interconnected open pores, as further described. The reticulations can carry a coating, such as PTFE, while preserving the open pores, as further described.

[0310] The foam material of the body 3002 has a high porosity. "Porosity" as used herein has its usual and customary meaning and refers to open void content between the interconnected reticulations of the foam. The porosity of the body 3002 may be at least about 65%, at least about 70% at least about 75%, at least about 80%, at least about 85%, at least about 90%, at least about 95% or more. The porosity may be within the range of approximately 90-95%. The porosity may be approximately 90%. The porosity may be approximately 95%. The porosity may be 90%, 91%, 92%, 93%, 94%, or 95%. The high porosity promotes quick and tenacious tissue ingrowth, allows it to be compressed into a small catheter, and/or allows blood to pass if the implant embolizes, among other advantages.

[0311] The foam body 3002 has pores or cells formed between the interconnected reticulations of the foam material. The foam body 3002 has cells with sizes in the range of from about 250 μm to about 500 μm . The foam may have a cell size from about 125 μm to about 750 μm , from about 175 μm to about 650 μm , from about 200 μm to about 600 μm , from about 225 μm to about 550 μm , from about 275 μm to about 450 μm , less than 125 μm , or greater than 750 μm . These sizes may refer to the size of the cell prior to application of any coating, such as PTFE. The cell size may thus change, e.g. decrease, after application of the coating. The desired porosity and/or cell size may be determined based on allowing the passage of blood while blocking debris of a size capable of potentially causing ischemic stroke. The allowable size of such debris may drive the selection of the particular porosity and/or cell size. For example, the cell size from about 250 μm to about 500 μm may be based on prevention of debris of a particular size from passing through the body 3002.

[0312] In an embodiment, the foam body 3002 is made from a non-resorbable, reticulated, cross-linked, polycarbonate polyurethane-urea matrix, structurally designed to support fibrovascular tissue ingrowth, with a fully interconnected, macroporous morphology with over 90-95% void content and cell sizes ranging from 250 to 500 μm .

[0313] The body 3002 has a proximal end 3004 and a distal end 3006. In some embodiments, the axial length of the device 3000 from the proximal end to the distal end in a free, unconstrained state is 20 mm. As used herein, the "free, unconstrained" state, and the like, refers to a state of the device 3000 without any external forces applied to the device 3000 other than a normal or reactive force from a surface (e.g. table top) on which the device 3000 is placed. In some embodiments, this axial length may be from about 10 mm to about 30 mm, from about 12 mm to about 28 mm, from about 14 mm to about 26 mm, from about 16 mm to about 24 mm, from about 18 mm to about 22 mm, or about 20 mm. The body 3002 may have any of these lengths regardless of outer diameter of the body 3002.

[0314] The proximal end 3004 of the body 3002 has a proximal end wall or face 3008. The proximal face 3008 faces generally toward the LA when the device 3000 is implanted into the LAA. The device 3000 may be implanted off-axis, as further described, in which case the proximal face 3008 may not reside at a perpendicular to a longitudinal axis of the LA. The proximal face 3008 thus provides a closed proximal end 3004 of the body 3002. The closed proximal end 3004 is configured to span the ostium but the porosity, as further described, is sufficient to permit the passage of blood while blocking debris of a size capable of potentially causing ischemic stroke. This membrane may be formed by the body 3002 and/or the cover 3100. In some embodiments, the proximal face 3008 or portions thereof may be open. For example, there may not be a proximal face 3008, there may be a partial proximal face 3008, there may be a proximal face 3008 with portions removed, etc. In some embodiments, the proximal face 3008 or portions thereof is/are not included and any opening or openings is/are covered by the cover 3100. The size of any such openings in the proximal face 3008 may be driven by the desired size of embolic debris to be prevented from escaping the LAA, as further described.

[0315] The proximal face 3008 is flat or generally flat and generally perpendicular to the longitudinal axis of the device 3000. The proximal face 3008 has a circular or generally circular shape as viewed from the proximal end 3004 in an unconstrained expansion. In some embodiments, the proximal face 3008 may be flat, rounded, segmented, angled with respect to the longitudinal axis, other shapes, or combinations thereof. The proximal face 3008 may have a non-circular, polygonal, other rounded shape, other shapes, or combinations thereof, as viewed from the proximal end 3004.

[0316] The proximal face 3008 has an outer surface 3010 and an opposite inner surface 3012. The outer surface 3010 faces proximally away from the device 3000 and the inner surface 3012 faces distally toward the frame 3040. The surfaces 3010, 3012 may define outer and inner sides of the proximal face 3008. The thickness of the proximal face 3008 may be measured axially between the outer surface 3010 to the inner surface 3012. This thickness in a free, unconstrained state (e.g. uncompressed and expanded) may be from about 0.5 mm to about 5 mm, from about 1 mm to about 4 mm, from about 2 mm to about 3 mm, about 2.5 mm, or 2.5 mm. In some embodiments, the thickness may be less than 0.5 mm or greater than 5 mm. The thickness of the proximal face 3008 may be uniform or non-uniform. Thus the thickness may be greater or smaller in different regions of the proximal face 3008.

[0317] The body 3002 includes a sidewall 3014 extending distally from the proximal face 3008. The sidewall 3014 extends circumferentially about a perimeter of the proximal face 3008 to form a closed cross-section (i.e. extends circumferentially 360 degrees about the axis). The sidewall 3014 extends axially to define a tubular body concentric about the longitudinal axis of the device 3000. The longitudinal axis extends through a geometric center of the tubular body defined by sidewall 3014. The sidewall 3014 is tubular or generally tubular, e.g. cylindrical, along the axis. In some embodiments, the sidewall 3014 may be conical or frustoconical, for example where the proximal end is wider than the distal end or vice versa. The sidewall 3014 may have an outer profile at the proximal end thereof, and as

viewed from the proximal or distal end, to match that of the outer perimeter of the proximal face 3008.

[0318] In some embodiments, the cross-section of the sidewall 3014 may not be closed, for example where there are openings in the sidewall 3014. Thus cross-sections taken at various locations along the longitudinal axis may or may not show a closed section. In some embodiments, the sidewall 3014 may be non-tubular, non-cylindrical, non-circular, polygonal, other rounded shapes, other shapes, or combinations thereof. In some embodiments, as shown, the sidewall 3014 may extend continuously for the entire length from the proximal end 3004 to the distal end 3006. In some embodiments, the sidewall 3014 may not extend continuously for the entire length from the proximal end 3004 to the distal end 3006. For example, the sidewall 3014 may include a plurality of disconnected sections, such as annular portions of the sidewall, located and spaced along the longitudinal axis and connected to the frame 3040.

[0319] The sidewall 3014 has an outer surface 3016 and an opposite inner surface 3018. The outer surface 3016 faces radially outward from the axis. The inner surface 3018 faces radially inward toward the axis. The thickness of the sidewall 3014 may be measured radially between the outer surface 3016 to the inner surface 3018. This thickness in a free, unconstrained state (e.g. uncompressed) may be from about 0.5 mm to about 5 mm, from about 1 mm to about 4 mm, from about 2 mm to about 3 mm, about 2.5 mm, or 2.5 mm. In some embodiments, the thickness may be less than 0.5 mm or greater than 5 mm. The thickness of the sidewall 3014 may be uniform or non-uniform. Thus the thickness may be greater or smaller in different regions of the sidewall 3014. The thickness of the sidewall 3014 may be the same or different as the thickness of the proximal face 3008. In some embodiments, the thickness of the proximal face 3008 is 2.5 mm and the thickness of the sidewall 3014 is 2.5 mm. In some embodiments, the thickness of the proximal face 3008 is about 2.5 mm and the thickness of the sidewall 3014 is about 2.5 mm.

[0320] The sidewall 3014 has a distal free end 3020 having a distal surface 3022. The distal surface 3022 is flat or generally flat and perpendicular to the longitudinal axis of the device 3000. In some embodiments, the distal surface 3022 is non-flat, angled with respect to the axis of the device 3000, curved, rounded, segmented, other shapes, or combinations thereof.

[0321] The body 3002 may have a distal opening 3024. The opening 3024 is formed by the distal free end 3020 of the sidewall 3014. The opening 3024 is at a distal end of an internal central volume or cavity 3028 of the body 3002 that is formed at least partially by the sidewall 3014, the proximal face 3008 and/or the shoulder 3030. The frame 3040 may reside within the cavity 3028, as further described. The distal opening 3024 may be completely open. In some embodiments, the distal opening 3024 may be mostly open, partially open, or closed, for example where the body 3002 has a distal face similar to the proximal face 3008 to enclose or partially enclose the cavity 3028.

[0322] The body 3002 has a shoulder 3030, shown as a bevel, that extends between the proximal face 3008 to the sidewall 3014. The shoulder 3030 may be an intersection of a proximal end of the sidewall 3014 and the proximal face 3008. The shoulder 3030 extends circumferentially about the entire perimeter of the intersection. The shoulder 3030 has an outer surface 3032. The outer surface 3032 may be a

beveled surface. The outer surface 3032 is flat or generally flat in an axial direction. The outer surface 3032 extends circumferentially about the entire perimeter of the shoulder 3030. In some embodiments the shoulder 3030 and/or outer surface 3032 may be non-flat, rounded, other shapes in an axial direction, or combinations thereof. The shoulder 3030 and/or outer surface 3032 may extend circumferentially less than the entire perimeter of the shoulder 3030. The thickness of the shoulder 3030 may be measured inward perpendicularly to the outer surface 3032. The thickness of the shoulder 3030 may be the same as the thicknesses of the proximal face 3008 and/or the sidewall 3014, as described herein. In some embodiments, the thickness of the shoulder 3030 may be different from the thicknesses of the proximal face 3008 and/or the sidewall 3014. The shoulder 3030 may function as a recapture ramp, to facilitate drawing the implant proximally into the deployment catheter.

[0323] The compressibility of the body 3002 contributes to the superior sealing capability of the device 3000. The foam may be compressible to provide a larger radial “foot-print” and spread out the radial forces from struts on the frame 3040, as further described. The foam body 3002 may have a compressive strength of at least 1 pound per square inch (psi) or within a range of about 1 psi to about 2 psi, or no more than about 2 psi. The “compressive strength” here refers to the pressure to compress the foam to 50% strain. With some foam materials for the body 3002, the pressure may not change from 50% strain through at least 80% strain, and the relation of pressure versus strain may be flat or generally flat. Thus, even with thicker foams for the body 3002, the body 3002 will not exert much more outward force on the tissue due to the increased thickness by itself. In an embodiment, the foam body 3002 is a reticulated, cross linked matrix having at least about 90% void content, an average cell size within the range of from about 250-500 microns, a wall thickness of at least about 2 mm and a compressive strength of at least about 1 psi. In an embodiment, the body 3002 is formed from a foam material having or substantially having the material properties indicated in Table 1. In some embodiments, the body 3002 is formed from materials described in, for example, U.S. Pat. No. 7,803,395, issued Sep. 28, 2010, and titled “Reticulated elastomeric matrices, their manufacture and use in implantable devices,” or U.S. Pat. No. 8,337,487, issued Dec. 25, 2012, and titled “Reticulated elastomeric matrices, their manufacture and use in implantable devices,” the entire disclosures of which are incorporated herein by reference.

TABLE 1

Example material properties for an embodiment of foam material that may be used for the foam body 3002.	
Material Property	Value
Permeability	311 Darcy
Average Cell Size	377 μm
Density	2.7 lb/ft ³
Compressive Strength	1.1 psi
Tensile Strength Parallel	68 psi
Tensile Strength Perpendicular	32 psi
Elongation Parallel	219%
Elongation Perpendicular	243%

[0324] The device 3000 may include markers 3023 (see FIGS. 85B and 87D); for clarity only some of the markers 3023 are labelled in the figures) to facilitate visualization

during delivery. The markers 3023 may be radiopaque marker bands sewn into the distal free end 3020 of the body 3002. The markers 3023 may be for visualization using fluoroscopy imaging of the distal end 3006 of the device 3000 during delivery. There may be a series of the markers 3023 located circumferentially along the distal surface 3022 of the body 3002 (for clarity, only some of the markers 3023 are labelled in FIG. 85B). In some embodiments, the markers 3023 may additionally or alternatively be located in other areas of the body 3002 and/or on other parts of the device, such as the cover 3100 or frame 3040.

[0325] In some embodiments, four platinum iridium (PtIr) radiopaque (RO) tubular markers 3023 are sewn onto the distal end 3006 of the foam body 3002 to enable visualization of the distal edge of the device 3000 under fluoroscopy. In some embodiments, a PtIr marker 3023 is attached to the foam body 3002 at the location of the proximal shoulder 3030 to use as a marker during recapture of the device 3000. Visualization of the proximal and/or distal markers 3023 may facilitate with identifying the amount of recapture. If the device 3000 is recaptured up to but not including the anchors proximal 3090 inside the access sheath, the device 3000 can be redeployed and reused. If the proximal anchors 3090 are recaptured into the access sheath, the device 3000 may be removed and discarded due to permanent deformation of the anchors 3090. In some embodiments, other materials may be used for the markers 3023, such as gold or other suitable materials.

[0326] As shown in FIGS. 85D and 87D, the device 3000 may include one or more markers 3023A. As one example only, there are three markers 3023A shown. In some embodiments, there may be one marker 3023A. There may be two, four, five or more markers 3023A. In some embodiments, there is one proximal marker 3023A and ten of the distal markers 3023. The markers 3023A may have the same or similar features and/or functionalities as other markers described herein, for example the marker 3023, and vice versa, except as otherwise noted. The markers 3023A may be located at or near the proximal end of the device 3000. As shown, the markers 3023A are located on an inner surface 3012 of the proximal end 3004 of the foam body 3002. The markers 3023A may be located at or near an inner surface of a shoulder 3030 (see FIG. 86B) of the foam body 3002. The markers 3023A may be distributed circumferentially, for example equidistant or equiangular, relative to each other, or they may be at different relative distances from each other. They may be radially located at the same or different location relative to each other. In some embodiments, there is only one marker 3023A. There may be one proximal marker 3023A and four of the distal markers 3023. The one or more markers 3023A may be on the inside, outside, or within the foam body 3002, or combinations thereof. The one or more markers 3023A may be located on or at the distal surface 3022 of the foam body 3002. The markers 3023A may be elongated circumferentially as shown. In some embodiments, the markers 3023A may be linear when the device 3000 is viewed from a particular angle, such as a side view. The markers 3023A may be aligned or oriented in the same or similar orientation, or in different orientations. Some, none, or all of the markers 3023A may be oriented circumferentially, laterally, axially (for example along an inner surface 3018 of the sidewall 3014), other orientations, or combinations thereof.

[0327] As further shown in FIG. 87D, there may be one or more markers 3023B. The one or more markers 3023B may have the same or similar features and/or functionalities as the other markers described herein, such as the marker 3023 or 3023A and vice versa, except as otherwise noted. The markers 3023B may be located along the sidewall 3014 of the body 3002. There may be one or more markers 3023B located along an inner surface 3018 of the sidewall 3014.

[0328] As shown, two markers 3023B are visible on either side of the interior of the foam body 3002. The markers 3023B are attached through the foam and around the frame 3040. The marker 3023B may be attached, for example sutured, around a proximal face 3060 member of the frame 3040, such as one of the struts 3061. The marker 3023B may be attached to the frame 3040 just proximally of one of the proximal apices 3084 of the frame 3040, for example at an outer curved portion 3066 of the strut 3061. There may be only one marker 3023B, or two, three, four or more markers 3023B. There may be one of the markers 3023B for each strut 3061. The markers 3023B may be used additionally to connect the frame 3040 with the foam body 3002. The markers 3023B may be sutures as described herein.

[0329] The one or more markers 3023A and/or 3023B at or near the proximal end of the device 3000 provide various desirable features. For instance, the marker 3023A at the shoulder 3030 facilitates visualization of the device 3000 during and after implantation. The typically non-circular shape of the opening of the LAA (ostium) may compress the proximal end 3004 of the device and cause the proximal end 3004 to protrude slightly in the proximal direction. However, the shoulder 3030 may provide a location for the marker 3023A where linear bulging of the foam body 3002 in the proximal direction is reduced or prevented. Thus, the marker 3023A in that location can provide a more useful visualization of the positioning of the device 3000 and reduce complexity. For example, in some embodiments, the marker 3023A at the shoulder 3030 (e.g. on an inner surface as shown) may be particularly useful during delivery, allowing for delivery using fluoroscopy imaging only without the need for echo or other ultrasound imaging. The one or more markers 3023B may provide similar benefits.

[0330] As further shown in FIGS. 85D and 87D, the device 3000 may include an inner cover 3101. The inner cover 3101 may have the same or similar features and/or functionalities as the cover 3100 (described in further detail below, see section "Proximal Cover"), except as otherwise described. The inner cover 3101 may be a cover for the hub 3050 (see, e.g., FIGS. 86C and 89A-90C). The inner cover 3101 may be formed from expanded Polytetrafluoroethylene ("ePTFE"). The inner cover 3101 may be a separate portion of the same material as the proximal cover 3100.

[0331] The inner cover 3101 may be located between the foam body 3002 and the frame 3040. As shown, the inner cover 3101 is located between the inner surface 3012 of the foam body 3002 and a proximal end of the hub 3050 of the frame 3040. The inner cover 3101 may be circular or other shapes. The inner cover 3101 may have an area sufficient to provide a barrier in between the hub 3050 and the proximal end 3004 of the foam body 3002. In some embodiments, the inner cover 3101 may extend radially to an outer circumference of the hub 3050, or it may extend radially to the sidewall 3014 such as to an inner surface 3018 of the foam body 3002, or to any radial locations in between. The inner cover 3101 may have a diameter from about 4 mm to about

22 mm, from about 5 mm to about 15 mm, from about 6 mm to about 10 mm, about 8 mm, or 8 mm. The inner cover 3101 may be flat or generally flat. The inner cover 3101 may have a thickness from about 0.0001"-0.0020", from about 0.0002"-0.0010", about 0.0005", or 0.0005" thick. The inner cover 3101 may include one or more openings 3103 such as holes therethrough. The inner cover 3101 may include two holes 3103 to receive therethrough a tether 3240 (see, e.g., FIGS. 93A-93B). The two holes 3103 in the cover 3101 may align the tether 3240, such as a suture, that extends distally into the hub 3050 through one hole 3103 in the inner cover 3101 and exits proximally back out of the hub 3050 through the other hole 3103 of the inner cover 3101.

[0332] The inner cover 3101 may prevent the hub 3050 and/or other features of the frame 3040 from directly contacting the foam material. The cover 3101 may protect the integrity of the foam body 3002 from stresses that may be imparted by the hub 3050 on the foam material. This protection may be desirable for example during loading, deployment, retrieval, re-deployment, etc. of the device 3000. The inner cover 3101 may prevent or reduce damage to the foam body 3002 from the hub 3050.

[0333] The foam body 3002 may be attached to various features of the device 3000. The body 3002 may be attached to the frame 3040 at numerous points, including for example the center of the proximal end of the frame 3040, as further described herein. Attachment can be done using suture, such as polypropylene monofilament suture, although other methods known in the art such as adhesive bonding could be utilized. The proximal row of proximal anchors 3090 may be individually attached to (e.g. inserted through) the foam body 3002 to prevent relative movement between the foam body 3002 and the frame 3040. In other embodiments, the foam body 3002 could be formed around the endoskeleton so that the metallic frame is within the foam body 3002, eliminating the need for a secondary attachment step. Attachment of the body 3002 to the frame 3040 promotes retrieval without damage to the foam body 3002, among other advantages. The attachment also ensures that a bumper 3026, further described herein, extends beyond the frame 3040 at all times, including during initial exposure of the device 3000 upon proximal retraction of the delivery sheath.

[0334] As shown in FIG. 87D, the device 3000 may include one or more attachments 3001. The attachments 3001 may connect the frame 3040 with the foam body 3002. The attachments 3001 may be sutures. Other suitable attachment structures may be used, including staples, ties, wires, components of the frame 3040, other mechanical attachments, adhesives, other suitable means, or combinations thereof. The attachments 3001 may extend around the frame 3040 and through the foam body 3002, for example through the sidewall 3014.

[0335] As shown, four attachments 3001 are visible in FIG. 87D. There are two proximal attachments 3001 and two distal attachments 3001 visible. The proximal attachments 3001 are each located at the base of a respective proximal anchor 3090. The distal attachments 3001 are each located at the base of a respective distal anchor 3094. There may be one, two, three, four, five, six, seven, eight, or more attachments 3001. There may be twenty attachments 3001. There may be one of the attachments 3001 for each anchor 3090, 3094 of the device 3000. The attachments 3001 may each be located at a proximal apex 3084 or at a distal apex 3088 of the frame 3040, as further described herein, for example

with respect to FIG. 89A. For example, the attachments 3001 may be wrapped around one or more of the struts 3082, 3086, as further described herein. The attachments 3001 may locally compress the foam body 3002 at and/or around the location of attachment, as further described herein, for example with respect to FIG. 95C. The attachment 3001, such as a suture, may extend from within the cavity 3028, through the foam body 3002, exit the foam body 3002 and extend along the outer surface 3016 of the foam body 3002, extend back into and through the foam body 3002 into the cavity 3028, and be tied or otherwise connected together around the frame 3040. In some embodiments a similar routing of the attachments 3001 may be used with the attachment 3001 tied or otherwise connected together around and outside the foam body 3002. In some embodiments the attachments 3001 may also extend through the cover 3300, or other covers as described herein. The attachments 3001 may extend through the material of the cover 3300. The attachments 3001 may extend through openings in the cover 3300, such as the side openings 3324, or windows 3177 (see, e.g., FIGS. 88B-88E). As shown, the proximal attachments 3001 may extend through the foam body 3002 and through openings in the cover 3300, and the distal attachments 3001 may not extend through the cover 3300 but only through the foam body 3002.

[0336] The foam body 3002 may include a coating. In some embodiments, there may not be a coating. In embodiments with a coating, the coating is applied to the interconnected reticulations of the foam material. The body 3002 may be coated with pure polytetrafluoroethylene (PTFE). The PTFE coating minimizes the thrombogenicity of the LA surface, while also reducing the friction of the foam body 3002 against the delivery system to facilitate ease of deployment and retrieval. The body 3002 may be coated with conformable, vacuum deposited, pure PTFE. In addition or alternatively, the body 3002 may be coated with a coating other than PTFE. The coating, whether PTFE or otherwise, may be about 0.5 μm thick, and covers at least a portion of the surface of the interconnected reticulations of the foam without occluding the pores. The coating may be applied to some or all of the foam body 3002. The coating may be applied to some or all of the outer surfaces of the foam body 3002.

[0337] In some embodiments, the thickness of the coating is from about 0.1 μm to about 1 μm , from about 0.2 μm to about 0.9 μm , from about 0.3 μm to about 0.8 μm , from about 0.4 μm to about 0.7 μm , about 0.4 μm to about 0.6 μm , or about 0.5 μm thick. In some embodiments, greater or smaller thicknesses of the coating may be applied. The coating has a uniform or substantially uniform thickness. In some embodiments, the coating may have a non-uniform thickness. For example, the portion of the body 3002 facing the LA when implanted, such as the proximal face 3008 and/or shoulder 3030, may have a thicker coating relative to a coating along the sidewall 3014 of the body 3002. In some embodiments, the outer surface 3010 of the proximal face 3008 has a PTFE coating and the proximal face 3008 also has a ePTFE cover 3100.

[0338] The coating is applied using a vapor deposition process. In some embodiments, the coating is applied through coating, vapor deposition, plasma deposition, grafting, other suitable processes, or combinations thereof. The coating is applied to the outer surfaces 3010, 3032 and 3016 of, respectively, the proximal face 3008, the shoulder 3030

and the sidewall 3014. In some embodiments the coating is applied to the outer surfaces 3010, 3032 and only partially on the outer surface 3016. In some embodiments the coating is applied to outer and inner surfaces of the body 3002.

[0339] In some embodiments, other biocompatible, thromboresistant and/or lubricious materials could be applied to the surface(s) of the foam body 3002 and/or the cover 3100. These materials may encourage tissue ingrowth. Such materials may include, for example, heparin, albumin, collagen, polyethylene oxide (PEO), hydrogels, hyaluronic acid, materials that release nitric oxide, oxygen, nitrogen, amines, bioabsorbable polymers, and other biomaterials, pharmacologic agents, and surface modification materials. Additionally, the surface(s) of the body 3002 could be roughened, textured, or otherwise modified or coated to promote healing or to make it more echogenic.

[0340] 2. Proximal Cover

[0341] The device 3000 may include a cover 3100, which may be an ePTFE cover as further described. Other embodiments for this outer cover 3100 are described herein, for example the cover 3101, 3300, 3150, 3151, etc. The various embodiments of the cover may have the same or similar features and/or functionalities as each other, except as otherwise noted. The cover 3100 may have a series of openings. In some embodiments, the cover 3100 may be solid and not have any openings. In some embodiments, the cover 3100 may only have openings to receive anchors and/or a tether therethrough, as further described herein. In some embodiments, the device 3000 may include an inner cover such as an inner cover 3101, as shown and described with respect to FIG. 85D.

[0342] The outer cover 3100 is a generally flat material applied over and covering at least a portion of the body 3002. The cover 3100 is on the proximal end 3004 of the device 3000. The cover 3100 covers the proximal face 3008 of the body 3002 and at least part of the sidewall 3014. The cover 3100 covers a proximal portion of the sidewall 3014. The cover 3100 has a proximal surface 3102 that at least partially faces the LA when implanted. The cover 3100 has an outer edge 3104 forming outer vertices 3106 (for clarity, only some of the outer edges 3104 and outer vertices 3106 are labelled in the figures). In some embodiments, the cover 3100 may cover only the proximal face 3008 or portions thereof. In some embodiments, the cover 3100 may extend over more of the sidewall 3014, such as the middle or distal portion thereof, or the entire sidewall 3014.

[0343] The cover 3100 may have a thickness measured perpendicularly from the proximal surface 3102 to an opposite distal surface of the cover 3100 that faces the body 3002. The cover 3100 may have a thickness of 0.001" (inches). In some embodiments, the cover 3100 may have a thickness from about 0.00025" to about 0.005", from about 0.0003" to about 0.004", from about 0.0004" to about 0.003", from about 0.0006" to about 0.002", from about 0.0008" to about 0.0015", or about 0.001". In some embodiments, the cover 3100 may have a thickness of 0.0005". In some embodiments, the cover 3100 may have a thickness from about 0.0002" to about 0.0008", from about 0.0003" to about 0.0007", from about 0.0004" to about 0.0006", or about 0.0005".

[0344] The cover 3100 may be attached to the frame 3040 through the foam body 3002. The cover 3100 may in addition or alternatively be attached to the body 3002. The cover 3100 may be attached at least two or four or six or

more of the outer vertices **3106**. The cover **3100** may be attached to the frame **3040** and/or body **3002** at various locations, including at the outer vertices **3106**, through the proximal surface **3100**, at the proximal face **3008** of the body **3002**, other locations, or combinations thereof. The cover **3100** is attached using mechanical attachments, such as sutures. In some embodiments, polypropylene 6-0 sutures are used throughout the device to attach the foam body **3002**, proximal cover **3100**, and RO markers **3023** to the foam body **3002** and/or frame **3040**. In some embodiments, the cover **3100** is attached to the frame **3040** via standard braided or monofilament suture material, such as polypropylene, ePTFE, or polyester. In some embodiments, a polypropylene monofilament is utilized. Proximal anchors **3090** of the frame **3040** (further described herein) may extend through the outer vertices **3106** of the cover **3100**. Such penetrating anchors **3090** may further secure the cover **3100** in place relative to the body **3002**. In some embodiments, the cover **3100** may be attached to the various parts of the device **3000** with mechanical attachments, fasteners, adhesives, chemical bonds, other suitable techniques, or combinations thereof.

[0345] As shown, the cover **3100** is formed from expanded Polytetrafluoroethylene ("ePTFE"). An ePTFE cover **3100** provides many advantages. For example, the ePTFE cover **3100** may enhance the ability to recapture the device **3000** in vivo by distributing the proximal retraction forces applied by the catheter. The cover **3100** may be an ePTFE material approximately 0.001" thick, with the appropriate porosity to encourage healing and minimize thrombus formation, similar to the underlying PTFE coated foam.

[0346] An ePTFE cover **3100** may assist in recapture of the implant into the access sheath while providing a smooth, thromboresistant surface which encourages tissue coverage and integration. The ePTFE may cover the entire proximal face and partially covers the sides, as shown in FIG. **85C**. The ePTFE cover **3100** is fabricated from a previously laminated sheet comprised of two or more sheets of oriented material, offset to form a biaxially orientated material. Alternatively, one could use a tube, preferably biaxially oriented, that is then cut to form a sheet. The thickness of the final construct can be from 0.0005"-0.005" but is preferably about 0.001".

[0347] In some embodiments, the cover **3100** is fabricated from other thromboresistant, high strength, biocompatible materials, such as knitted or woven polyester fabrics, polypropylene, polyethylene, non-woven vascular scaffolds, porous films, or bioabsorbable scaffolds such as polylactic acid, polyglycolic acid, and co-polymers. The shape of the cover prior to attachment with the device **3000**, such as shown in FIGS. **88A** and **88B**, minimizes wrinkling and provides a smooth surface following attachment to the implant. This shape may be a star shape, an outer pointed shape, or other shapes.

[0348] The cover **3100** may be perforated with a series of openings **3120** (for clarity, only some of the openings **3120** are labelled in the figures). The openings **3120** are perforations or holes formed in the cover **3100** via laser or mechanical cutting. The openings **3120** include proximal openings **3122** and side openings **3124** (for clarity, only some of the proximal openings **3122** and side openings **3124** are labelled in the figures). When the cover **3100** is assembled with the body **3002**, the proximal openings **3122** are located over the proximal face **3008** and/or shoulder **3030**, and the side

openings **3124** are located over the sidewall **3014**. In some embodiments, the cover **3100** includes forty proximal openings **3122**. In some embodiments, the cover **3100** includes forty side openings **3124**. The number of openings **3120** located over the proximal face **3008** and/or shoulder **3030** when assembled with the body **3002** may range from ten to eighty, from twenty to seventy, from thirty to sixty, from thirty five to fifty, or forty openings **3120**. The number of openings **3120** located over the sidewall **3014** may range from ten to eighty, from twenty to seventy, from thirty to sixty, from thirty five to fifty, or forty openings **3120**.

[0349] The openings **3120** may have a variety of sizes. The openings **3120** are 0.070" in width, e.g. minor axis, or diameter for circular openings. The openings **3120** may have a width from about 0.010" to about 0.200", from about 0.020" to about 0.150", from about 0.030" to about 0.110", from about 0.040" to about 0.100", from about 0.050" to about 0.090", from about 0.060" to about 0.080", or about 0.070". In some embodiments, the width may be less than 0.010" or greater than 0.200", such as 0.25", 0.5" or greater. These widths may apply to circular as well as non-circular shaped openings **3120**.

[0350] In some embodiments, the openings **3120** may be various shapes. The openings **3120** may be elongated slots. The openings **3120** may extend radially along the cover **3100** from or near a center portion of the proximal surface **3102** toward and/or to the outer edge **3104**. The openings **3120** may be annular openings extending circumferentially along the cover **3100** and having varying radial positions. The openings **3120** may be of uniform size and shape. Some of the openings **3120** may have varied sizes and/or shapes with respect to other of the openings **3120**. The openings **3120** may have various distributions or concentrations about the cover **3100**. For example, the openings **3120** may be more densely located in various areas, such as along the proximal surface **3102** that faces the LA, along the shoulder **3030**, etc.

[0351] The openings **3120** enable blood to flow through the device **3000**. The openings **3120** may allow blood to adequately flow through the device **3000** and thereby mitigate the risk of occlusion in the bloodstream should the device **3000** embolize within the vasculature system. In some embodiments, should the device **3000** embolize, it may act as a stationary filter at low pressures but may pass through the bloodstream at higher pressures. In some embodiments, the device **3000** allows for about two to about fourteen liters, from about four to about twelve liters, from about six to about ten liters, or from about eight liters per minute of blood to pass at <30 mmHg pressure drop to prevent shock in the event of a device embolization. In some embodiments, there are forty circular openings **3120** each having a diameter of 0.070", and allowing for approximately eight liters per minute of blood to pass at <30 mmHg pressure drop. In some embodiments, the proximal end of the device **3000** may be a foam layer such as the foam proximal face **3008** or a membrane such as the cover **3100** or both, enclosing the cavity **3028** defined within the tubular side wall **3014** of the body **3002**.

[0352] In one implementation, having both the foam proximal face **3008** and the cover **3100**, the foam body **3002** has the open cell structure further discussed herein that can permit the passage of blood but block escape of embolic debris. The cover **3100** may be occlusive to blood flow, and is present to provide structural integrity and reduced friction

for retracting the expanded body **3002** back into the deployment catheter. In one implementation, the cover **3100** is ePTFE in a form that is substantially occlusive to blood flow, as described. In this embodiment, the cover **3100** is therefore provided with a plurality of perfusion windows or openings **3120**, so that blood can pass through the open cell foam and cover **3100** but the device **3000** still benefits from the other properties of the cover **3100**.

[0353] In some embodiments, the device **3000** may allow for a particular flow rate of water at specified conditions, to test the perfusion performance of the device **3000**. The device **3000** may have the foam body **3002** and cover **3100** configured to allow for a flow rate of water axially through the device **3000** of at least four liters per minute. The water may be at sixty-eight degrees Fahrenheit (F) or about sixty-eight degrees F. and an upstream pressure of twenty-five millimeters of Mercury (mmHg) or about twenty-five mmHg. In some embodiments, the device **3000** may be configured to allow for flow rates under such conditions from about one liter to about seven liters, from about two liters to about six liters, from about three liters to about five liters, more than two liters, more than three liters, or more than four liters of water per minute. The particular flow rate may depend on the porosity of the foam body **3002** and the open area of the cover **3100**. The particular flow rate may depend on the inner cover **3101** features as well. The cover **3100** may have particular percentages of the cover area open with the series of openings, as further described herein, to attain a particular desired flow rate. The flow rate of water at the specified conditions may be used to extrapolate or otherwise calculate the corresponding expected flow rate of blood in the body through the device **3000** should it embolize, as described herein. The device **3000** may allow for a cardiac index from about 1.6-2.4, from about 1.7-2.3, from about 1.8-2.2, from about 1.9-2.1, about 2.0, or 2.0, liters per minute per square meter. The device **3000** may have these and other flow rate capabilities either aligned or approximately aligned with the direction of flow of the fluid, or off-axis where the device **3000** is angled with respect to the direction of flow of the fluid (a flow axis), as further discussed herein for example in the section "Off-Axis Delivery and Deployment."

[0354] FIGS. 87A-87C depict an embodiment of the LAA occlusion device **3000** having another embodiment of a cover **3300**. The device **3000** includes the foam body **3002** and the frame **3040**, and features thereof, as described herein, and additionally includes the cover **3300**. The cover **3300** may have the same or similar features and/or functionalities as the cover **3100**, and vice versa. The cover **3300** is on the proximal end **3004** of the device **3000**. The cover **3300** covers the proximal face **3008** of the body **3002** and a proximal part of the sidewall **3014**. The cover **3300** has a proximal surface **3302**. The cover **3300** has an outer edge **3304** forming a plurality of at least two or four or six or eight or ten or more outer vertices **3306** (for clarity, only some of the outer vertices **3306** are labelled in the figures). The cover **3300** is attached to the body **3002** at the outer vertices **3306**. The proximal anchors **3090** extend through side openings **3324** in the outer vertices **3106** of the cover **3100**.

[0355] The cover **3300** includes a series of openings **3320**. The openings **3320** include proximal openings **3322**, shoulder openings **3323**, and the side openings **3324**. The proximal openings **3322** are located over the proximal end **3004** of the body **3002**. The shoulder openings **3323** are located

over the shoulder **3030**, e.g. a bevel, of the body **3002**. The side openings **3324** are located over a proximal portion of the sidewall **3014** of the body **3002**. The proximal anchors **3090** may extend through the side openings **3324** that are located in the outer vertices **3106**. The openings **3320** may have the same or similar features and/or functionalities as the openings **3120**, and vice versa. In some embodiments, the proximal anchors **3090** may extend through the cover **3300** material at or near the outer vertices **3106**.

[0356] FIG. 88A shows another embodiment of a cover **3150** that may be used with the device **3000**. The cover **3150** may have the same or similar features and/or functionalities as the cover **3100** and/or cover **3300**, and vice versa. The cover **3150** may be used to cover the proximal face **3008** of the body **3002** and part of the sidewall **3014**. The cover **3150** has a proximal surface **3152**. The cover **3150** has an outer edge **3154** forming outer vertices **3156**. The cover **3150** may be attached to the body **3002** at the outer vertices **3156**. The proximal anchors **3090** may extend through the outer vertices **3156** of the cover **3100**. The cover **3150** includes a series of openings **3170**. The openings **3170** include proximal openings **3172** and side openings **3174** (for clarity, only some of the openings **3170**, **3172**, **3174** are labelled in the figures). When the cover **3150** is assembled with the body **3002**, the proximal openings **3172** are located over the proximal end **3004** and the side openings **3174** are located over the sidewall **3014**. As shown, the openings **3174** may be substantially uniformly located along the cover **3150** except for a center region of the proximal surface **3152**.

[0357] FIG. 88B is a top view of another embodiment of a proximal cover **3151** that may be used with the various LAA occlusion devices described herein. FIG. 88C is a top view showing the cover **3151** assembled with the device **3000**. The cover **3151** may have the same or similar features and/or functionalities as other covers described herein, such as the cover **3100** and/or cover **3300**, and vice versa, except as otherwise noted. For example, the cover **3151** may include the proximal surface **3152** and outer edge **3154** forming outer vertices **3156**.

[0358] The cover **3151** further includes another embodiment of a series of openings **3171**. The openings **3171** include smaller openings **3175** and larger openings **3173**. The openings **3175**, **3173** may have the same or similar features and/or functionalities as other cover openings described herein, such as the openings **3120**, **3122**, **3124**, **3320**, **3322**, **3324**, **3170**, **3172** and/or **3174**, and vice versa. The smaller openings **3175** may be relatively smaller, in width and/or area, than the larger openings **3173**. There may be openings with widths or areas smaller than that of the smaller openings **3175**, larger than that of the larger openings **3173**, or anywhere in between. As shown, the openings **3173**, **3175** may be generally uniformly distributed about the proximal surface **3152** of the cover **3151**. The openings **3173**, **3175** may be circumferentially evenly spaced or approximately evenly spaced about the cover **3151**.

[0359] There may be a variety of different quantities of each of the openings **3173**, **3175**. There may be a total of ten, twenty, thirty, forty, fifty, sixty, seventy, eighty, ninety, one hundred, one hundred fifty, two hundred, three hundred, four hundred, or more openings of the series of openings **3171**, or any lesser, greater or in between number of openings. The series of openings **3171** may be holes as shown. They may have circular shapes. They may have other shapes, including non-circular, segmented, other shapes, or combinations

thereof. The openings **3171** may all have the same general shape or different shapes. In some embodiments, there may not be any holes in the cover **3151**.

[**0360**] When the cover **3151** is assembled with the foam body **3002**, the large and small openings **3173**, **3175** may be located over the proximal end **3004** and/or the sidewall **3014** of the foam body **3002**. When assembled with the foam body **3002**, on the proximal-facing portion of the cover **3151**, there may be a collective total of one hundred forty or about one hundred forty openings **3173**, **3175**. On this proximal-facing portion of the cover **3151**, there may be a collective total from about ten to about three-hundred, from about fifty to about two hundred fifteen, from about one hundred ten to about one hundred seventy, from about one hundred twenty to about one hundred sixty, from about one hundred thirty to about one hundred fifty, or from about one hundred thirty-five to about one hundred forty-five openings **3173**, **3175**. On this proximal-facing portion of the cover **3151**, there may be from about thirty to about fifty, from about thirty-five to about forty-five, about forty, or forty of the larger openings **3173**. On this proximal-facing portion of the cover **3151**, there may be from about sixty to about one hundred forty, from about eighty to about one hundred twenty, from about ninety to about one hundred ten, about one hundred, or one hundred of the smaller openings **3175**.

[**0361**] When assembled with the foam body **3002**, on the portion of the cover **3151** located over and/or near the shoulder **3030**, such as over the outer surface **3032** of the foam body **3002** (see, e.g., FIG. **86B**), there may be from about five to about eighty, from about ten to about forty, from about fifteen to about thirty, about twenty, or twenty of the smaller openings **3175**. In some embodiments, at this same portion of the cover **3151**, there may be from about five to about eighty, from about ten to about forty, from about fifteen to about thirty, about twenty, or twenty of the larger openings **3173**.

[**0362**] When assembled with the foam body **3002**, on the portion of the cover **3151** located over and/or near the sidewall **3014**, such as over the outer surface **3016** of the foam body **3002** (see, e.g., FIG. **86B**), there may be from about five to about eighty, from about ten to about forty, from about fifteen to about thirty, about twenty, or twenty of the larger openings **3173**. In some embodiments, at this same portion of the cover **3151**, there may be from about five to about eighty, from about ten to about forty, from about fifteen to about thirty, about twenty, or twenty of the smaller openings **3175**.

[**0363**] The larger and smaller openings **3173**, **3175** may have a variety of different sizes, for example as described herein with respect to the openings **3122**. In some embodiments, the openings **3173**, **3175** may have diameters ranging from about 0.025 inches to about 0.040 inches. In some embodiments, the larger openings **3173** may be 0.040 inches or about 0.040 inches in diameter. The larger openings **3173** may be from about 0.030 inches to about 0.050 inches, or from about 0.035 inches to about 0.045 inches, in diameter. These values may also refer to the widths, for example maximum widths, of non-circular larger openings **3173**. In some embodiments, the smaller openings **3175** may be 0.025 inches or about 0.025 inches, in diameter. The smaller openings **3175** be from about 0.015 inches to about 0.035 inches, or from about 0.020 inches to about 0.030 inches, in

diameter. These values may also refer to the widths, for example maximum widths, of non-circular smaller openings **3175**.

[**0364**] The series of openings **3171** may be configured to provide a desired amount of open area through the cover **3151**. This open area refers to the total area of certain openings in the cover **3151**. The cover **3151** may be covering a proximal face **3008** at the proximal end **3004** of the foam body **3002**. The open area may refer to openings through the portion of the cover that is over the proximal face **3008** of the foam body **3002** when assembled with the foam body **3002**. The series of openings in the various covers described herein may collectively provide the open area. For example, the series of openings **3171** in the cover **3151** over the proximal face of the foam may collectively provide an open area. This is the sum of the area of the openings in the cover **3151** over the proximal face. As further example, the open area may be the sum of the proximal openings **3122** of the cover **3100**. As further example, the open area may be the sum of the proximal openings **3322** of the cover **3300**.

[**0365**] The open area may be at least five percent of the area of the proximal face **3008** of the foam body **3002**. The open area may be at least six, at least seven, at least eight, at least nine, at least ten, at least eleven, at least twelve, at least thirteen, at least fourteen percent, at least fifteen, at least sixteen, at least seventeen, at least eighteen, at least nineteen, at least twenty, at least twenty-five, at least thirty, at least forty, or at least fifty percent, of the area of the proximal face **3008**. The open area may be from about one to about fifty percent, from about five to about twenty percent, from about eight to about fifteen percent, from about ten to about twelve percent, or about eleven percent, of the area of the proximal face **3008**. The “area” of the proximal face **3008** is understood here to refer to an area equal to $\text{Pi} \times R^2$, where R is the radius of the proximal face **3008** and extends perpendicularly from the longitudinal axis of the device **3000**. Further, “ R ” may be measured to the inner boundary of the shoulder **3030**, to the outer boundary of the shoulder **3030**, or to the outer surface **3016** of the sidewall **3014**. Further, as mentioned, some embodiments may not include a cover at all.

[**0366**] The cover **3151** may include one or more windows **3177**. As shown, there may be ten windows **3177**. There may be one window **3177** for each proximal anchor **3090**. There may be four, six, eight, twelve, fourteen or more windows **3177**, or any lesser or in between number. The windows **3177** may be openings in the cover **3151**. The windows **3177** may be located at or near the outer edge **3154** of the cover **3151**. The windows **3177** may be located along portions of the outer edge **3154**, for example at or near the outer vertices **3156**. The windows **3177** may have a shape conforming to the shape of the cover **3151** at the respective portions of the outer edge **3154**. As shown, the window **3177** may be diamond or generally diamond shaped. The window **3177** may be square, rectangular, triangular, rounded, circular, segmented, flattened diamond, other polygonal shapes, other shapes, or combinations thereof. The cover **3150** may be attached to the body **3002** at the outer vertices windows **3177**. The windows **3177** may have the same or similar feature and/or functionalities as the side openings **3324**, described and shown in FIG. **87B**. The proximal anchors **3090** may extend through the windows **3177** of the cover **3151** to retain the cover **3151** on the device **3000**.

[0367] FIG. 88D-88E are side and perspective views, respectively, of another embodiment of a proximal cover 3153 shown assembled with the device, that may be used with the various LAA occlusion devices described herein. The cover 3153 may have the same or similar features and/or functionalities as other covers described herein, such as the cover 3100, 3151, and/or cover 3300, and vice versa, except as otherwise noted. For example, the cover 3151 may include the proximal surface 3152, outer edge 3154 forming outer vertices 3156, and windows 3177.

[0368] The device 3000 with cover 3151 may have proximal anchors 3090 extending through the windows 3177. The proximal anchor 3090 may extend through the opening of the respective window 3177. The proximal anchor 3090 may extend through a distal portion of the window 3177, for example to contribute to securing the cover 3153 on the device 3000. The proximal anchors 3090 may extend through the window 3177 at a distal edge or distal vertex of the window 3177. In some embodiments, the proximal anchor 3090 may extend through the cover 3151 material, for example through material adjacent (such as distal) to the window 3177. In some embodiments, the proximal anchor 3090 may extend through various other locations within, adjacent or near the window 3177. Some of the proximal anchors 3090 may extend through first locations and other of the proximal anchors 3090 may extend through second locations of the cover 3153 different from the first locations. For instance, one or more anchors 3090 may extend through a first region of the window 3177, one or more other anchors 3090 may extend through a second region of the window 3177, still one or more other anchors 3090 may extend through other regions, such as through the cover 3153 material, etc.

[0369] The cover 3153 may include proximal vertices 3155. The proximal vertices 3155 may be formed by the outer edge 3154. The proximal vertices 3155 may be indentations along the outer edge 3154 of the cover 3153, for example angled as shown or other shapes, configurations, etc. The proximal vertices 3155 may define a region 3016A of the outer surface 3016 of the sidewall 3014. The region 3016A may be partially enveloped by the outer edge 3154 of the cover 3153. The region 3016A may receive one or more of the distal anchors 3094 therethrough. The distal anchor 3094 may extend through a distal portion of the region 3016A, or in other locations within, adjacent, or near the region 3016A. In some embodiments, the distal anchor 3094 may not extend through or near the region 3016. There may be multiple such regions 3016A of the foam body 3002 defined circumferentially about the device 3000 by the cover 3153.

[0370] The cover 3153 may include the series of openings 3320, for example as described with respect to FIG. 87A. The series of openings 3320 may include the proximal openings 3172, the shoulder openings 3323, and/or the side openings 3174. The cover 3153 may include different patterns, sizes, distributions, etc. of the openings 3320, for example as shown and described with respect to FIGS. 88B-88C.

[0371] 3. Compliant Frame

[0372] The expandable and compliant support or frame 3040 is shown, for example, in FIGS. 85B, 85D, 86C and 87C-E. FIGS. 89A and 89B are side and proximal perspective views, respectively, of the frame 3040 shown in a deployed configuration and in isolation from the rest of the

device 3000. The frame 3040 provides a compliant structure with anchors to facilitate delivery, anchoring, retrieval and to enable the foam body 3002 to compress against the LAA tissue to facilitate sealing, among other things, as further described. The frame 3040 is located inside the cavity 3028 formed by the foam body 3002. In some embodiments, the frame 3040 may be located partially or entirely inside one or more portions of the body 3002, e.g. within the proximal face 3008 and/or the sidewall 3014, as further described. For example, the frame 3040 may be partially located within the sidewall 3014 as shown in FIG. 87C.

[0373] The frame 3040 has a proximal end 3042 and an opposite distal end 3004. The frame 3040 may be tubular, e.g. cylindrical, in a free, unconstrained state. Thus the width of the proximal end 3042 may be the same or similar to the width of the distal end 3004 in the free, unconstrained state. In some embodiments, the frame 3040 or portions thereof may be conical or frustoconical, e.g. where in the free, unconstrained state the width of the proximal end 3042 is greater than the width of the distal end 3004 or vice versa.

[0374] At the proximal end 3042, the frame 3040 has a proximal hub 3050, shown as a cylindrical nipple. The hub 3050 is a rounded, structural end piece. The hub 3050 may be tubular, e.g. circular and having the cylindrical shape as shown, or may be rounded, non-circular, segmented, other shapes, or combinations thereof. The hub 3050 extends axially and may have a central lumen. The hub 3050 may be wider than it is long, or vice versa. The hub 3050 is hollow and has a sidewall defining a space therethrough, such as a longitudinal opening. In some embodiments, the hub 3050 may be partially hollow, solid, or other configurations. The hub 3050 facilitates delivery and retrieval of the device 3000, as further described. The hub 3050 may provide a central structural attachment, as further described herein. The hub 3050 may be located within the cavity 3028 at a proximal end thereof. In some embodiments, the hub 3050 may be located partially or entirely within the foam body 3002, e.g. within the proximal face 3008.

[0375] A pin 3051 is located within the hub 3050 (shown in FIGS. 89A and 89B). The pin 3051 is an elongated, rounded structural element extending laterally across the central lumen. "Lateral" here refers to a direction perpendicular or generally perpendicular to the longitudinal axis. The pin 3051 has a cylindrical shape. The pin 3051 provides a rounded outer surface configured to provide a smooth engagement surface with a tether, as further described. The pin 3051 provides a high strength connection with the frame 3040 to allow for pulling on the device 3000 with sufficient force to re-sheath the device 3000. The pin 3051 may be formed from Nitinol. The pin 3051 is secured across the width, e.g. diameter, of the proximal hub 3050. The pin 3050 may be secured at its two opposite ends with the sidewall of the hub. The pin 3051 is configured to be engaged by a tether 3240, which is wrapped around the pin 3051 in sliding engagement for temporary attachment to a delivery catheter, as further described. In some embodiments, the pin 3051 is assembled with a cap 3180, as further described herein, for example with respect to FIGS. 90A-90C.

[0376] The frame 3040 at the proximal end 3042 includes a proximal face 3060. The proximal face 3060 may be located within the cavity 3028 at a proximal end thereof. In some embodiments, the proximal face 3060 may be located partially or entirely within the foam body 3002, e.g. within the proximal face 3008 and/or sidewall 3014. The proximal

face **3060** includes a series of recapture or reentry struts **3061**. The struts **3061** are located at a proximal end of the cavity **3028**. In some embodiments, the struts **3061** or portions thereof may be located partially or entirely within the foam body **3002**, e.g. within the proximal face **3008** and/or sidewall **3014**.

[0377] The struts **3061** are elongated structural members. The struts **3061** may have rectangular, circular or other shaped cross-sections. In some embodiments, the struts **3061** have a cross-section, e.g. rectangular, with a width that is greater than a thickness such that the struts **3061** are stiffer in one direction compared to another direction. This width may be in the lateral direction or a direction generally perpendicular to the longitudinal axis of the device **3000** when the device **3000** is in the expanded configuration, with the thickness perpendicular to the width. The struts **3061** may be less stiff in the direction of flexing or bending, for example to facilitate contraction and expansion of the device **3000** in the delivery and expanded configurations. The struts **3061** may be elongated pins. The struts **3061** may extend from the hub **3050**, for example, and incline radially outwardly in the distal direction from the hub **3050**. The struts **3061** may be attached inside, outside, and/or at the end of the sidewall of the hub **3050**. The struts **3061** may be separate parts that are then attached to the hub **3050**, for example welding, bonding, fastening, other suitable means, or combinations thereof. In some embodiments, some or all of the struts **3061** and the hub **3050** may be a single, continuous structure formed from the same raw material such as a laser cut hypotube. Some or all of the struts **3061** may be attached, e.g. with sutures as described herein, to the body **3002** and/or the cover **3100** at one or more attachment locations.

[0378] Each recapture strut **3061** may include an inner curved portion **3062** connected to a distal end of the hub **3050**, a middle straight portion **3064**, and/or an outer curved portion **3066** (for clarity, only some of the portions **3062**, **3064**, **3066** are labelled in the figures). In the deployed configuration, the inner curved portion **3062** extends from the hub **3050** primarily in a distal direction and then curves to face more outwardly radially. The middle straight portion **3064** extends from the inner curved portion **3062** primarily radially but also slightly distally. The outer curved portion **3066** extends from the middle straight portion **3064** primarily in the radial direction and then curves toward the distal direction. The portions may have different shapes in the delivery configuration inside a delivery catheter. In the delivery configuration, the portions may extend primarily distally. The portions may then take the deployed configuration as described upon deployment from the delivery catheter. In some embodiments, the struts **3061** may include fewer or more than the portions **3062**, **3064**, **3066**.

[0379] The device **3000** may include ten of the proximal recapture struts **3061**. Such configuration may accompany a device **3000** having a foam body **3002** with an outer diameter of 27 mm in the free, unconstrained state. Such configuration may accompany a device **3000** having a foam body **3002** with an outer diameter of 35 mm in the free, unconstrained state. In some embodiments, the device **3000** may have from about two to about thirty, from about four to about twenty, from about six to about eighteen, from about eight to about sixteen, from about ten to about fourteen, or other numbers of struts **3061**. In some embodiments, the device **3000** has twelve of the proximal recapture struts **3061**, for example for the 35 mm diameter device.

[0380] In the deployed configuration, each strut **3061** may extend radially outward and distally at an angle to the axis. This angle, measured relative to a portion of the axis that extends distally from the device **3000**, may be from about 60° to about 89.9°, from about 65° to about 88.5°, from about 70° to about 85°, from about 72.5° to about 82.5°, from about 75° to about 80°, or other angular amounts. This angle may be much smaller when the device **3000** is in the delivery catheter. The struts **3061** may bend or flex when transitioning between, or when positioned in, the delivery and expanded configurations. The struts **3061** may bend or flex at the inner curved portion **3062**, the middle straight portion **3064**, and/or the outer curved portion **3066**.

[0381] The proximal end **3042** of the frame **3040**, such as the proximal face **3060**, may therefore have a conical shape in the expanded configuration. The conical proximal face **3060** may facilitate with recapture of the device **3000** back into the delivery catheter. For example, the orientation of the struts **3061** inclining distally and radially outward from the hub **3050** in the expanded configuration provides an advantageous conical shape to the proximal face **3008** such that distal advance of the delivery sheath over the device **3000** will bias the struts **3061** inward and cause the device **3000** to stow back toward the delivery configuration and size for retrieval within the catheter.

[0382] The proximal face **3060** foreshortens considerably upon expansion of the device **3000** relative to the delivery configuration. “Foreshortening” here refers to the difference in axial length of the proximal face **3060** between the reduced delivery configuration and the expanded configuration (expanded either freely or as implanted). This length may be measured axially from the distal or proximal end of the hub **3050** to the distal ends of the outer curved portions **3066** of the recapture struts **3061**. The proximal face **3060** may foreshorten by 50%, 60%, 70%, 80%, 90% or more. The proximal face **3060** has significantly more foreshortening upon expansion than the tubular body **3080**, the latter of which may be referred to as the “working length” or “landing zone.” The landing zone is further described with respect to the tubular body **3080** herein.

[0383] As shown, the struts **3061** are angularly spaced about the axis in even angular increments. That is, looking at the frame **3040** from the distal or proximal end, the angles between the struts may be equal. In some embodiment, the struts **3061** may not be evenly angularly spaced about the axis as described. The struts **3061** may or may not be symmetrically disposed about the axis or about a plane that includes the axis.

[0384] In some embodiments, portions of the frame **3040** may be at various distances from the proximal end of the foam body **3002**, such as the proximal end wall having the proximal face **3008**. As shown in FIG. 87D, there may be a gap of size *Z* in the axial direction between the proximal face **3060** of the frame **3040** and the inner surface **3012** of the proximal face **3008**. The length of *Z* may be one, two, three, four, five, six, seven, eight, nine, ten, or more millimeters. The length of *Z* may vary depending on the radial distance at which it is measured. For instance, the length of *Z* may decrease, increase, or combinations thereof, as measured along the length of the strut **3061**. In some embodiments, the length of *Z* may be zero at more or points along the length of the strut **3061**. As shown in FIG. 87E, the proximal face **3060** or portions thereof may contact the proximal inner surface **3012** of the foam body **3002**. The inner curved

portion **3062**, the straight portion **3064**, and/or the outer curved portion **3066** may contact the proximal end wall such as the inner surface **3012** and/or other portions of the foam body **3002**. The hub **3050** may compress the proximal face **3008** or proximal end wall of the foam body **3002** slightly in a proximal direction as shown. The proximal face **3008** may therefore have a smaller thickness in this compressed region as compared to other portions of the proximal face **3008**, for example portions adjacent to this compressed portion. The hub **3050** may be located based on the axial location of connection of the anchors **3090**, **3094** to the sidewall **3014**, as described herein. In some embodiments, the hub **300** may not compress the foam body **3002** as shown. In some embodiments, the proximal face **3060** may extend radially outwardly as shown. For instance, the struts **3061**, or portions thereof for instance the straight portions **3064**, may extend radially outwardly perpendicularly or generally perpendicularly to the longitudinal axis of the device **3000**. The proximal face **3060** may extend radially outwardly and incline in a distal direction, as described herein, or it may incline in a proximal direction. The device **3000** may have any of these features in the constrained, unconstrained and/or implanted configurations.

[0385] The frame **3040** includes a tubular body **3080**. The body **3080** provides a mechanical base structure for the device **3000**, as further described. The tubular body **3080** is attached to a distal end of the proximal face **3060** of the frame **3040**. The tubular body **3080** extends to the distal end **3044** of the frame **3040**. The tubular body **3080** is attached at a proximal end to the outer curved portions **3066** of the recapture struts **3061**, as further described. The tubular body **3080** may be attached to other portions of the recapture struts **3061**. The tubular body **3080** of the frame **3040** may be attached to the body **3002** and/or the cover **3100**, e.g. with sutures as described herein, at one or more attachment locations, as further described. The tubular body **3080** may be located within the cavity **3028**. In some embodiments, the tubular body **3080** may be located partially or entirely within the foam body **3002**, e.g. within the sidewall **3014**.

[0386] The tubular body **3080** includes a series of proximal struts **3082** and distal struts **3086** (for clarity, only some of the struts **3082**, **3086** are labelled in the figures). The proximal struts **3082** and/or distal struts **3086** may have rectangular, circular or other shaped cross-sections. In some embodiments, the proximal struts **3082** and/or distal struts **3086** have a cross-section, e.g. rectangular, with a width that is greater than a thickness, or vice versa, such that the struts **3061** are stiffer in one direction compared to another direction. The struts **3061** may be less stiff in the direction of flexing or bending, for example to facilitate contraction and expansion of the device **3000** in the delivery and expanded configurations. Proximal ends of pairs of adjacent proximal struts **3082** join at proximal apexes **3084**. Each proximal strut **3082** is connected at a respective proximal apex **3084** to a respective outer curved portion **3066** of one of the recapture struts **3061**. Each distal end of the proximal struts **3082** connects to a distal end of an adjacent proximal strut **3082** and to proximal ends of two distal struts **3086** at an intermediate vertex **3087**. Pairs of adjacent distal struts **3086** extend distally to join at a respective distal apex **3088**. A repeating pattern **3089**, shown as a diamond shape, may be formed by adjacent pairs of proximal struts **3082** and adjacent pairs of distal struts **3086**. Some or all of the proximal struts **3082** and/or distal struts **3086** may be

attached, e.g. with sutures as described herein, to the body **3002** and/or the cover **3100** at one or more attachment locations. Some or all of the proximal struts **3082** and/or distal struts **3086** may be located within the cavity **3028**. In some embodiments, some or all of the proximal struts **3082** and/or distal struts **3086** may be located partially or entirely within the foam body **3002**, e.g. within the sidewall **3014**.

[0387] There are the same number of proximal apexes **3084** as distal apexes **3088**. As shown, there are eleven proximal apexes **3084** and eleven distal apexes **3088**. The number of proximal and distal apexes **3084**, **3088** may each be at least seven, at least eight, at least nine, at least ten, at least eleven, at least twelve, at least thirteen, at least fourteen, at least fifteen, at least sixteen, or fewer or more apexes. In some embodiments, there may not be the same number of proximal apexes **3084** as distal apexes **3088**. In some embodiments, there may be more than one row of the pattern, e.g. diamond pattern, formed by the proximal struts **3082** and distal struts **3086**. There may be two, three, four or more rows of the pattern. Some or all of the proximal apexes **3084** and/or distal apexes **3088** may be attached, e.g. with sutures as described herein, to the body **3002** and/or the cover **3100** at one or more attachment locations.

[0388] The body **3080** may be tubular, e.g. cylindrical or generally cylindrical, in the expanded configuration. The tubular body **3080** may be cylindrical, rounded, segmented, polygonal, tube-like, other shapes, or combinations thereof, all of which are subsumed non-exhaustively under the category "tubular." The tubular shape is formed by the proximal struts **3082** and distal struts **3086** in the expanded configuration. The tubular shape may also be formed by the outer curve portions **3066** of the recapture struts **3061** in the expanded configuration. The tubular shape may also be formed by the foam body **3002** exerting an outward radial force on the frame **3040**. The frame **3040** may therefore have a proximal conical section and a cylindrical working length. In some embodiments, the body **3080** may be conical or frustoconical, for example where the distal end is wider than the proximal end or vice versa.

[0389] The tubular body **3080** may be referred to as a "landing zone," as described. This landing zone may refer to the axial length of the body **3080**, from a distal-most end to a proximal-most end at the transition to recapture struts **3061**, in the expanded configuration. The landing zone may have an axial length as measured from the proximal apex **3084** to the distal apex **3088**. The length of the landing zone may be 10 mm or about 10 mm. The landing zone may have a length from about 5 mm to about 15 mm, from about 6 mm to about 14 mm, from about 7 mm to about 13 mm, from about 8 mm to about 12 mm, from about 9 mm to about 11 mm, or other lengths. The tubular body **3080** may foreshorten slightly upon expansion of the device **3000** relative to the delivery configuration. The tubular body **3080** has significantly less foreshortening upon expansion than the length of the proximal face **3060**. The tubular body **3080** may foreshorten by no more than about 5%, 10%, 15%, 20% or 30%.

[0390] The frame **3040** self-expands upon delivery from the sheath. The proximal face **3060** and the tubular body **3080** will self-expand. Upon expansion, the radially outward portions of the tubular body **3080** will contact and compress the foam body **3002** against tissue of the LAA wall. The tubular body **3080**, for example the proximal struts **3082** and distal struts **3086**, will contact the inner surface **3018** of the

sidewall **3014** and press against the sidewall **3014** so that the outer surface **3016** of the sidewall **3014** contacts and compresses against the LAA wall.

[0391] When compressed against the LAA wall, the foam body **3002** provides a larger “footprint” than the skeletal frame **3040** components and forms a complete seal. Thus, the sidewall **3014** acts as a force dissipation layer, spreading radial force out from the struts **3082**, **3086** of the frame **3040** over a larger area than just the area of the individual struts **3082**, **3086** (e.g. a larger area than just the area of the radially outer surfaces of the struts **3082**, **3086**). The use of the foam material in the body **3002** and the thickness of that foam, such as 2.5 mm, provide advantages in this regard over devices with thinner and less resilient materials than foam. For example, thin fabrics or similar materials that are pressed against the LAA wall with a skeletal frame will not spread the radial force out, and may even sag or otherwise bend, creating gaps and an unsealed portion of the LAA wall. The foam body **3002** as described herein will take the shape of the LAA wall to create a complete circumferential seal and will also spread out the radial forces from the frame **3040** to create a stronger seal and retention with the foam body **3002**.

[0392] Further, the device **3000** described herein with the compressible body **3002** allows for a structural frame **3040** that is compliant due to the smaller required radial force from the frame **3040**. For example, existing devices with a non-compressible fabric material will have a less effective seal, and so the structural elements of those devices must provide larger radial forces to compensate and ensure an effective seal, resulting in a less compliant device. In contrast, the current device **3000** provides advantages in this regard by having the compressible foam body **3002**, allowing for among other things smaller radial forces from, and thus better compliance of, the frame **3040**, while still providing an effective seal. This structural configuration has a cascading effect in terms of performance advantages. For instance, the compliance of the device **3000** allows for delivery off-axis while still providing an effective seal, among other advantages as further described herein.

[0393] The frame **3040** includes a series of proximal anchors **3090**. Each proximal anchor **3090** extends from a respective intermediate vertex **3087**. The proximal anchors **3090** may extend from other portions of the tubular body **3080**. As shown, in the deployed configuration, the proximal anchors **3090** extend from the tubular body **3080** radially and proximally. The proximal anchors **3090** may extend into an adjacent region of the sidewall **3014**. The proximal anchors **3090** may extend through the outer surface **3016** of the sidewall **3014** to penetrate tissue adjacent the device **3000**.

[0394] The frame **3040** includes a series of distal anchors **3094**. Each distal anchor **3094** extends from a respective distal apex **3088**. The distal anchors **3094** may extend from other portions of the tubular body **3080**. As shown, in the deployed configuration, the distal anchors **3094** extend from the tubular body **3080** radially and proximally. The distal anchors **3094** may extend into an adjacent region of the sidewall **3014**. The distal anchors **3094** may extend through the outer surface **3016** of the sidewall **3014** to penetrate tissue adjacent the device **3000**. The anchors **3090**, **3094** may incline radially outward in a proximal direction to engage the tissue to resist proximal movement of the device **3000**.

[0395] The anchors **3090**, **3094** are elongated structural members. The tips of the anchors **3090**, **3094** may be sharpened to facilitate tissue engagement and penetration. The anchors **3090**, **3094** may be straight, extending generally along a local axis thereof. The anchors **3090**, **3094** may have a curved or other non-straight proximal portion where they attach to the tubular body **3080**. In some embodiments, the anchors **3090**, **3094** or portions thereof may be non-straight, curved, rounded, segmented, other trajectories, or combinations thereof. In some embodiments, the tissue engaging tips may be curved. In some embodiments, the anchors **3090**, **3094** may have engagement features extending radially away from the anchor **3090**, **3094**, such as barbs, hooks, or other features.

[0396] The cross-section of the anchors **3090**, **3094** may be rectangular. In some embodiments, the cross-section may be circular, rounded, non-rounded, square, rectangular, polygonal, other shapes, or combinations thereof. The cross-sections may or may not be uniform along the length of the anchor **3090**, **3094**. The anchors **3090**, **3094** may be about 0.006" thick and about 0.008" wide. The anchors **3090**, **3094** may range from about 0.003" to about 0.009" in thickness and from about 0.003" to about 0.015" in width. The cross-section of the anchors **3090**, **3094** may reduce in size, for example taper, toward the distal tip.

[0397] In some embodiments, the anchors **3090**, **3094** in the deployed configuration are inclined at an incline angle of about 30° relative to a portion of the central axis that extends proximally from the device **3000**. This incline angle may be from about 10 degrees to about 50°, from about 15° to about 45°, from about 20° to about 40°, from about 25° to about 35°, or about 30°. This incline angle of the anchors **3090**, **3094** in the delivery configuration may be smaller than in the deployed configuration. The anchors **3090**, **3094** may have the angle B, as shown in and described with respect to FIGS. 94A-94C.

[0398] The anchors **3090**, **3094** may have various lengths. The length of the anchor **3090**, **3094** is measured from a proximal end that connects to the tubular body **3080** to a distal tissue engaging tip of the anchor. In some embodiments, the length of the anchors **3090**, **3094** may be from about 0.5 mm to about 10 mm, from about 1 mm to about 9 mm, from about 2 mm to about 8 mm, from about 3 mm to about 7 mm, from about 4 mm to about 6 mm, about 5 mm, or other greater or lesser lengths. In some embodiments, the anchors **3090**, **3094** are 5 mm long. In some embodiments, the anchors **3090**, **3094** are about 5 mm long. In some embodiments, the anchors **3090**, **3094** have a length of at least 2.5 mm, at least 3 mm, at least 3.5 mm, at least 4 mm, at least 4.5 mm, at least 5 mm or more. The anchors **3090**, **3094** may each be the same or similar length. In some embodiments, the anchors **3090**, **3094** may not be the same length. In some embodiments, some or all of the proximal anchors **3090** may have lengths that are less than or greater than some or all of the lengths of the distal anchors **3094**. The anchors **3090**, **3094** may have the length L, as shown in and described with respect to FIGS. 94A-94C. Further, the outer tips of the anchors **3090**, **3094** may extend to an outer radial location that is less than, the same as, or more than a radially outermost surface of the foam body **3002**, as shown in and described with respect to FIGS. 94A-94C.

[0399] In the expanded configuration, the anchors **3090**, **3094** extend for a length outside of the uncompressed sidewall **3014**. This length of the anchor **3090**, **3094** is

measured along a local longitudinal axis of the anchor from the outer surface 3016 of the body 3002 to the distal tip of the anchor. The anchors 3090, 3094 may extend through the sidewall 3014 and/or the cover 3100, and then be trimmed so that the anchors 3090, 3094 extend beyond the sidewall 3014 and/or cover 3100 by the desired length. In a free, unconstrained state, the anchors 3090, 3094 extend about 0.5 mm beyond the outer surface 3016 of the sidewall 3014. In some embodiments, in the free, unconstrained state, the anchors 3090, 3094 extend beyond the outer surface 3016 of the sidewall 3014 for a length of from about 0.1 mm to about 1.5 mm, from about 0.2 mm to about 1.25 mm, from about 0.3 mm to about 1.0 mm, from about 0.4 mm to about 0.8 mm, from about 5 mm to about 0.6 mm, or other greater or lesser lengths. In a compressed state, such as in the delivery configuration or after implantation, the anchors 3090, 3094 extend about 1.0 mm beyond the outer surface 3016 of the sidewall 3014. In some embodiments, in the compressed state, the anchors 3090, 3094 extend beyond the outer surface 3016 of the sidewall 3014 for a length of from about 0.25 mm to about 2.5 mm, from about 0.5 mm to about 2 mm, from about 0.75 mm to about 1.5 mm, from about 0.875 mm to 1.125 mm, or other greater or lesser lengths.

[0400] The geometry of the anchors 3090, 3094 provides several advantages. For example, the relatively long length allows for flexibility of the anchors 3090, 3094. This provides for potentially less trauma to the LAA tissue should the device 3000 need to be unanchored and/or retrieved. The anchors 3090, 3094 are less susceptible to loss of strength with off-axis orientation within the LAA. Further, the anchors 3090, 3094 provide high resistance to pull out. For instance, the device 3000 may provide at least about 0.5 lb-force of dislodgment resistance from the LAA. Such pullout tests may be simulated with in vitro or benchtop models, as further described below.

[0401] The anchors 3090, 3094 in the illustrated embodiment are located in two circumferential rows. One row is located proximal to the other distal row. Each row has ten anchors each. This configuration may be incorporated, for example, in the device 3000 having a foam body 3002 with a free, unconstrained outer diameter of 27 mm. Each row may have fourteen anchors each. This configuration may be incorporated, for example, in the device 3000 having a foam body 3002 with a free, unconstrained outer diameter of 35 mm. In some embodiments, a single row of anchors 3090, 3094 may have twelve anchors. In some embodiments, a single row of anchors 3090, 3094 may have from two to twenty-four, from four to twenty-two, from five to twenty, from six to eighteen, from seven to sixteen, from eight to fifteen, from nine to fourteen, from ten to thirteen anchors, or greater or fewer amounts of anchors 3090 or 3094. In some embodiments, there may only be one row or greater than two rows of anchors. The anchors 3090, 3094 may be spaced circumferentially in a single row. In some embodiments, the device has twenty-four total anchors 3090, 3094, with each row having twelve anchors, and twelve of the proximal recapture struts 3061, for example for the 35 mm diameter device 3000. In some embodiments, the device has twenty total anchors 3090, 3094, with each row having ten anchors, and ten of the proximal recapture struts 3061, for example for the 27 mm diameter device 3000.

[0402] In embodiments with multiple rows of anchors 3090, 3094, the rows may be circumferentially offset, as shown. That is, as viewed from the proximal or distal end of

the device 3000, the anchors 3090, 3094 are angularly spaced apart from each other about the axis. The anchors 3090, 3094 may not be circumferentially offset, e.g. they may be evenly angularly spaced when viewed as described. The anchors 3090, 3094 are located axially at or near a middle portion of the sidewall 3014. The anchors 3090, 3094 may be located such that the tips of the anchors 3090, 3094 extend to adjacent tissue at a middle portion of the sidewall 3014. The offset and middle locations of the anchors 3090, 3094 may ensure engagement with the LAA tissue distal to the ostium. Having the anchors 3090, 3094 located at the largest width, increases the stability of the device 3000. With a cylindrical or generally cylindrical shaped device 3000, the anchors 3090, 3094 effectively sit on the largest diameter of the device 3000. The cylindrical shape provides advantages over typical LAA occluders which taper distally thus decreasing implant stability and locating the anchors on a smaller diameter than the ostial diameter of the occluding surface. In addition to adding stability, the cylindrical shape of the device 3000 along the axial length helps with dislodgement resistance by allowing the anchors 3090, 3094 to be placed on the largest diameter section of the device 3000. In some embodiments, the anchors 3090, 3094 may be located proximal, distal, or centrally along the length of the frame body 3080. In some embodiments, the anchors 3090, 3094 may not be offset and/or may not be angularly evenly spaced.

[0403] The anchors 3090, 3094 may provide advantageous flexibility, as demonstrated by pullout tests and in comparison to existing devices. For example, the device 3000 was tested to determine the force required to dislodge the device 3000 from a simulated tissue model by pulling the device 3000 proximally outward from the model. A low durometer silicone tube with a circular inner diameter (ID) was used as the model. For the device 3000 having a foam body 3002 with a 27 mm outer diameter in a free unconstrained state, tubes with ID's of 16.5 mm, 21 mm and 25 mm were tested. The pullout forces for existing devices drop off significantly going up to a 21 mm model, whereas the forces for the device 3000 drop only slightly.

[0404] In the largest diameter (25 mm) model, where there is not a lot of interference in the fit, the forces for the existing devices approach zero as the device does not engage the model wall because the anchors are sitting at a smaller diameter on a trailing edge of the device. The device 3000 consistently resists dislodgment with about 0.7 lbs of force. Since there is very little friction resisting pullout, that force is almost entirely resisted by the anchors 3090, 3094. When examining failure modes, all devices eventually begin to slide out of the model. Upon failure, the anchors 3090, 3094 fold backward or sideways before slipping starts. Assuming 0.7 lbs force is required to cause all twenty anchors 3090, 3094 to fold backward, then the force per anchors is estimated to be about 0.035 lbs.

[0405] The frame 3040 may be laser cut. The tubular body 3080 may be laser cut from a single tube. The body 3080 may be cut from a tube having a thickness from about 0.002" to about 0.014", or about 0.008". The tube may have an outer diameter (OD) from about 0.05" to about 0.30". The tube may have an outer diameter (OD) of 0.124" for the 27 mm device 3000 (i.e. the embodiment of the device 3000 having a foam body 3002 with an OD of 27 mm in the unconstrained, free state). The tube may have an OD of 0.163" for

the 35 mm device **3000** (i.e. the embodiment of the device **3000** having a foam body **3002** with an OD of 35 mm in the unconstrained, free state).

[**0406**] In some embodiments, the body **3080** is laser cut from a superelastic nitinol tube, however, numerous other biocompatible metallic materials can be utilized such as shape memory Nitinol, stainless steel, MP35N, or Elgiloy. The frame **3040** is self-expandable. In some embodiments, a balloon-expandable frame **3040** could be utilized. Additionally, the body **3080** could be fabricated from drawn wire as opposed to being laser cut from a tube.

[**0407**] As shown, an embodiment of the device **3000** includes the frame **3040** having ten proximal recapture struts **3061** and twenty total anchors **3090**, **3094**, with the foam body **3002** having an outer diameter of 27 mm. In some embodiments, the device **3000** may include the frame **3040** having fourteen proximal recapture struts **3061** and twenty-eight total anchors **3090**, **3094**, with the foam body **3002** having an outer diameter of 35 mm.

[**0408**] In one embodiment, the frame **3040** includes a proximal hub **3050**, tether pin **3051**, front face with ten or fourteen recapture struts **3061**, a diamond pattern cylindrical body **3080**, and twenty or twenty-eight anchors **3090**, **3094**. The frame proximal face **3060** supports recapture, the frame body **3080** supports the foam cylinder body **3002**, and the anchors **3090**, **3094** located on the cylinder provide resistance to embolization.

[**0409**] The design of the device **3000** provides numerous advantages, some of which have been described. As further example, the frame **3040** provides many advantages, including but not limited to: 1) implant radial stiffness/compliance—the frame **3040** provides enhanced radial stiffness while still being sufficiently compliant to allow for off-axis implantation, recapture, etc.; 2) dislodgement resistance—the frame **3040** provides for high pullout strength, as described; 3) transcatheter delivery—the frame **3040** can be compressed into a delivery catheter and then fully expand when delivered; 4) recapture—the frame **3040** allows for recapture/retrieval into the delivery catheter after deployment or even after implantation in the LAA; and 5) mechanical integrity—the frame **3040** has acute and long term structural integrity, for example the ability to withstand loading into the delivery catheter, deployment from the catheter, and cyclic loading/fatigue. The frame **3040** also provides a conformable structure to enable the foam body **3002** to compress against the LAA tissue to facilitate sealing and anchoring with minimal compression (oversizing). The resulting compliance of the frame **3040** provides better anchoring than existing solutions, as described.

[**0410**] As further example, the device **3000** seals against irregularly shaped LAA ostia and necks. For instance, a combination of a Nitinol frame **3040** with a foam body **3002** having a coating of PTFE and cover **3100** of ePTFE contribute to ability of the device **3000** to conform to the anatomy and seal against irregular projections and shapes, while providing a smooth thromboresistant LA surface.

[**0411**] As further example, the device **3000** provides for controlled & safe delivery. The design of the combined frame **3040** and foam body **3002** facilitates delivery in a controlled fashion by slowing the speed of expansion. The bumper **3026** acts as an atraumatic leading edge portion when delivering the implant into the LAA mitigating the risk of injury. The user has the ability to recapture and redeploy the device **3000**, if necessary. A flexible tether **3240** attach-

ment, as further described, from the delivery catheter to the device **3000** permits the device **3000** to sit tension free immediately following implantation so the user can ensure final appropriate positioning prior to release of the device **3000**.

[**0412**] As further example, the device **3000** provides for simplified placement. The foam-covered cylindrical design makes alignment of the device **3000** with the central axis of the LAA during delivery non-critical (by allowing deployment up to, for example, 45 degrees off-axis), which is designed to simplify the implantation procedure, as further described.

[**0413**] As further example, the device **3000** provides for simple sizing. The foam and frame design contributes to the ability to need only two diameters (e.g., 27 mm and 35 mm) to seal the range of expected LAA configurations and diameters (e.g. targeting LAA diameters of 16 to 33 mm). The conformability of the foam and frame allow the 20 mm long implant to fit into LAA's as short as 10 mm deep. The short landing zone requirement (LAA depth) of the device **3000**, combined with the need for only two implant diameters, enables treatment of a wide range of LAA anatomies with minimal need for burdensome echo and CT sizing. The conforming nature of the implant is key to facilitating a simple to use product platform that is adaptable to a variety of anatomic structures.

[**0414**] As further example, the device **3000** provides thromboresistant materials and design. The removable tether leaves a smooth, metal-free surface in the LA. Thromboresistant materials (PTFE-coated foam and an ePTFE cover) create a smooth LA face (no metal attachment connection) to reduce anticoagulation needs, enhance thromboresistance, and encourage endothelialization.

[**0415**] As further example, the device **3000** provides thin, low profile anchors **3090**, **3094** around the midpoint of the device **3000** to provide secure yet atraumatic anchoring.

[**0416**] 4. Distal Bumper

[**0417**] The foam body **3002** has a distal bumper **3026**. The bumper **3026** may be a foam distal region of the body **3002**, such as a distal portion of the sidewall **3014**. The bumper **3026** may be a portion of the foam body **3002** that extends beyond the distal end **3044** of the frame **3040**. The bumper **3026** may extend beyond the distal end **3044** of the frame **3040** in the delivery configuration and in the deployed configuration. The body **3002** may be attached to the frame **3040** in various locations such that the body **3002** may stretch in some embodiments, for example in the delivery configuration, to ensure the bumper **3026** extends beyond the frame **3040** upon initially retracting the sheath during delivery.

[**0418**] The device **3000** can conform both in length and diameter due to conformability of both the foam body **3002** and the frame **3040**. This allows for the device **3000** to accommodate most patient LAA anatomies with only a couple or few different sizes of the device **3000**, such as 27 mm and 35 mm outer diameter body **3002** as described herein, and one length, such as 20 mm. The frame **3040** may thus be shorter than the foam body **3002**, resulting in some embodiments in about 5 mm of foam bumper **3026** distal to the distal-most end of the frame **3040**. The distal bumper **3026** acts as an atraumatic tip during delivery of the device **3000** and can be compressed following implantation to allow the device **3000** to conform to appendages with a depth (landing zone) as short as 10 mm. This ability to

conform both in length and diameter is due to the conformability of both the foam body 3002 and the frame 3040.

[0419] The length of the bumper 3026 may be measured axially from the distal-most end of the frame 3040 to the distal surface 3022 of the body 3002. For example, the bumper 3026 may extend from the distal apexes 3088 to the distal surface 3022. The bumper 3026 may have a length of 5 mm or about 5 mm. The bumper 3026 may have a length of about 1 mm, 2 mm, 3 mm, 4 mm, 5 mm, 6 mm, 7 mm, 8 mm, 9 mm or more. The bumper 3026 may have a length from about 2.5 mm to about 7.5 mm, from about 3 mm to about 7 mm, from about 3.5 mm to about 6.5 mm, from about 4 mm to about 6 mm, from about 4.5 mm to about 5.5 mm.

[0420] In some embodiments, the bumper 3026 may fold in response to axial and/or radial compression of the device 3000. The bumper 3026 may fold inward, for example radially inward. The folds may be in the axial or approximately in the axial direction. The folds may be circumferential or approximately in the circumferential direction. The folds may be combinations of the radial and circumferential directions, or angled with respect thereto. The folding of the bumper 3026 is further discussed herein, for example in the section "Device Compliance."

[0421] 5. Cap & Pin

[0422] FIGS. 90A-90C are proximal perspective views of the frame 3040 having a cap 3180. FIG. 90D is a distal perspective view of the cap 3180. In some embodiments, the pin 3051 is placed across the proximal hub 3050 diameter and serves to engage the delivery catheter tether 3240 (e.g. a suture), which is wrapped around the pin 3051 for temporary attachment to the delivery catheter 3220, as described further herein for example with respect to FIGS. 89A-89B. As shown, the hub 3050 has a pair of opposite side openings 3053 extending through a sidewall of the hub 3050. The cap 3180 has a corresponding pair of opposite side openings 3190 extending through a sidewall 3184 of the cap 3180. When the cap 3180 is assembled with the hub 3050, the pin 3051 may be inserted through the aligned pairs of openings 3053, 3182. The assembly can be further secured by welding the ends of the pin 3051 to the hub 3050.

[0423] As shown in FIG. 90D, the cap 3180 includes a proximal end 3182 and a distal end 3184. The cap 3180 includes a rounded sidewall 3186 extending from the proximal end 3182 to the distal end 3184. The sidewall 3186 defines a longitudinal opening 3188 through the cap 3180. The sidewall 3186 includes a pair of lateral openings 3190 located opposite each other. The cap 3180 includes a flange 3192 at the proximal end 3182 extending radially outward.

[0424] The cap 3180 is formed from titanium and the pin 3051 is formed from Nitinol or superelastic Nitinol. In some embodiments, the cap 3180 and/or pin 3051 may be formed from other materials, for example numerous biocompatible metallic or polymeric materials such as shape memory Nitinol, stainless steel, MP35N, Elgiloy, polycarbonate, polysulfone, polyether ether ketone (PEEK), or polymethyl methacrylate (PMMA) or other materials.

[0425] The cap 3180 and pin 3051 facilitate attachment to the tether 3240. The cap 3180 and pin 3051 also mitigate damage to the foam body 3002 during recapture of the device 3000. The cap 3180 also creates an atraumatic surface for the hub 3050 of the frame 3040. For example, the cap 3180 may prevent the hub 3050 from cutting through the foam body 3002 as the device 3000 is collapsed into an

access sheath. Without the cap 3180, the sharp edges of the hub 3050 may shear through the foam body 3002 during recapture of the device 3000 into the access sheath.

[0426] 6. Loading System

[0427] FIG. 91 is a side view of an embodiment of a loading system 3200 for loading the device 3000 into a delivery catheter 3220. The system 3200 includes a loading tool 3210. The loading tool 3210 has a conical portion 3212, having a distal opening 3213, and a cylindrical portion 3214. The delivery catheter 3220 extends through the cylindrical portion 3214 with a distal end 3222 of the delivery catheter 3220 located within the cylindrical portion 3214. A pusher 3230, such as a pusher catheter, extends through the delivery catheter 3220. A tether 3240 (see FIGS. 92A-92C) is attached to the device 3000 and extends through the loading tool 3210, the delivery catheter 3220 and the pusher 3230. The tether 3240 and pusher 3230 are pulled in the proximal direction while the delivery catheter 3220 and the loading tool 3210 are held stationary. The device 3000 is compressed laterally by the conical portion 3212 as the device 3000 is pulled proximally by the tether 3240 through the loading tool 3210. A distal end 3232 of the pusher 3230 remains adjacent to the proximal end 3004 of the device 3000 as the device 3000 is loaded into the delivery catheter 3220. The removable tether 3240, which may be fabricated from ultra-high molecular weight polyethylene (UHMWPE), is used to attach the implant to the delivery catheter. The material UHMWPE for the tether 3240 may provide high strength and low friction to facilitate delivery of the device 3000.

[0428] In some embodiments, the conical portion 3212 of the loading tool 3210 has a chamfered distal edge of approximately 45°-75° (degrees), preferably 60°. In some embodiments, the conical portion 3212 has a distal inner diameter (ID) greater than the outer diameter (OD) of the device 3000 and an angle A of ideally between 15° and 25°, and in one implementation about 20°, to appropriately collapse the anchors 3090, 3094 which may protrude off the foam body 3002 surface at an angle of 30° or about 30°. The distal opening of the conical portion 3210, for example the diameter or greatest width, may be greater than the proximal opening of the conical portion 3210, for example the diameter or greatest width, that couples with the cylindrical portion 3214. The cylindrical portion 3214 may have an opening, for example diameter or greatest width, that is smaller than the distal opening of the conical portion 3210 and/or the same or similar size as the opening at the proximal end of the conical portion 3210.

[0429] The decreasing width, for example gradual taper, of the loading tool 3210 ensures, for example, that the frame 3040 folds evenly without crossovers or extra strain. The angled conical portion 3212 may ensure that the anchors 3090, 3094 fold or rotate proximally and not distally. The sidewall of the conical portion 3212 may extend at a "total" angle A as measured between two opposite portions of the sidewall, as shown in FIG. 91. The angle A may be from about 12° to about 35°, from about 15° to about 30°, from about 17° to about 25°, from about 18° to about 22°, about 20°, or 20°. The angle A may be at least 100, at least 15°, at least 20°, at least 250, or at least 300. The angle A may be constant along the axial length of the conical portion 3212. The angle of the conical portion 3212 may also be described with respect to a longitudinal geometric center axis, defined by the conical portion 3212 and/or the cylindrical portion 3214. The sidewall may extend in a direction that is at an

angle with respect to such longitudinal axis and which is half of the value of the total angle A. This “half angle” may thus be at least 50, at least 7.5°, at least 100, at least 12.50, or at least 15°, etc. The conical portion 3212 may have a frusto-conical shape. The cross-sectional shape of the conical portion 3212 perpendicular to its longitudinal axis may be circular or approximately circular. In some embodiments, this cross section may be rounded, non-circular, segmented, other shapes, or combinations thereof. The cross-sectional shape of the conical portions 3212 may be constant along its axis, or there may be different shapes along the axis. In some embodiments, the angle A may change along the axial length of the conical portion 3212, for example where the inner surface is curved in the axial direction.

[0430] The loading tool 3210 may be smooth or generally smooth on its inner surface or surfaces. Inner surfaces 3211, 3215 of the conical portion 3212 and/or cylindrical portion 3214 may be smooth or generally smooth. In some embodiments, these inner surfaces 3211, 3215 or portions thereof may not be smooth. In some embodiments, these inner surfaces 3211, 3215 or portions thereof may be smooth, non-smooth, rough, etched, scored, grooved, have varying degrees of roughness or smoothness, other features, or combinations thereof.

[0431] In one example, the tool 3210 may be used by positioning a proximal end of a loading body, such as the tool 3210, adjacent the distal end 3222 of the delivery catheter 3220. The loading body may have a sidewall defining a channel therethrough with the distal opening 3213 at a distal end that is larger than a proximal opening at a proximal end. The left atrial appendage occlusion device 3000 may be advanced proximally through the loading body to thereby radially compress the device 3000. The retracting step may comprise pulling the tether 3240 proximally through the delivery catheter 3220. The device may then be received into the distal end 3222 of the delivery catheter 3220. The device 3000 may be radially compressed within the delivery catheter 3220 having an outer diameter of no more than fifteen French. In some embodiments, the device 3000 may be radially compressed within the delivery catheter 3220 having an outer diameter of no more than ten, eleven, twelve, thirteen, fourteen, fifteen, sixteen, seventeen, eighteen, nineteen, or twenty French. The proximal end of the loading tool 3210 may have an inner diameter configured to provide an interference fit with the distal end 3222 of the delivery catheter 3220. The proximal end of the loading tool, 3210, such as the cylindrical portion 3214, may have an inner diameter slightly larger than the outer diameter of the delivery catheter 3220, for instance slightly larger than 5 mm for a delivery catheter 3220 having an outer diameter of fifteen French. The device 3000 may compress radially to a compressed width in a constrained state that is less than fifty, forty, thirty, twenty, ten, and/or five percent of a radial uncompressed width of the device in an unconstrained state. The radial widths here may be measured perpendicularly to a longitudinal axis of the device 3000, such as defined by the tubular foam body 3002.

[0432] The loading tool 3210 may be formed of a material that is biocompatible, strong, transparent and can be molded smooth to minimize friction, such as polycarbonate. In some embodiments, the loading tool 3210 could be formed from hard plastics like Delrin, UHMWPE, Ultem®, polyetherimide, acrylic, metals like stainless steel, aluminum, other materials, or combinations thereof. In some embodiments,

the loading tool 3210 may have one or more coatings. Such coating may be applied to reduce friction and therefore loading forces. The coating may be silicone, hydrophilics, various oils, other suitable coatings, or combinations thereof. Additional embodiments of a loading tool and system are described herein, for example with respect to FIGS. 103A-103B.

[0433] 7. Delivery System

[0434] FIG. 92A is a side view of a schematic of a delivery system 3201 for delivering the device 3000. FIGS. 92B-92C are additional views of the system 3201. As shown in FIG. 92A, the delivery system 3201 includes the delivery catheter 3220 having a distal end 3222 and a proximal end 3224. The delivery system 3201 includes the pusher 3230, such as a pusher catheter, having a distal end 3232 and a proximal end 3234. The tether 3240 includes a first end 3242 and a second end 3244. A restraint 3246 secures the first and second ends 3242, 3244.

[0435] To deliver the device 3000 to the LAA, an access sheath is placed across the interatrial septum into the LAA through which the delivery catheter 3220, containing the device 3000, is placed. The device 3000 is loaded into the distal end 3222 of the delivery catheter 3220 using the loading tool 3210, either at the point of manufacture or at the treatment site. To load the implant device 3000, the pusher 3230 and tether 3240 are pulled proximally, collapsing the implant device 3000 as it enters the distal tip of the delivery catheter 3220. Once the loaded delivery catheter 3220 is placed through the sheath into the LAA, the pusher 3230, such as a catheter or rod, is held axially steady as the delivery catheter 3220 and access sheath are simultaneously retracted proximally, deploying the implant device 3000.

[0436] The tether 3220 passes from the proximal end of the delivery catheter 3220, through an opening 3221 of the catheter pusher 3230, around the implant tether pin 3051, and back through the delivery catheter 3220. When both ends of the tether 3240 (held together by the restraint 3246 at the proximal end of the catheter) are pulled, the device 3000 is pulled into the delivery catheter 3220. Once the device 3000 is properly placed in the anatomy, one end of the ends 3242, 3244 of the tether 3240 is cut and the entire tether 3240 can be removed from the system by pulling proximally on the uncut end and sliding the cut end distally into the system and around the pin 3051, disengaging from the pin 3051. The distal end 3232 of the pusher 3230 and/or the distal end 3222 of the delivery catheter 3220 may contact, for example push against, the proximal end of the device 3000, such as in the relative locations shown in FIG. 92A. For example, the distal end 3232 of the pusher 3230 may contact and prevent proximal movement of the device 3000 during tether 3240 retrieval, as further described herein. Further details of the release of the tether are provided herein, for example with respect to FIGS. 92B-92B.

[0437] In some embodiments, the delivery system 3201 may include other features. For example, the delivery catheter 3220 may include an injection lumen. The injection lumen may allow for injecting a radiopaque dye distal to the device 3000 following implantation to check for leaks using fluoroscopy.

[0438] 8. Tether Release System

[0439] FIGS. 92B and 92C are proximal and distal perspective views of the delivery system 3201. An approach to releasing the tether, and other features of the system, are

described in this section. For clarity, some features are not shown, such as the cover 3100, foam body 3002, and frame 3040.

[0440] The system 3201 as shown in FIGS. 92B and 92C shows the delivery catheter 3220, the pusher 3230 and the hub 3050 in different axial positions relative to each other. In some embodiments, during release, the distal end 3222 of the delivery catheter 3220 may be co-extensive with, or otherwise near or adjacent, the distal end 3232 of the pusher 3230. Further, the distal ends 3222 and/or 3232 may contact or be adjacent the proximal end 3004 of the device 3000, such as contacting or adjacent the cover 3100 and/or foam body 3002. In some embodiments, the distal end 3232 of the pusher may be located distally of the distal end 3222 of the delivery catheter 3220, as shown, during tether 3240 release.

[0441] The tether 3240 may extend from a proximal end of the pusher 3230, through the opening 3221 of the pusher 3230, wrap around the pin 3051, and extend proximally back through the opening 3221 of the pusher 3230 and out the proximal end of the pusher 3230, as described with respect to FIG. 92A. The tether 3240 may extend through the cover 3100 and foam body 3002. The tether 3240 may extend distally through first aligned paths in the cover 3100 and foam body 3002, around the pin 3051, and extend proximally back through second aligned paths in the cover 3100 and foam body 3002. The tether 3240 may extend through openings within the inner cover 3101, as described for example with respect to FIGS. 85D and 87D. The tether 3240 may only extend around a distal surface or surfaces of the pin 3051, as shown. The tether 3240 may extend distally and wrap around the pin 3051 and extend distally at 180° or approximately 180° relative to the proximally extending portion. In some embodiments, the tether 3240 may be wrapped one or more times, for example two, three or more times, around the pin 3051. In some embodiments, the tether 3240 may be on a spool about the pin 3051. In some embodiments, the tether 3240 may be wrapped, partially, fully or multiple times, about a bushing that is rotatable coupled about the pin 3051.

[0442] The system 3201 may facilitate removal of the tether 3240 while the pusher catheter 3230 is in contact with the device 3000. Such contact may assist, for example, with avoiding or reducing inadvertent dislodgement of the device 3000 from the LAA after implantation and anchoring. For instance, during release of the tether 3240, the pusher 3230 may have the positioning relative to the device 3000 as shown in FIG. 92A. The pusher 3230 may contact the device 3000 on the proximal end 3002 of the device to prevent or reduce any proximal movement of the device 3000 upon tether 3240 removal. For example, there may be friction between the tether 3240 and the pin 3051 as the tether 3240 unwraps about the pin 3051. The distal end of the pusher 3230 may prevent this friction or other forces from dislodging or otherwise moving the device 3000 proximally. In some embodiments, the delivery catheter 3220 may also be contacting, adjacent to, etc. the device 3000. In some embodiments, during tether release and removal, the distal ends of the delivery catheter 3220 and pusher 3230 may be axially co-extensive, adjacent or near each other, etc., as described. Further, the tether 3240 may be proximally pulled completely out of the delivery catheter 3220 and/or pusher 3230 before the delivery catheter 3220 and/or pusher 3230 are removed from the patient. In some embodiments, the tether 3240 may be removed from the patient along with the

delivery catheter 3220 and/or pusher 3230, for example while the tether 3240 is still entirely or partially within the pusher 3230.

[0443] FIGS. 93A and 93B are proximal and distal perspective views respectively of another embodiment of a tether release system 3400. The release system 3400 includes a tube 3420 and a lock 3402. The tube 3420 has a proximal end 3422 and a distal end 3424. An opening 3426 extends through the tube 3420. The system 3400 may be used similarly as described with respect to the system 3201, except as otherwise noted. For example, the pusher 3230 and/or tube 3420 may contact the device 3000 during tether removal, as described.

[0444] The lock 3402 includes a proximal end 3404 and a distal end 3406. An opening 3408 defined by a sidewall 3409 extends through the lock 3402 from the proximal end 3404 to the distal end 3406. The tube 3420 extends through the opening 3408 at the proximal end 3404 of the lock 3402 and to the distal end 3406 of the opening 3408. The sidewall 3409 of the lock 3402 has a first groove 3410 extending longitudinally from the proximal end 3404 to the distal end 3406 and extending radially partially through the thickness of the sidewall 3409. The sidewall 3409 of the lock 3402 has a second groove 3412 extending longitudinally from the proximal end 3404 partially along the sidewall 3409 toward the distal end 3406 and radially partially through the thickness of the sidewall 3409.

[0445] The tether 3240 includes a first end 3243 and the second end 3245. The tether 3240 extends distally from the first end 3243 within the opening 3426 of the tube 3420 and out through the distal end 3424 of the tube 3420 to the cap 3180. The tether 3240 extends distally into the opening 3188 of the cap 3180 and around the pin 3051 and back in the proximal direction. The tether 3240 then extends proximally into the first groove 3410 of the lock 3402, around the proximal end 3404 of the lock 3402, and then distally into and through the second groove 3412. The tether 3240 terminates at the second end 3245 in a knot 3247.

[0446] In use, the knot 3247 may be secured due to the relative location of the lock 3402 and the pusher catheter 3230 inside the delivery catheter 3220. The knot 3247 may be prevented from advancing distally due to the inner diameter of the distal end of the pusher 3230 fitting tightly about the outer diameter of the lock 3402. The grooves 3410 and/or 3412 in the lock 3402 may hold the tether 3240 in an orientation that prevents the tether 3240 from slipping (e.g., if pulled hard enough) when the lock 3402 is engaged in the pusher 3230. The pusher 3230 may be advanced distally to expose the lock 3402, for example the full length of the lock 3402, or portions thereof. When the proximal end of the tether 3240 is pulled proximally, the knot 3247 falls away from the second groove 3412, advances around the proximal end 3404 of the lock 3402, advances distally by falling away from the first groove 3410, into the cap 3180 and around the pin 3051, and then distally through the opening 3408 of the lock 3402 and can be retrieved with the pusher 3230. In some embodiments, the distal end of the lock 3402 may be located axially proximal to the distal end of the tube 3420, for example to contact the device 3000 with the tube 3420 to prevent proximal movement of the device 3000 after implantation, as described above. Additional embodiments of a delivery system and associate features, such as a

proximal delivery control handle and dual lumen delivery catheter pusher, are described herein, for example with respect to FIGS. 104A-106C.

[0447] 9. Off-Axis Delivery and Deployment

[0448] The device 3000 may be deployed off-axis within an LAA while still providing a complete, stable, and atraumatic seal. In some embodiments, the device 3000 may be deployed at an angle of at least about 15° or 25° and in some embodiments as much as 35° or 45°, for example, relative to a central longitudinal LAA axis and still provide an effective seal. The LAA axis here is defined as the geometric center of the ostium to the LAA, and tracks the best fit geometric center of the LAA cavity.

[0449] This ability of the device 3000 to be deployed off-axis is due in part to the relatively thick, compressible foam body 3002 material, the compliant frame 3040 and the cylindrical shape of the device 3000 with the foam bumper 3026. The device 3000 is stable within the LAA despite having a length that is less than the diameter, or having $L/D < 1$. As described, the length may be 20 mm for the device 3000 having an OD of both 27 mm and 35 mm. Thus not only is flexibility and simplicity allowed with manufacturing processes by having one length, but also stability and effectiveness of the device in use. Further, the axial compressibility of the bumper 3026, combined with the axially compliant frame 3040, allows a 20 mm long device 3000 to be placed within a 10 mm deep LAA, whereas existing LAA closure devices require longer landing zones, or at least landing zones equal to the size of the length of the metallic frame.

[0450] In some embodiments, the device 3000 may be configured to allow for sufficient flow of blood in case of accidental embolization, as described herein. Further, the device 3000 may be configured to allow for sufficient flow of blood even if the device 3000 embolizes and is misaligned with the direction of flow of blood. For example, the device 3000 may define a longitudinal axis, and the direction of flow of blood may define a flow axis. The device longitudinal axis may be at an angle with respect to the flow axis and still provide for a sufficient blood flow through the device 3000 should it embolize and lodge within the circulatory system of a patient. Thus, the capabilities of the device 3000 with regard to flow of blood through the device in case of embolization, or tests thereof with water under controlled conditions, as described herein for example with respect to the section “Proximal Cover,” may also apply to the device 3000 in such off-axis configurations or orientations with the circulatory system of the body. The device axis may be at an angle of five, ten, twenty, thirty or more degrees with respect to the flow axis and still provide sufficient flow of blood through the device 3000.

[0451] 10. Anchor/Foam Interface

[0452] As described, the frame 3040 with anchors 3090, 3094 and foam body 3002 may have a variety of geometries, such as lengths, thicknesses, etc. This section discusses some particular embodiments of the frame 3040, in particular the anchors 3090, 3094, and the foam body 3002. FIGS. 94A-94C depict various embodiments of an anchor/foam interface 3500, using the anchor 3090 as an illustrative example. FIGS. 94A-94C are a side cross-section views of a portion of the device 3000 showing an embodiment of the interface 3500. In some embodiments, the outer tips of the anchors 3090, 3094 may, or may not, extend radially beyond

portions of the outer surface 3016 of the foam body 3002, even in an unconstrained configuration, as further described herein.

[0453] The interface 3500 includes a portion of the tubular body 3080 of the frame 3040, having the proximal strut 3082 and the distal strut 3086, as described in further detail herein, for example with respect to FIG. 89A. The anchor 3090 extends radially outwardly in a proximal direction from the frame 3040, such as from the tubular body 3080. The same or similar features and/or functionalities as described in this section with respect to the interface 3500 having the anchor 3090 may apply to other anchor/foam interfaces with other anchors, such as anchor/foam interfaces with the distal anchor 3094. For example, the frame 3080 could have a distal end at the base of the anchor 3094, where the distal apex 3088 is located (see, e.g., FIG. 89A).

[0454] As shown in FIGS. 94A-94C, the anchor 3090 extends outwardly and proximally from the frame 3040, which may be from the proximal apex 3084 as described herein. The anchor 3090 has an axial length L. The length L extends from the distal base of the anchor 3090 at the frame 3040 to a proximal tip 3091 of the anchor 3090. The length L may include only the straight portion of the anchor 3090, for example if the base of the anchor 3090 is bent. In some embodiments, the length L can include the complete anchor 3090, such that L extends axially along the anchor 3090 from a tip 3091 of the anchor 3090 to the frame 3040. The anchor 3090 is shown with a flat end, but it may be sharpened, angled, etc. The length L may extend proximally to the farthest endpoint axially along the length of the anchor 3090, such as to the tip 3091. In some embodiments, L is 2.5 mm, about 2.5 mm, or from about 2.25 mm to about 2.75 mm. The length L may be a variety of other lengths or within other ranges of lengths, for example as described in further detail herein with respect to the anchors 3090, 3094 in the section “Compliant Frame.”

[0455] The anchor 3090 extends at an angle B relative to the proximal strut 3082. In some embodiments, the proximal strut 3082 as shown may be considered a projection of the proximal strut 3082 onto a vertical plane that intersects the longitudinal axis of the device 3000 and the anchor 3090. Thus the angle B may be relative to such plane and/or to the strut 3082. For simplicity, the angle B will be described relative to the strut 3082. The angle B may be 30° or about 30°. The angle B may be a variety of other angles or within ranges of angles, for example as described in further detail herein with respect to the anchors 3090, 3094 in the section “Compliant Frame.” The anchor further has a radial height H. The radial height H may be the radially outermost extent of the anchor 3090, such as the proximal tip 3091 of the anchor 3090. The length L and angle B may define the radial height H of the anchor 3090. The height H may be in a direction perpendicular to the longitudinal axis of the device 3000 (see, e.g., FIG. 87B).

[0456] Further shown is the sidewall 3014 of the foam body 3002. The sidewall 3014 has a thickness T. The thickness T extends radially outward from the inner surface 3018 to the outer surface 3016 of the sidewall 3014. The thickness T may extend radially outward perpendicularly to the longitudinal axis of the device 3000. The thickness T may be equal to a distance from a radially outer portion of the frame 3040 to the outer surface 3016 of the sidewall 3014, for example where the inner surface 3018 of the sidewall 3014 contacts the outside of the frame struts 3082,

3086. The thickness T could be the thickness of the sidewall **3014** in an unconstrained configuration, a compressed configuration while inside the delivery catheter, or a compressed configuration after implantation within the LAA, as further described. The measurement of the thickness T of the sidewall **3014** may be in the same direction as the measurement of the height H of the anchor **3090**. The thickness T of the sidewall **3014** may be 2.5 mm or about 2.5 mm. The thickness T of the sidewall **3014** may be other values or ranges of values, for example as described in further detail herein in the section “Compressible Foam Body.”

[0457] As shown in FIG. **94A**, in some embodiments, the height H of the anchor **3090** may be greater than the thickness T of the foam sidewall **3014**. The difference may be equal to a delta D. The device **3000** may have this configuration in an unconstrained configuration, for example as resting on a tabletop as described herein. The delta D may be from about 0.05 mm to about 5 mm, from about 0.075 mm to about 4 mm, from about 0.1 mm to about 3 mm, from about 0.2 mm to about 2 mm, from about 0.3 mm to about 1.5 mm, from about 0.4 mm to about 1 mm, about 0.5 mm, or 0.5 mm. In some embodiments, these example values for delta D may be negative, where T is greater than H. In some embodiments, the delta D may be zero, as described with respect to FIG. **94B**.

[0458] As shown in FIG. **94B**, in some embodiments, the height H of the anchor **3090** may be the same as or about the same as the thickness T of the foam sidewall **3014**. Thus the delta D may be zero or about zero. The device **3000** may have this configuration in an unconstrained configuration, for example as resting on a tabletop as described herein. The anchors **3090**, **3094** may extend through the foam body **3002** to the outer surface **3016** in the unconstrained configuration, and then extend radially outward beyond the outer surface **3016** when loaded for delivery and/or after implantation in the LAA. In other embodiments, the foam body **3002** is locally compressed so the anchor extends beyond the outer surface **3016**, as further described.

[0459] As shown in FIG. **94C**, the device **3000** may include one or more attachments, such as sutures, for example the attachment **3001** described in further detail herein with respect to FIG. **87D**. The attachment **3001** may connect the foam body **3002** to the frame **3040**. As shown, the attachment **3001** may extend out through the sidewall **3014** and around the outer surface **3016**, back in through the sidewall **3014** and around the frame **3040**, such as around the proximal strut **3082**. The attachment **3001** may locally compress the sidewall **3014** as shown. The sidewall **3014** may have a local radial thickness R. The thickness R may be less than the thickness T. The thickness R may be a local minimum of the thickness of the foam body **3002**. The thickness T may be located adjacent or otherwise around the location of the thickness R. The sidewall **3014** may increase in thickness from the location of the thickness R to the surrounding thicknesses T. The increase may be gradual or abrupt.

[0460] The local compression of the sidewall **3014** may allow for the anchor **3090** to extend proximally and outwardly beyond the outer surface **3016** of the foam body **3002**. As shown, the attachment **3001** may locally compress the thickness of the sidewall **3014** such that the proximal tip **3091** of the anchor **3090** extends at the angle B for the length L beyond the outer surface **3016** of the foam body **3002**. The attachment **3001** may be located proximally to the anchor

3090 as shown, or in other location, such as distally to the anchor **3090**, adjacent the base of the anchor **3090**, farther proximally/distally from the base of the anchor **3090**, etc. The attachment **3090** may be located and configured to allow for local compression of the sidewall **3014** to allow the tip **3091** of the anchor **3090** to extend beyond the outer surface **3016** of the foam that is located directly radially inwardly of the tip **3091** of the anchor **3090**. In some embodiments the attachment **3001** may be located directly radially inwardly of the tip **3091** of the anchor **3090** (e.g., directly “below” the tip **3091** of the anchor **3090** as oriented in the figure). In some embodiments, there may be multiple attachments **3001** distributed axially along the frame **3040** and all contributing to a single local compression of the foam body **3002** about a particular one of the anchors **3090**.

[0461] The foam sidewall **3014** may be compressed into the configuration shown in FIG. **94C** in an unconstrained configuration. The foam sidewall **3014** may be compressed into the configuration shown in FIG. **94C** in a constrained configuration, for example within the delivery catheter or after deployment from the delivery catheter. The foam sidewall **3014** may be compressed into the configuration shown in FIG. **94C** from the configurations shown or described with respect to FIG. **94A** or **94B**. Thus in FIG. **94C**, the height H may equal to or approximately equal to the thickness T, or the height H may be greater or less than the thickness T. In some embodiments, in an unconstrained configuration, the length L is 2.5 mm or about 2.5 mm, the angle B is 30° or about 30°, and the thickness T is 2.5 mm or about 2.5 mm.

[0462] Design of the anchor length may be based on a balance between longer length to provide flexibility to assist with removal, and shorter length for not penetrating through the LAA wall. The anchors **3090**, **3094** may be flexible and capable of bending in the distal direction due to their length. The anchors **3090**, **3094** are thus less likely to tear tissue during repositioning and therefore less traumatic. The anchors **3090**, **3094** may be longer than other tissue engaging features of existing solutions for LAA occlusion. In some embodiments of the device **3000**, the anchors **3090**, **3094** are designed to be long enough to effectively anchor into the LAA wall. The foam body **3002** and corresponding thickness of the sidewall **3014** allows the anchors **3090**, **3094** to have longer length. An advantage of making the anchors **3090**, **3094** longer is to increase their flexibility, making them less damaging to tissue during removal and repositioning. However, anchors **3090**, **3094** beyond a certain length may penetrate through the LAA wall, which is not desirable. The foam body **3002** and thickness thereof assists with preserving the advantageous longer length of the anchors **3090**, **3094** while mitigating the risk of the anchors **3090**, **3094** penetrating through the LAA wall. For example, the foam sidewall **3014** between the struts of the frame **3040** and the tips **3091** of the anchors **3090**, **3094** limits how far the anchors **3090**, **3094** will penetrate allowing for longer and therefore more flexible anchors **3090**, **3094**.

[0463] For example, with a 2.5 mm foam sidewall **3014** thickness, the anchors **3090**, **3094** may be 2.5 mm in axial length and formed at an angle between 30-40 degrees, or 25-45 degrees, off the struts. In some embodiments, as discussed, when the frame **3040** is first placed into the foam body **3002** and anchors **3090**, **3094** pierce into the foam sidewall **3014**, the tips **3091** of the anchors **3090**, **3094** may not extend all the way through the foam as the anchors **3090**,

3094 may be radially too short. In some embodiments, the frame **3040** OD is about 24 mm and the foam body **3002**, such as foam cup shape, has a sidewall **3014** with an ID of about 22 mm. So there may be an interference fit where the frame **3040** bulges into the foam sidewall **3014**. With the anchor **3090**, **3094** length and angle, the tips **3091** of the anchors **3090**, **3094** are at about 27 mm diameter, which corresponds to just getting to the outer surface **3016** of the sidewall **3014**. As discussed, the assembly may be attached by suturing the foam body **3002**, and the frame **3040** (and in some locations the cover **3100**) together at every anchor-frame interface location. This may cause a dimpling of the foam body **3002** local to the corresponding anchor **3090**, **3094**, thus exposing a length of the anchor **3090**, **3094** at the outer surface **3016**. The exposed length of the anchor **3090**, **3094** may be a fraction of the total anchor **3090**, **3094** length. Further, the anchor **3090**, **3094** length and radial height of the foam sidewall **3014** surrounding the anchor **3090**, **3094** can be adjusted to expose the desired amount of the anchor **3090**, **3094**.

[0464] In some embodiments, the tip **3091** may be exposed beyond the foam body **3002** when the foam is compressed, but the tip **3091** may be positioned within the foam, below the outer surface **3016**, when the foam is uncompressed. Thus, with the foam uncompressed the tip **3091** may not be positioned radially outwardly relative to the outer surface **3016**, but with the foam compressed the tip **3091** may be positioned radially outwardly relative to the adjacent portion of the outer surface **3016**. Therefore, the tip **3091** may not be exposed with “H” less than “T” in the uncompressed configuration, and the tip **3091** may be exposed with “H” greater than “T” in the compressed configuration.

[0465] 11. Device Compliance

[0466] The device **3000** is capable of conforming to the geometry of the LAA. The device **3000** is designed for compliance such that it can conform to the LAA and reduce or minimize remodeling of the LAA. For example, the device **3000** may be implanted into the LAA and after a period of time the ostium or opening of the LAA may have the same or similar profile as before implantation of the device **3000**. Further, the device **3000** may exhibit such properties while conforming to extreme non-circular shapes, both at the opening of the LAA and within the LAA. A single size of the device **3000** may be used for all or a wide range of patients with varying geometries, due to the compliance and other advantages.

[0467] FIG. 95A is a schematic showing an embodiment of a profile of the ostium **110**. The view shown may be looking into the LAA, for example in a plane that is perpendicular to a geometrically centered axis at the ostium. The geometry of the ostium **110** may vary greatly, as described herein, for example with respect to FIG. 1. As shown in FIG. 95A, the ostium may be approximated as an oval or ellipse having a relatively shorter minor axis **A1** and relatively longer major axis **A2**. The ostium **110** is shown as generally symmetric about the axes **A1**, **A2**, but the ostium **110** may have asymmetries, other local grooves, discontinuities, etc. Thus the ostium **110** schematic shown is merely for illustrative purposes to describe the enhanced compliance capabilities of the device **3000**. In some embodiments, the minor axis **A1** may refer to a maximum width of the ostium **110** in a first direction, and the major axis **A2** may

refer to a maximum width in a second direction. The first direction may be perpendicular to the second direction.

[0468] The lengths of the axes **A1**, **A2** may have a variety of values or ranges of values. The minor axis **A1** may be from about 5 mm to about 30 mm, from about 7.5 mm to about 20 mm, from about 10 mm to about 17.5 mm, from about 12 mm to about 15 mm, about 14 mm, or 14 mm. The major axis **A2** may be from about 10 mm to about 40 mm, from about 15 mm to about 37 mm, from about 20 mm to about 35 mm, from about 22 mm to about 32 mm, from about 25 mm to about 30 mm, about 27 mm, or 27 mm.

[0469] FIG. 95B shows the ostium **110** from the same perspective but with the device **3000** implanted into the LAA. The cover **3100** is visible, showing the proximal surface **3102** with proximal openings **3122**. Other covers as described herein may be included, such as the cover **3150**, etc. The ostium in **110** with the device **3000** may have the same or similar shape and size as the ostium shown in FIG. 95A without the device **3000**. The other portions of the LAA may also have the same shape and sizes before and after implantation of the device **3000**. The device **3000** may therefore conform to the shape of the LAA, such as the ostium **110**. The device **3000** may conform to the anatomical shape due to the configuration of the foam body **3002** and frame **3040** as described herein. The device **3000** may exhibit sufficient compliance to assume the anatomical shape to provide a sufficient occluding function and without remodeling or otherwise deforming the shape of the LAA, such as the ostium **110**.

[0470] The LAA may retain the same or similar original size and shape of the LAA immediately after implantation of the device **3000** and for a period of time thereafter. In some embodiments, the anatomical geometry, for example size and shape, of the LAA will still be the same or approximately the same after implantation of the device **3000** after a period of twenty four hours or more, seven days or more, thirty days or more, six months or more, one year or more, five years or more, or longer periods. A test construct having approximately the same geometry, stiffness, etc. may be constructed to confirm the minimal long-term changes in the construct due to the device **3000**. A construct having an opening with a minor axis of about 14 mm and a major axis of about 27 mm and with a stiffness generally present in normal LAA ostiums of patients may have the same or similar size and shape after implanting the device **3000** for the aforementioned periods. The device **3000** may allow for the same or similar geometry along the length of the LAA, e.g. distal to the ostium **110**, for these periods of time as well, as further described.

[0471] In one example use, the device **3000** may be configured to insert into a non-cylindrical opening, having a non-cylindrical profile, of a test body. The test body may be rigid such that the test body does not deform in response to the device **3000** being implanted therein. The test body may be formed of rigid plastics, metals, etc. The opening and profile may have a size and shape substantially similar to that of a native left atrial appendage. The device **3000** may expand radially within the non-cylindrical opening, and conform to the non-cylindrical profile, which may be at least at the opening of the test body. The device **3000** may conform to the opening and have no visible gaps between the device **3000** and the opening. There may be one or more radial gaps that are each no more than five, four, three, two and/or one millimeter across at their widest portion. Such

gaps may be measured radially, or perpendicularly to a longitudinal axis extending through the geometric center of the test body opening. The gap may be measured between the outer surface of the device 3000 and the inner surface of the opening of the test body. The gap may be measured at the location of maximum space between the device 3000 and the test body. The device may conform to this shape after a period of at least thirty days, at least sixty days, and/or at least one hundred twenty days after implantation. In another example use, the device 3000 may be configured to insert into a non-cylindrical opening of a test body having a size and radial stiffness substantially similar to that of a native left atrial appendage, expand radially within the non-cylindrical opening, and assume a non-cylindrical profile at least at the opening of the test body after a period of at least thirty days, at least sixty days, and/or at least one hundred twenty days.

[0472] FIG. 96A depicts a side view of the device 3000 in a radially constrained configuration. The device 3000 may have the configuration shown after implantation in the LAA, for example after the aforementioned time periods above. The device 3000 is shown with a proximal end 3004 having a width D1 and a distal end having a width D2. The widths D1, D2 may be diameters, or they may be maximum widths of the respective ends of the device 3000. The width D1 is greater than the width D2. In some embodiments, the width D1 may be less than the width D2. In some embodiments, the width D1 may be equal to or approximately equal to the width D2. In some embodiments, the width D2 may be about 15% of the width D1. The width D2 may be 95% or less, 90% or less, 85% or less, 80% or less, 75% or less, 70% or less, 65% or less, 60% or less, 55% or less, 50% or less, 45% or less, 40% or less, 35% or less, 30% or less, 35% or less, 30% or less, 25% or less, 20% or less, 19% or less, 18% or less, 17% or less, 16% or less, 15% or less, 14% or less, 13% or less, 12% or less, 11% or less, or 10% or less of the width D1. In some embodiments, the width D2 may be at other locations along the device 3000 alternatively or in addition to the distal end of the device 3000, for example a portion proximal to and adjacent or near the distal end, a middle portion of the device 3000, etc. In some embodiments, the entire device 3000 or a substantial portion of the device 3000 may have the width D2. For example, the entire device may have the width D2 when constrained within the delivery catheter, as described herein for example in the section "Loading System."

[0473] FIG. 96B depicts a side view of the device 3000 in an axially constrained configuration relative to an axially unconstrained configuration. The device 3000 has an axial length L1 in an unconstrained state, and an axial length L2 in the constrained state. The lengths L1, L2 between the proximal end 3004 and the distal end 3006 of the device 3000 in the respective configurations. The device 3000 may have the configuration shown with the length L2 after implantation in the LAA, for example after the aforementioned time periods above. The length L2 is less than the length L1. The length L2 may be 95% or less, 90% or less, 85% or less, 80% or less, 75% or less, 70% or less, 65% or less, 60% or less, 55% or less, 50% or less, 45% or less, or 40% or less of the length L1. In some embodiments, L2 may be equal to or approximately equal to L1.

[0474] In some embodiments, the bumper 3026 may allow for extreme shortening of the distal end 3006 of the device. In some embodiments, the bumper 3026 may fold inward to

accommodate radial and/or axial constraining of the device 3000. The bumper 3026 may fold radially inward and/or proximally inward. Further, the compliant frame 3040 within the foam body 3002 may allow for further axial shortening beyond the length of the bumper 3026. The frame 3040 may fold radially and/or axially inward.

[0475] Further, the cylindrical shape of the device 3000 facilitates with sealing the LAA, even with atypical geometries of the LAA anatomy. The cylindrical shape ensures that the anchors are located at the locations of maximum width of the device 3000. The tubular body 3080 may provide a cylindrical foundation for the anchors 3090, 3094, as described herein, such that the anchors are located at the radially outer most portion of the device 3000. Such cylindrical shape of the device along its longitudinal axis assists with the device 3000 performing the necessary sealing, even in the constrained configurations shown in FIGS. 96A and 96B. In some embodiments, the device 3000 may be constrained both axially and radially, for example with both of the deformations shown in FIGS. 96A and 96B. The compliance of the device 3000 along with the cylindrical shape can ensure superior sealing performance compared to currently available typical LAA occlusion devices.

[0476] FIG. 97 is a side view of an embodiment a laser cut tube frame 3040 shown in a flat configuration. The frame 3040 may have the various dimensions as shown in inches. The dimensions are just one embodiment and some or all dimensions may be different in other embodiments. The hub 3050 is located at a proximal end having holes 3053. The struts 3061 extend distally from the hub 3050, having curved (when assembled) proximal portions 3062, straight portions 3064, and outer curved (when assembled) portions 3066. The struts 3061 connect at proximal apexes 3084 to the proximal struts 3082. Proximal anchors 3090 extend proximally from intermediate vertices 3087. Distal struts 3086 extend from the vertex 3087 to form the distal apexes 3088, from which the distal anchors 3094 extend proximally. The frame 3040 may have approximately the dimensions shown, or they may vary therefrom. The frame 3040 shown may be used with the device 3000 having a width of 27 mm or about 27 mm.

[0477] The device 3000 provides many advantages over existing solutions to LAA occlusion, as described herein. A key advantage is that the device is highly compliant while still providing superior resistance to embolization. This unique feature of being more compliant yet better anchoring is counterintuitive. As compared to existing solutions, the device 3000 is much more conformable and thus able to take the oval shape of the LAA ostium, as described, while also providing superior dislodgement resistance, in some embodiments with a pull out force in bench testing of greater than 0.8 pounds (lbs).

[0478] 12. Conformability

[0479] The device 3000 provides superior conformability to a range of different shapes and sizes of LAA's compared with existing solutions to LAA occlusion. This section further details some of the features of the device 3000 that contribute to its conformability, among other advantages. For example, some of the features described herein relate to the shape or contour of the proximal face 3060, the angular transition between the proximal face 3060 and the tubular body 3080, the lengths of the struts 3082, 3086 forming the diamond or square shapes along the tubular body 3080, and the angles of the proximal and distal apexes 3084, 3088 of

the diamond or square shapes. For instance, and as further detailed herein, the frame **3040** may have a flat or substantially flat shape or contour of the proximal face **3060**, a 90° or approximately 90° angular transition between the proximal face **3060** and the tubular body **3080**, relatively short lengths of the struts **3082**, **3086** forming the diamond or square shapes along the tubular body **3080**, and relatively larger angles of the proximal and distal apices **3084**, **3088** of the diamond or square shapes.

[**0480**] FIGS. **98A-98C** are various views of the frame **3040** indicating some of the structural aspects contributing to the LAA occlusion device's **3000** conformable capabilities. FIG. **98A** is a side view of the frame **3040**. FIG. **98B** is a detail view of a portion of the frame **3040** showing the detail region **98B** as labelled in FIG. **98A**. FIG. **98C** is a detail view of a portion of the frame **3040** showing the detail region **98C** as labelled in FIG. **98A**. The frame **3040** in FIGS. **98A-98C** is shown in an unconstrained configuration, for example after deployment from a delivery catheter and without any outside forces acting radially inwardly on the device frame **3040**.

[**0481**] As shown in FIG. **98A**, the frame **3040** includes the proximal face **3060** having a plurality of the proximal struts **3061**, and a tubular body **3080** or "landing zone" extending distally from the proximal face **3060**, between a proximal transition and a distal end. The frame **3040** includes the proximal anchors **3090** and distal anchors **3094** extending from the tubular body **3080**, as described. The anchors **3090**, **3094** incline radially outward in a proximal direction from the tubular body **3080**.

[**0482**] As indicated in FIG. **98A**, the anchors **3090** in an unconstrained configuration may extend at an angle C with respect to the central longitudinal axis defined by the frame **3040**. The angle C may be from 25° (degrees) to 45°, about 35°, or 35°. In some embodiments, the angle C may be from 5° to 65°, from 10° to 60°, from 15° to 55°, from 20° to 50°, from 25° to 45°, or from 30° to 40°. In some embodiments, the angle C is 25°, 26°, 27°, 28°, 29°, 30°, 31°, 32°, 33°, 34°, 35°, 36°, 37°, 38°, 39°, 40°, 41°, 42°, 43°, 44°, or 45°. The distal anchor **3094** may also be inclined at any of the angles C as described with respect to the proximal anchor **3090**. The distal anchor **3094** may be inclined at the same or different angle as the proximal anchor **3090**. Each of the proximal anchors **3090** may be inclined at the same angle **25** as the other proximal anchors **3090**, or some may be inclined at different angles as compared to others of the proximal anchors **3090**. Similarly, each of the distal anchors **3094** may be inclined at the same angle as the other distal anchors **3094**, or some may be inclined at different angles as compared to others of the distal anchors **3094**.

[**0483**] The frame **3040** further includes the proximal face **3060** defined at least partially by a plurality of the proximal struts **3061**, as described. The struts **3061** each include a straight portion **3064** extending radially outward and defining a line. The plurality of straight portions **3064** may extend radially outward and together define a geometric surface.

[**0484**] As indicated in FIG. **98A**, the straight portions **3064**, or the lines or surface defined thereby, in an unconstrained configuration may extend at an angle D with respect to the central longitudinal axis. The angle D may be from 85° (degrees) to 110°, about 100°, or 100°. Thus the straight portions **3064** in an unconstrained configuration may extend radially outward in a distal direction or directly radially outward. In some embodiments, the straight portions **3064** in

an unconstrained configuration may extend radially outward in a proximal direction. In some embodiments, the angle D may be from 80° to 120°, from 85° to 115°, or from 95° to 105°. In some embodiments, the angle D may be greater than 90°. In some embodiments, the angle D may be greater than 80°, greater than 85°, greater than 95°, greater than 100°, greater than 105°, or greater than 110°.

[**0485**] The angle D is measured relative to a straight collinear extension of the part of the strut **3061**, which may be or include the straight portion **3064**, as mentioned. In some embodiments, the straight portion **3064** may not be perfectly straight. It may be slightly curved, have one or more curved portions therein, or not be perfectly flat, for example as further described with respect to FIG. **98B**. In such cases, the angle D may be measured from a straight part of the strut **3061**, if any, or the angle D may be measured from a line of best fit as determined by the straight portion **3064**.

[**0486**] FIG. **98B** shows a detail of the region **98B** as indicated in FIG. **98A**. As shown in FIG. **98B**, the strut **3061** extends radially outward from the hub **3050** to the proximal strut **3082**. The strut **3082** may be part of the tubular body **3080** or "landing zone" as described herein. In particular, the strut **3061** includes the inner curved portion **3062** extending arcuately from the hub **3050** in the distal and radially outward directions, to the straight portion **3064** extending radially outwardly, and to the outer curved portion **3066** extending arcuately in the distal direction, as described herein. The outer curved portion **3066** is connected with the proximal strut **3082** of the tubular body **3080**, as described.

[**0487**] As indicated in FIG. **98B**, the straight portion **3064** of the proximal face strut **3061** and the proximal strut **3082** of the tubular body **3080** may be angled relative to each other at an angle E. The angle E may be measured relative to the straight portion **3064**, for example relative to a line, plane and/or surface defined by the straight portion **3064**, as described with respect to FIG. **98A**. The angle E may be measured relative to the outer surface of tubular body **3080** or portions thereof. For example, the proximal strut **3082** may extend distally along a linear or curved path, as viewed from the side. The strut **3082** is shown as curved, but it may be straight or define a line of best fit. Similarly, the distal struts **3086** of the tubular body **3080** may be curved, straight, and/or define a line of best fit, as viewed from the side. Further, the proximal and distal struts **3082**, **3086** may together define a line, plane, and/or surface, as viewed from the side. For example, the tubular body **3080** may be cylindrical or generally cylindrical, as described, and thus the proximal and distal struts **3082**, **3086** may together define a line, plane, and/or surface, that as viewed from the side is parallel or substantially parallel to the longitudinal axis. In some embodiments, the proximal and distal struts **3082**, **3086** may together define a curved path and/or surface, that as viewed from the side initially extends distally and radially outward and then distally and radially inward, and from which a line of best fit may be determined. The angle E may thus be measured relative to any of these geometric references of the tubular body **3080**.

[**0488**] In some embodiments, the angle E is measured relative to portions of the frame located on either side of the curved portion **3066**. The proximal end of the curved portion **3066** may be attached to a radial outer end of the straight portion **3064**. The angle E may be measured relative to this radial outer end of the straight portion **3064**. The distal end

of the curved portion **3066** reaches a transition to a proximal end of the proximal strut **3082**, for example at the proximal apex **3084** as described herein and as shown in FIG. **98C**. The angle E may be measured relative to this proximal end of the proximal strut **3082**.

[**0489**] The angle E may be 90° or about 90° . In some embodiments, the angle E is from 70° to 110° , from 75° to 105° , from 80° to 100° , or from 85° to 95° . In some embodiments, the angle E is greater than 90° . In some embodiments, the angle E is greater than 70° , greater than 75° , greater than 80° , greater than 85° , greater than 95° , or greater than 100° .

[**0490**] Further, the inner curved portion **3062** may have a radius R1 as indicated in FIG. **98B**. The radius R1 may have a proximally-facing concavity as shown, i.e. a positive or upward concavity as oriented in the figure.

[**0491**] The substantially straight portion **3064** may have a radius R2 to produce a distally facing concavity and proximally facing convex surface. In some embodiments, the radius R2 is infinite, where the straight portion **3064** is linear. The straight portion **3064** as shown may therefore not have a concavity, whether proximally-facing or distally-facing. In some embodiments, the straight portion **3064** may have a slight concavity proximally and/or distally. The portion **3064** may have a single concavity from inner transition to curve **3062** to outer transition **3066** without any points of inflection. The concavity may have a radius R2 of at least about 2 cm, 5 cm or 10 cm or more.

[**0492**] As shown, the straight portion **3064** extends radially inwardly to an inner transition to the inner curved portion **3062**. The entire straight portion **3064** may therefore be located distally of the inner curved portion **3062** in the unconstrained configuration as shown. In some embodiments, the entire straight portion **3064** is located distally of a distal end of the inner curved portion **3062**. In some embodiments, all portions of the strut **3061** besides the inner curved portion **3062** are located distally of the inner curved portion **3062**, and there are no points of inflection along the strut portion **3064**.

[**0493**] The straight portion **3064** may have a flatness defined by a width S as indicated in FIG. **98B**. The straight portion **3064** may extend radially outward between the two parallel closest fit geometric reference lines that are separated by the width S. The width S may be the strut width, for example where the straight portion **3064** is perfectly straight. In some embodiments, the width S may be no greater than 0.2 mm, no greater than 0.3 mm, no greater than 0.4 mm, no greater than 0.5 mm, no greater than 0.6 mm, no greater than 0.7 mm, no greater than 0.8 mm, no greater than 0.9 mm, no greater than 1 mm, no greater than 1.1 mm, no greater than 1.2 mm, no greater than 1.3 mm, no greater than 1.4 mm, or no greater than 1.5 mm more than the strut width.

[**0494**] The outer curved portion **3066** may have a radius R3 as indicated in FIG. **98B**. The radius R3 may have a distally-facing concavity as shown, i.e. a downward concavity as oriented in the figure. The radius R3 may be 1 mm or about 1 mm. In some embodiments, the radius R3 may be from about 0.2 mm to 2 mm, from about 0.3 mm to 1.8 mm, from about 0.4 mm to 1.6 mm, or from about 0.5 mm to 1.4 mm.

[**0495**] The radius R3 may extend along an arc having an arc length. The arc length may be measured from a first transition between a radially outward end of the straight portion **3064** to a second transition to the proximal end of the

strut **3082**, for example at the proximal vertex **3084** (shown in FIG. **98C**, for example). This arc length may be no greater than 0.2 mm, no greater than 0.3 mm, no greater than 0.4 mm, no greater than 0.5 mm, no greater than 0.6 mm, no greater than 0.7 mm, no greater than 0.8 mm, no greater than 0.9 mm, no greater than 1.0 mm, no greater than 1.1 mm, no greater than 1.2 mm, no greater than 1.3 mm, no greater than 1.4 mm, no greater than 1.5 mm, no greater than 1.6 mm, no greater than 1.7 mm, no greater than 1.8 mm, no greater than 1.9 mm, or no greater than 2.0 mm.

[**0496**] FIG. **98C** shows a detail of the region **98C** as indicated in FIG. **98A**. As shown in FIG. **98C**, the quadrilateral shape defined by the struts **3082** and **3086** may define angles G and F as indicated. The angles G may be defined by the proximal and distal apices **3084**, **3088**. The angles G may therefore be measured between adjacent proximal struts **3082** and between adjacent struts **3086**. The two angles G may be the same or within about 2° or 4° of each other. In some embodiments, the angles G may be different for the proximal apex **3084** as compared to the distal apex **3088**, for example where one or more of the struts **3082**, **3086** forming the quadrilateral shape are a different length than the other struts. The angles F are defined between adjacent proximal and distal struts **3082**, **3086** as indicated.

[**0497**] The angles G and F may each be 90° in the unconstrained configuration. In some embodiments, the angles G and F may each be approximately 90° such as within about $+1^\circ$, $+2^\circ$, $+4^\circ$ or $+6^\circ$ of 90° . Thus the quadrilateral formed by the struts **3082**, **3086** may be a square or approximately a square. The angles G may be no less than 85° . In some embodiments, the angles G may be no less than 45° , no less than 50° , no less than 55° , no less than 60° , no less than 65° , no less than 70° , no less than 75° , no less than 80° , or no less than 90° . The sum of the four angles G and F may be 360° . Thus, the angles F may each be equal to $(360^\circ - (2 \times G))/2$.

[**0498**] The quadrilateral shapes defined by the struts **3082**, **3086** may define a longitudinal length between opposing apices **3084** and **3088**, for example between opposing apices forming angles G. A longitudinal distance between a proximal apex **3084** and an opposing distal apex **3088** may be no more than 5 mm, no more than 4.5 mm, no more than 4 mm, no more than 3.5 mm, no more than 3 mm, no more than 3 mm, or no more than 2.5 mm.

[**0499**] The various structural aspects detailed in this section and elsewhere contributes to the enhanced conformability of the device **3000**. For example, the struts **3082**, **3086** of the tubular body **3080** may be mechanically independent such that applying a radially inward force on one strut of the struts **3082**, **3086**, or on one of the quadrilateral shapes defined by four adjacent struts **3082**, **3086**, does not cause the adjacent struts or quadrilateral shapes to collapse in a similar manner. Such radial force may cause the perimeter of the frame **3040** to instead bulge out. The struts **3082**, **3086** may therefore behave independently which contributes to allowing the device **3000** to conform to various and extremely non-circular, for example oval, cross sectional shapes of LAA's, as further described herein, for example with respect to FIGS. **95A-95B** and **99A-99B**, while still providing a fully sealed and occluded LAA.

[**0500**] Further, the relatively shorter longitudinal lengths between opposing apices **3084**, **3088**, the flat shape of the proximal face **3060**, and the approximately 90° transition between the proximal face **3060** and the tubular body **3080**

each provides enhanced conformability capabilities, as further described herein for example with respect to FIGS. 95A-95B and 99A-99B.

[0501] This conformability of the device 300 allows the device 3000 to be sized based on the average diameter of a patient's LAA, and not the maximum diameter which is used for other existing LAA occluders. This allows a given size of the device 300 to effectively seal a much larger range of LAA sizes, simplifying the implantation procedure and reducing costs associated with design and manufacturing.

[0502] An advantage of the device 3000 that contributes to its conformability is that when the device 3000 is compressed radially along a first, transverse axis, the average diameter remains relatively constant. As the frame 3040 is compressed to create a short, minor axis, the opposing major axis lengthens, maintaining the overall circumference or average diameter. This is in contrast to existing solutions for LAA occlusion devices, where compression of the outer diameter causes an inward collapse of the struts on the proximal side, resulting in an overall lengthening of the device in the distal and proximal directions.

[0503] FIGS. 99A-99B are top views of the device of FIGS. 85A-88E shown, respectively, in an uncompressed configuration and a compressed configuration. The device 3000 shown may have the same or similar features and/or functions as the devices described herein, for example with respect to FIGS. 85A-88E.

[0504] FIG. 99A shows the device 3000 unconstrained prior to application of a compressive radial force P on opposing sides of the device 3000. The force P may be applied by two planar plates located on opposite sides of the device 3000. The plates may be brought together a desired distance to compress the device 3000, where the device 3000 takes an oval-like shape, such as that shown in FIG. 99B.

[0505] FIG. 99B shows the device 3000 compressed after being inserted into a collapsible tube 4000 and compressed to form a minor axis and mimic deployment within a non-cylindrical LAA. The tube 4000 has a wall 4002 with an inner surface 4004 and an outer surface 4006. The wall 4002 may extend along the longitudinal length of the device 3000. The tube 4000 may be compressed by the compressive radial forces P as shown such that the device 3000 takes the oval-like shape shown. The tube 4000 may be an elastic tube capable of compression, either by hand or by two plates as mentioned. The device 3000 may be placed into the circular tube 4000 and then the tube 4000 may be compressed. Or the tube 4000 may be pre-compressed to have the oval-like shape, and then the device 3000 may be deployed within the tube 4000 to take the pre-existing shape of the tube 4000.

[0506] The compressed device 3000 may have a minor axis A1 and a major axis A2, where the minor axis A1 is shorter than the major axis A2. As the device 3000 is compressed, A1 may decrease relative to a starting uncompressed width W (see FIG. 99A) as A2 increases relative to the starting uncompressed width W. A mean diameter "MD" may be calculated based on the resulting minor axis A1 and major axis A2. MD may be equal to $(A1+A2)/2$. The mean diameter MD may remain constant or relatively constant before, during and after compression. Thus the MD as calculated for the configuration in FIG. 99A (for example, where $A1=A2=W$) may be equal to or approximately equal to the MD as calculated for the configuration in FIG. 99B. In some embodiments, the compressed MD for the device 3000 may be within 98% or more, within 96% or more,

within 94% or more, within 92% or more, within 90% or more, within 88% or more, within 86% or more, within 84% or more, within 82% or more, or within 80% or more of the uncompressed MD for the device 3000.

[0507] In some embodiments, the device 3000 may seal LAA's having widths that are larger than the uncompressed MD of the device 3000, as long as the MD of the LAA is less than or equal to the uncompressed MD of the device minus 2 mm. In other words, for this embodiment, $MD_{LAA} \leq (MD_{DEVICE} - 2 \text{ mm})$. Thus the device 3000 may be used for extreme oval shapes where the major diameter of the oval shape is larger than the uncompressed diameter of the device 3000, due to the conformable features of the device 3000. Other sizes of the device 3000 for other ranges of sizes of ostia may be similarly determined based on the MD.

[0508] As an example, the device 3000 having an uncompressed MD of 27 mm may be used to seal and anchor in a 25 mm diameter or smaller circular hole. Thus, for oval-shaped holes, the device 3000 having an uncompressed MD of 27 mm may be used to seal any oval having an MD that is less than or equal to 25 mm. For example, an oval having a major diameter of 27 mm and a minor diameter 20 mm results in an MD of 23.5 mm, which is less than or equal to 25 mm, and thus the device 3000 having an uncompressed MD of 27 mm may be used for that oval shaped ostium. As further example, an oval having a major diameter of 30 mm and a minor diameter 16 mm results in an MD of 23 mm, which is less than or equal to 25 mm, and thus the device 3000 may be used for that oval shaped ostium. As further example, an oval having a major diameter of 38 mm and a minor diameter 10 mm results in an MD of 24 mm, which is less than or equal to 25 mm, and thus the device 3000 may be used for that oval shaped ostium.

[0509] Any of the above relationships for the compressed and uncompressed MD may apply for various compressions of the device 3000 from a starting uncompressed width W, as shown in FIG. 99A. The above relationships between the compressed and uncompressed MD may apply where the device 3000 is compressed such that the compressed minor diameter A1 (shown in FIG. 99B) is no more than 90%, no more than 80%, no more than 70%, no more than 60%, no more than 50%, no more than 40%, no more than 30%, or no more than 20% of W. Thus, for example, in some embodiments, the compressed MD for the device 3000 may be within 90% or more of the uncompressed MD for the device 3000 when the device 3000 is compressed such that the compressed minor diameter A1 is less than 30% of W.

[0510] Further, the major axis A2 of the compressed device 3000 may be larger than, and in some cases much larger than, the starting width W of the uncompressed device 3000. In some embodiments, the major axis A2 may be more than 100%, more than 105%, more than 110%, more than 115%, more than 120%, more than 125%, more than 130%, more than 135%, more than 140%, more than 145% or more than 150% of W.

[0511] Further contributing to the enhanced sealing capability of the device 3000 is the behavior of the circumference of the device 3000. As shown in FIGS. 99A and 99B, the device 3000 may have a circumference C as measured along a perimeter of the device 3000, which may be at or near a proximal end of the device 3000. In cylindrical embodiments, the circumference C may also be measured in other locations, for example at or near the distal end of the device 3000, or between proximal and distal ends.

[0512] The circumference C, as measured at a given longitudinal point along the length of the device 3000, may be the same or approximately the same in the uncompressed and compressed configurations, for example in the configurations of FIG. 99A and FIG. 99B respectively. In some embodiments, the circumference C of the compressed device 3000 may be within 1%, within 2%, within 3%, within 4%, within 5%, within 6%, within 7%, within 8%, within 9%, within 10%, or within 15% of the circumference C of the uncompressed device 3000 measured at the same longitudinal transverse plane. Such relationships for the compressed and uncompressed circumferences may apply along with any of the other described relationships herein, such as the relationships between A2 and W, between A1 and W, and/or between the compressed MD and uncompressed MD.

[0513] The above relationships of the device 3000 may be tested using the plates (for example a vice) or tube as shown and described with respect to FIGS. 99A and 99B, respectively. For example, the device 3000 having a 27 mm diameter (width W) may be placed in a metal vice submerged within a body temperature saline bath. The vice may be initially set with an opening of 25 mm. The vice may then be closed to discrete distances between the plates. At each measurement point, the minor axis A1 (equal to the opening of the vice) and major axis A2 of the compressed device 3000 may be determined. The mean diameter MD may be calculated based on the determined lengths A1 and A2. The circumference may be measured, or otherwise determined based on known geometric equations for calculating a circumference based on A1 and A2.

[0514] Another feature of the device 3000 that contributes to the enhanced sealing capability is the foam body 3002. The foam material of the body 3002 has a stiffness that may naturally bow radially outward, as opposed to collapsing inwards like the existing prior art devices that have polyester or ePTFE fabric which can “scallop” to form outward concavities between struts which may cause residual leaks. In contrast, the device 3000 has foam in the body 3002 which provides more stiffness and shape memory than knitted or woven polyester fabric or the like, contributing to the device's 3000 ability to conform to the irregular geometry of the interior surface of the LAA and thereby provide a better seal.

[0515] The device 3000 may also apply less of a radial outward force on the LAA while providing a superior seal, as compared to existing LAA occlusion devices. Thus the device 3000 may provide a “softer” solution for LAA occlusion devices. The radial stiffness of the device, which is an indication of the radial outward force the device 3000 would apply to an LAA, may be tested. For example, the device 3000 may be compressed, for example using the vice discussed in connection with FIG. 99A and/or a compressive force gauge, to measure the applied force. The applied force may then be compared to the resulting change in the width W of the device 3000 due to the applied force. In some embodiments, the required force in pounds (lbs) to compress the device 3000 a distance of D in inches (in) may be within 20%, within 15%, within 10%, or within 5% of F, where $F=0.44D+0.04$.

[0516] FIGS. 100A-100C are data plots 5000, 5100, 5200 respectively of test results showing various structural characteristics for certain embodiments of the device of FIGS. 85A-88E. FIG. 100A shows the data plot 5000 for the

relationship between the mean diameter MD of the device 3000 (on the Y axis) and the minor diameter A1 or “short axis” of the device 3000 (on the X axis). FIG. 100B shows the data plot 5100 for the relationship between the major diameter A2 or “long axis” of the device 3000 (on the Y axis) and the minor diameter A1 or “short axis” of the device 3000 (on the X axis). FIG. 100C shows the data plot 5200 for the relationship between an applied compressive force to the device 3000 (on the Y axis) and the decrease in the width W of the device or “compression” (on the X axis).

[0517] As the minor axis is compressed by 10 mm from an unconstrained diameter such as from 25 mm (in an unconstrained 25 mm device, or at a starting diameter of 25 mm in a larger device) to 15 mm, the mean diameter has a reduction of no more than about 5 mm, and preferably no more than about 3 mm or 2 mm or 1 mm or less. As the minor axis is compressed by 15 mm such as from 25 mm to 10 mm, the mean diameter has a reduction of no more than about 8 mm, and preferably no more than about 6 mm or 4 mm or 3 mm or less. As the implant is compressed from an unconstrained configuration starting diameter to a minor axis diameter that is 15 mm less than the starting diameter, the mean diameter has a reduction of no more than about 10 mm and in some implementations no more than about 8 mm or 6 mm or 4 mm or 3 mm or 2 mm or less, depending in part upon the starting diameter.

[0518] Referring to FIG. 100B, reduction of the short axis by 10 mm such as from 25 mm (unconstrained) to 15 mm produces an elongation of the major axis of at least about 2 mm and in some implementations at least about 4 mm or 6 mm or 8 mm or 10 mm or more. Reduction of the short axis by 20 mm such as from 25 mm (unconstrained) to 5 mm produces an elongation of the major axis of at least about 2 mm and in some implementations at least about 4 mm or 8 mm or 10 mm or more, enabling the implant to conform to a wide variety of non cylindrical LAA configurations.

[0519] Referring to FIG. 100C, Application of 0.10 lbs compressive force produces a compression along the minor axis of at least about 0.05 inches or 0.10 inches or 0.20 or more. Application of 0.20 lbs compressive force produces a compression along the minor axis of at least about 0.15 inches or 0.20 inches or 0.25 inches or 0.30 inches or 0.40 inches or more. Application of no more than about 0.37 lbs or 0.33 lbs. or 0.30 lbs or 0.27 lbs or less compressive force produces a compression along the minor axis of at least about 0.35 inches or 0.40 inches or 0.45 inches or 0.50 inches or more to produce a soft and conformable implant.

[0520] The foregoing relationships can be scaled and converted to a percent basis to apply to implants having an unconstrained expanded diameter that differs from 25 mm.

[0521] FIG. 101 is a schematic of an embodiment of a test setup 5300 that may be used to perform a flat plate test method, such as described herein, to characterize the stiffness and other structural attributes of the device 3000. The data plots 5000, 5100, 5200 in FIGS. 100A-100C may be generated using the test setup 5300. The test setup 5300 may thus be used for determining whether a given occlusion device exhibits the same or similar structural characteristics as the device 3000.

[0522] As shown in FIG. 101, the test setup 5300 includes a volume 5310, which may be a bath. The volume 5310 contains water 5320. The water 5320 may partially or completely fill the volume 5310. A thermal conditioner 5350, such as heating or cooling device, may be used to heat

or cool the water to the desired temperature. A recirculator **5360**, such as a pump, may be used to recirculate the water to provide a uniform distribution of temperature in the water.

[0523] The test setup **5300** further includes a mechanical press **5330**. The press **5330** may be a compression test stand. A variety of suitable compression test apparatuses known in the art may be used for the press **5330**. The press **5330** may be submerged, partially or completely, in the water **5320**. The press **5330** may be a vertical press as shown. A horizontal arrangement may be used. The press **5330** may have a graduated scale or scales. The press **5330** includes a lower plate **5332** having a force gage **5334** thereon. The force gage **5334** may instead be located on an upper plate. The force gage **5334** detects a compressive force and provides output indicative of the compressive force applied to the gage **5334**. The gage **5334** may be fitted with or include a flat surface for applying compression to the device **3000**. The occlusion device **3000** is shown located on top of the force gage **5334**, with an upper moveable plate **5336** located above the device **3000**. In some embodiments, the force gage **5334** may be located on top of the device **3000**, for example on an underside (as oriented in the figure) of the upper plate **5336**.

[0524] The upper plate **5336** is lowered from the position shown by dashed outline to contact the upper side of the device **3000** (as oriented in the figure) to the current location of the upper plate **5336** shown in solid line in the figure. The upper plate **5336** may be lowered farther to compress the device **3000**. The resulting compressive load as registered by the force gage **5334** as the upper plate **5336** is lowered may be recorded and plotted. The resulting plot of force versus amount of compression of the device **3000** may be the same or similar as the data plot **5200** shown in FIG. **100C**. In some embodiments, the resulting data plot using the test setup **5300** may be within $\pm 5\%$, $\pm 10\%$, $\pm 15\%$, $\pm 20\%$ or $\pm 25\%$ of the data points or line of best fit shown in FIG. **100C**.

[0525] The test setup **5300** may also be used to measure or approximate dimensions of the device **3000** as the device **300** is compressed. As described herein, for example with respect to FIGS. **99A-99B**, the minor and major axes of the device **3000** may be measured. The test setup **5300** may have dimensions located on the setup **5300** showing vertical and horizontal scales for determining the lengths of the major and minor axes of the device **300** as the device **3000** is compressed. In some embodiments, a separate measurement device, such as a ruler, may be used to measure the lengths. The resulting plot of minor (short) axis versus major (long) axis of the device **3000**, or parameters related thereto such as the mean diameter, may be the same or similar as the data plots **5000** and **5100** show respectively in FIGS. **100A-100B**. In some embodiments, the resulting data plots using the test setup **5300** may be within $\pm 5\%$, $\pm 10\%$, $\pm 15\%$, $\pm 20\%$ or $\pm 25\%$ of the data points or lines of best fit shown in FIGS. **100A-100B**.

[0526] FIG. **102** is a flow chart depicting an embodiment of a flat plate test method **5400**. The method **5400** may be performed using the test setup **5300**. The method **5400** may be performed to characterize the stiffness and other structural attributes of the device **3000**. The data plots **5000**, **5100**, **5200** in FIGS. **100A-100C** may be generated using the method **5400**. The method **5400** may thus be used for

determining whether a given embodiment of an occlusion device exhibits the same or similar structural characteristics as the device **3000**.

[0527] The method **5400** begins with step **5410** wherein the device **3000** is submerged in a bath or other volume of water, such as the volume **5310** having the water **5320**. The device **3000** may be submerged and placed onto a lower test plate, such as the lower plate **5332** having the force gage **5334**. The device **3000** may be submerged within the volume for a sufficient amount of time to equilibrate to the temperature within the volume of water. In some embodiments, the device **3000** may be submerged for one minute. In some embodiments, the device **3000** may be submerged for two, three, four, five or more minutes. The volume of water may be at a temperature of 37° C. (98.6° F.). The method **5400** may be performed at or near sea-level, or otherwise under sea-level conditions (e.g. sea-level atmospheric pressure). A thermometer may be used to determine the temperature at or near the device **3000**. A water heater and/or water recirculator, such as the thermal conditioner **5350** or recirculator **5360**, and/or other tools, may be used to achieve the desired temperature.

[0528] The method **5400** next moves to step **5420** wherein the device is secured on the compressive test apparatus, such as the test setup **5300**. The device **3000** may be placed and secured between the compressive test plates of the test setup. The distance between the two plates may be reduced. The upper plate **5336** may be lowered to contact and secure the device **3000** between the two plates. The upper plate **5336** may be lowered as shown in FIG. **101** to contact a side of the device **3000**. The initial compressive load on the device **3000** may be measured and recorded with just enough contact from the upper plate **5336** on the device **3000** to hold the device **3000** in position. This may be about 0.05 lbs.

[0529] The method **5400** next moves to step **5430** wherein the device **300** is compressed an incremental amount by reducing the distance between the plates an incremental amount. The upper plate **5336** may be lowered a first increment to compress the device **3000** radially inwardly. The upper plate **5336** may be moved 0.10". In some embodiments, a larger or smaller compressive increment may be used.

[0530] The method **5400** next moves to step **5440** wherein the resulting compressive force for the given incremental compression is measured and recorded. Thus the compressive load may be measured with the upper plate having been lowered 0.10" in step **5400**.

[0531] The method **5400** may next return to step **5430** and compress the device **3000** another incremental amount, after which step **5440** may be performed again to record the corresponding compressive load. Steps **5430** and **5440** may be repeated until a desired amount of compression is obtained. In some embodiments, steps **5430** and **5440** may be repeated at compressive increments of 0.10", 0.20", 0.30", 0.40", and 0.50". In some embodiments, the order of steps **5430** and **5440** as shown in FIG. **102** may be reversed. For example step **5440** may include applying a specified load (e.g. 0.05 lbs., 0.1 lbs., 0.15 lbs., 0.2 lbs., 0.25 lbs.) and step **5430** may include measuring the resulting compressive change in width, if any, of the device **3000** under each incremental given load. The method **5400** in this manner may be repeated for each incremental applied load.

[0532] The method **5400** may be repeated with the device **3000**. The device **3000** may be rotated an angular amount

and the method **5400** may be performed again. This may be repeated several times after completing the method **5400** as described. For example, the method **5400** may be performed a first time, then the device **300** may be rotated in first direction about its longitudinal axis sixty degrees, then the method **5400** may be repeated, then the device **3000** may be rotated in the first direction about the longitudinal axis another sixty degrees, and the method **5400** may be repeated. The load measurements during repeated tests at different angular amounts may be averaged for a given compression amount at a particular angle. In some embodiments, the averages of three measurements may be calculated, after initially testing the device **300** and then rotating the device **3000** by sixty degrees twice as described, and the resulting plot may be the same or similar as the data plot **5200** shown in FIG. **100C**. In some embodiments, the resulting data plot using the averages may be within +/-5%, +/-10%, +/-15%, +/-20% or +/-25% of the data points or line of best fit shown in FIG. **100C**.

O. Loading Tool with Ribs, Submersion, and Catheter Locking

[**0533**] FIGS. **103A** and **103B** are perspective and cross-section views, respectively, of an embodiment of a loading tool **3600**. The cross-section view of FIG. **103B** is taken along the line **103B-103B** as indicated in FIG. **103A**. The loading tool **3600** may have the same or similar features and/or functions as other loading tools described herein, such as the loading tool **3210**, and vice versa. The loading tool **3600** may be used with any of the embodiments of the LAA implant and related devices and systems described herein, such as the device **3000**, and vice versa.

[**0534**] As further described herein, the tool **3600** includes radially inwardly projecting ribs forming grooves therebetween, which among other things improves implant folding and helps align the barbs. Further, the tool **3600** includes a locking connection between the loader and catheter, to provide among other things a seal and eliminate gaps while assuring alignment (e.g., to prevent implant damage). Further, the tool **3600** is configured to hold fluid, so that among other things the implant can be fully submerged during loading, thus eliminating air bubbles from within the foam.

[**0535**] The loading tool **3600** includes a distal reservoir **3610** attached to a conical portion **3612**. A proximal projection **3614** attaches at a proximal end of the conical portion **3612**. The device **3000** is placed into the reservoir **3610** and pulled through the conical portion **3612** and then the projection **3614**. A delivery catheter is attached at the projection **3614** so that the device **3000** is constrained and delivered to the delivery catheter for implantation into the patient. For clarity, the reservoir **3610**, the conical portion **3612**, and the projection **3614** are shown as transparent in FIG. **103A**.

[**0536**] The conical portion **3612** includes ribs **3611**. The loading tool **3600** may include a plurality of internal guides such as at least four or ten or twenty or more axially oriented ribs **3611**. The ribs **3630** are formed between adjacent internal grooves **3631** formed on the inner surface of a conical portion **3612**. In one implementation, the grooves **3631** have a substantially constant width along their axial lengths, resulting in ribs **3611** having a width that increases in the distal direction as the inside diameter of the conical portion **3612** increases. The ribs **3630** may be longitudinally elongated, radially inwardly projecting structures located along the radially inwardly facing surface of the conical portion **3612**. Between adjacent ribs **3630** there may be one

of the internal grooves **3631** defined partially by the adjacent ribs **3611** and the inner surface of the conical portion **3612**. The ribs **3630** improve implant folding and help align the anchors **3090**, among other advantages. Such alignment may be through the foam sidewall of the implant, for example where the anchors **3090** press against the foam sidewall and occupy the grooves **3631** between the ribs **3611**. In some embodiments, some or all of the anchors **3090** may protrude through the foam sidewall of the implant to contact and be directly guided by the grooves **3631** and ribs **3630**. For clarity only some of the ribs **3611** and grooves **3631** are labelled in the figures.

[**0537**] The conical portion **3612** terminates at the distal end at a conical portion opening **3613**. The opening **3613** may open into the fluid reservoir **3610**. The fluid reservoir **3610** has a distal opening **3620** and an outwardly extending support flange **3650**. In some embodiments the location of the support flange **3650** may be different. The flange **3650** may extend outward in two opposite directions. The flange **3650** may secure the tool **3600** in an upright position on a table top for loading. The fluid reservoir **3610** may be defined within a housing having the distal opening **3620** and one or two or more stabilizing feet such as the transverse support flange **3650** for helping the loading tool **3600** to sit upright on a counter surface.

[**0538**] The reservoir **3610** is designed to hold fluid (e.g., saline) with the device **3000** also located therein so the implant can be fully submerged during loading, thus eliminating air bubbles from within the foam. In some embodiments the fluid reservoir **3610** may have a tubular, e.g., cylindrical side wall, with a closed base which incorporates a ramp such as a quarter-spherical portion to facilitate entry of the implant from the reservoir **3610** into the opening **3613**.

[**0539**] The distal opening **3620** of the fluid reservoir **3610** allows the device **3000** to be inserted into the loading tool **3600**. The reservoir **3610** is configured to receive the device **3000** therein, and the device **3000** may be oriented therein such that the proximal end of the device **3000** faces the conical portion **3612** and a sidewall of the device **3000** faces the proximal opening **3620** of the tool **3600**. For clarity, the tool **3600** in FIGS. **103A** and **103B** is shown without the device **3000** loaded therein.

[**0540**] The projection **3614** includes a sidewall **3618** that extends longitudinally away from the proximal end of the conical portion **3612** and defines a channel therethrough configured to receive a distal end of the delivery catheter therein. "Distal end" of the catheter here refers to the end of the catheter in the delivery context, where the distal end is advanced to the heart. The projection **3614** at a proximal end thereof includes a radially outwardly protruding lip **3617**. The lip **3617** projects outward and has a greater outer radius than the sidewall **3618**. The sidewall **3618** includes a series of longitudinal notches **3615**. There are four notches **3615** as shown, but there may be two, three, five, six, or more notches **3615**. The notches **3615** extend distally from the proximal end of the projection **3614**.

[**0541**] The loading tool **3600** may also include a lock **3640**. In FIGS. **103A-103B** the delivery catheter **3220** is shown as a dotted line for clarity. A proximally extending projection **3614** of the loading tool is configured to abut against or fit inside of the distal opening into the lumen of the delivery catheter to facilitate transfer of the implant. At least one or two or three or more axially extending slits **3615**

through the sidewall **3618** of the projection **3614** allow the inside diameter of the projection **3614** to adjust slightly in response to radial force from the compressed implant. The lock **3640** may include a sliding collar for sealing and aligning with the distal end of the delivery catheter **3220**. The collar is axially movable between a distal position as seen in FIG. **103A** to expose the proximal projection **3614** for mounting within the delivery catheter, and a proximal position in which it overlaps over the outside surface of the delivery catheter sidewall to reversibly support the connection. The lock may include grooves **3644** and ridges **3642** to provide a friction surface and improve user handling. The collar is configured to slide concentrically over the cylindrical portion **3614** and lock the delivery catheter **3220** between the projection **3614** and the collar. In some embodiments the projection **3614** may be cylindrical or a shape other than cylindrical.

[0542] In some embodiments, the lock **3640** may be a sliding cylindrical structure surrounding the projection **3614**, for sealing and aligning the catheter **3220**. The lock may include outer grooves **3644** defined between adjacent radially outwardly protruding ridges **3642**. For clarity only some of the ridges **3642** and grooves **3644** are labelled in the figures. The lock **3640** includes an inner channel **3645** extending longitudinally therethrough and defined by the sidewall of the lock **3640**. At a proximal end of the channel **3645** is a relatively wider opening **3646**. The opening **3646** is configured to surround the lip **3617** of the projection **3614** when the lock **3640** is slid to the proximal end of the projection **3614**.

[0543] In some embodiments, in a free state, where the lock is in the distal location as shown in FIGS. **103A** and **103B**, the projection **3614** has a wider inner diameter relative to the diameter when inward compressive forces are applied, so that the catheter can be easily inserted. The lock **3640** may then be slid proximally with the catheter inside the projection **3614**. The lock **3640** in a proximal location will cause the portions of the sidewall **3618** located adjacent the notches **3615** to move circumferentially closer to each other and to compress radially inwardly, to thereby reduce the inner diameter defined by the sidewall **3618**. The catheter tip will then be “sandwiched” by the inner surfaces of the sidewall **3618** to create radially inward securement forces acting on the catheter tip to secure the catheter. The opening **3646** may contact and secure therein the lip **3617** of the projection **3614** when the lock **3640** is slid to the proximal end of the projection **3614**. The inner diameter of the opening **3646** may be the same or less than the outer diameter of the lip **3617**, for example to create a compressive force thereon.

[0544] In some embodiments, in a free state, the outer surface of the sidewall **3618** may be tapered such that the outer surface has a greater outer width, e.g. radius or diameter, at a proximal end thereof (left end as oriented in the figures) as compared to a distal end thereof (right end as oriented in the figures). The lock **3640** may then be moved proximally and contact the outer surfaces of the sidewall **3618** to thereby decrease the inner diameter of the sidewall **3618**, as described. The lock **3640** is advantageous to provide a seal and eliminate gaps while assuring alignment of the catheter **3220** to the loading tool **3600**, among other advantages. For example, the seal, alignment and gap reduction serve to reduce the chance of the implant being damaged during loading. The tool **3600** and components thereof

may be made of plastic, polymer, metal, other suitable materials, or combinations thereof.

P. Delivery Catheter Handle

[0545] FIGS. **104A-104D** depict an embodiment of a delivery catheter handle **3700**. FIG. **104A** is a perspective view, FIG. **104B** is a cross-section view as taken along the line **104B-104B** indicated in FIG. **104A**, FIG. **104C** is a detailed partial cross-section view, and FIG. **104D** is a partial cross-section view of the handle **3700**. The handle **3700** may be used with the various LAA implants and associated devices and methods described herein. For example, the handle **3700** may be used to deliver the device **3000**. The loading tool **3600** may be used to load the device **3000** into a delivery catheter, which then may be used with the handle **3700** to deliver and secure the device **3000** within the human body.

[0546] The handle **3700** extends from a proximal end **3701** to a distal end **3702**. A main body **3703** attaches at a proximal end to a cap **3720** and at a distal end to a ribbed body **3760**. The ribbed body **3760** may be a tether control switch **3780**, as described with respect to FIGS. **105A-105C**. The cap **3720** attaches to a tether **3772** (see FIGS. **104C-104D**) and can be secured, for example screwed, to the proximal end of the body **3703**. Unsecuring, for example unscrewing, the cap **3720** allows for the tether **3772** to be pulled proximally after implantation of the device **3000**, to remove the tether from the delivery catheter. The tether **3772** may have the same or similar features and/or functions as other tethers or sutures described herein, for example the tether **3240**, and vice versa. For clarity, the tether **3772** is not shown in FIG. **104B**.

[0547] A locking mechanism **3740** includes a button **3741** that when depressed allows for axial movement of an internal shaft **3750**. When released, the button **3741** is spring-loaded via a pivot arm **3744**. Each arm **3744** pivots about a pin **3743**. There may be a torsion spring at each pin **3743** that bias the two arms **3744** toward the shaft **3750**. The shaft **3750** may be in the distal location as shown during implantation of the device **3000** and then moved proximally after implanting the device **3000** in the LAA, so that the pusher and/or delivery catheter can likewise be moved proximally prior to releasing the device **3000** from the tether **3000**. This removes the “snap back” effect of removing a pusher and/or delivery catheter from contacting LAA occlusion devices right after implantation in the LAA, in which the occlusion device may move slightly due to the backing off of the pusher.

[0548] The shaft **3750** locks in with the arms **3744** via protrusions **3745** on the arm **3744**, such as teeth, extending inwardly away from each arm **3744** and forming lateral grooves between adjacent protrusions **3745**. Corresponding lateral protrusions **3742** on the shaft **3750** extend outwardly away from the shaft **3750**. The protrusions **3742** of the shaft **3750** are received into grooves between corresponding protrusions **3745** of the arms **3744** when the shaft **3750** is in the proximal position as shown. When the shaft **3750** is advanced axially distally, the protrusions **3745** are received into grooves **3752** defined by protrusions **3751** at a proximal end of the shaft **3750**.

[0549] A tether **3772**, or suture, travels through the handle **3700** and wraps around a pin **3722** in a manner that incorporates a pulley-like effect so the tether **3772** only has to be pulled half the distance of the length of the catheter

during removal. The need to pull a suture the entire length of the catheter during removal is one of the disadvantages of using a suture as an attachment tether. This modification makes it less burdensome and more appealing to the user.

[0550] The handle 3700 may be configured to enable an operator to easily remove the tether 3772 from a patient. Specifically, during removal, the operator pulls the end cap portion 3720 proximally while holding the body 3703 fixed relative to the patient. As the cap 3720 moves proximally away from the body 3703, the tether 3772 feeds over the pin 3722. Since the tether 3772 is fixed to the body 3703 at a tether end 3710, all of the four tether segments 3772 elongate. The tether end 3710 may be secured to the body 3703 or other components therein in a variety of suitable manners, for example screwed, bonded, wrapped, other suitable approaches, or combinations thereof. The outcome of this elongation is that the tether 3772 portions inside the patient body translate twice as far as the cap 3720 translates. This phenomena is similar to a movable pulley arrangement used in reverse. The net effect of the system is to halve the applied force and double the length of the tether 3772 pulled. This reversed movable pulley arrangement is advantageous to reduce the pulled distance and applied force required to remove the tether 3772 from the patient, so the retraction of the tether from the patient may be at least about two times or four times or more the length of retraction of the proximal control. This makes the removal less arduous and time consuming for the operator.

[0551] The system arrangement includes, in some embodiments, a pulley in the form of the pin 3722, on which the tether 3772 is wrapped. The pin moves relative to the tether end 3710. Various embodiments are possible wherein the pin 3722 moves relative to the tether end 3710. Various such embodiments result in a pulley-like effect to reduce the total motion required to remove the tether 3772 from the patient. An arrangement with the pin 3722 and tether end 3710 is effective to reduce the total tether pull distance requirement by half.

[0552] In the example embodiment depicted in FIGS. 104A-104D, the cap 3720 is threaded onto the proximal end 3734 of the body 3703. The locking mechanism 3740 is coupled to the side of the body 3703, as described. The locking mechanism 3740 may include protrusions 3745 and can actuate to lock into the notches 3752 disposed on the inner shaft 3750. The inner shaft 3750 is fastened at the distal end 3754 to the ribbed body 3760, or in some embodiments to the tether control switch 3780 (shown in FIGS. 105A-105C). The ribbed body 3760 has a ribbed region 3762 and a cylindrical portion 3764. The tether 3772 extends through a central hole disposed through both the ribbed body 3760 and the inner shaft 3750. The body 3760 may be replaced with a tether control switch, such as a switch 3780 as described herein, for example with respect to FIGS. 105A-105C.

[0553] In the depicted embodiment, the notches 3752 interface with the protrusions 3742 when the locking mechanism 3740 is in the locked position. In the locked position, the relative positions of the inner shaft 3750 and the outer body 3730 are fixed. The locking mechanism 3740 can be actuated to allow relative motion between the inner shaft 3750 and the outer body 3750, as described.

[0554] FIGS. 105A-105D are various views of an embodiment of a tether control switch 3780 that may be used with the various LAA implant delivery handles, such as the

handle 3700 of FIGS. 104A-104D, and associated devices and systems, described herein. FIG. 105A is a side view, FIG. 105B is a partial side cross-section view, FIG. 105C is a partial view of some components of the switch 3780, and FIG. 105D is a bottom view of a slider 3786 used with the switch 3780.

[0555] The switch 3780 includes a body 3781 extending longitudinally from a proximal end 3784, that attaches to the delivery handle, to a distal end 3782 that receives the tether and the delivery catheter therein. A series of outwardly protruding grips 3788 extend outwardly away from the body 3781 for gripping the device. There may be seven grips 3788 as shown, or fewer or greater than seven grips 3788. The grips 3788 may be held by a user while a slider 3786 is moved axially along the body 3781.

[0556] The slider 3786 moves axially to selectively engage and disengage the tether 3772. As shown, in the proximal position (right as oriented), the slider 3786 is not engaged with the tether 3772, such that the tether can freely move through the switch 3780. When the slider 3786 is moved to the distal position (left as oriented), the slider 3786 is engaged with the tether 3772, such that the tether cannot freely move through the switch 3780. The switch 3780 includes a compression tube 3790 and pill 3792 to effectuate the engagement/disengagement of the tether 3772 via the slider 3786.

[0557] As shown in FIGS. 105B-105D, the slider 3786 has an inner ramped surface 3787 that is located farther from the longitudinal central axis of the switch 3780 at a proximal end and closer to the axis at a distal end. As the slider 3786 is moved proximally, the ramped surface 3787 applies an increasing force to the pill 3792, which then compresses the tube 3790 onto the tether 3772. The slider 3786 may be locked at the proximal and/or distal positions, for example to maintain the freedom or restriction of the movement of the tether 3772 therethrough. In some embodiments, the orientation of the ramped surface 3787 may be flipped to be in an opposite direction, such that the inner ramped surface 3787 is located farther from the longitudinal central axis of the switch 3780 at a distal end and closer to the axis at a proximal end. The tube 3790 may be formed of a foam or other compressible material. The pill 3792 may be relatively more rigid so as to transfer the force from the slider 3786 to the tube 3790. Further, with the tube 3790 compressed, fluid may be prevented from flowing through the switch 3780.

Q. Dual Lumen Pusher

[0558] FIGS. 106A-106C depict various views of various embodiments of a dual lumen delivery catheter pusher 3770 and 3800. Any of the features of the pusher 3700 may be implemented with the pusher 3800, and vice versa. FIG. 106A is an end view of an embodiment of the delivery catheter pusher 3770 with a two lumen shaft. A first lumen 3774 is separated from a second lumen 3772 by a wall 3776 extending therebetween. The first lumen 3774 is rounded, for example cylindrical. The second lumen 3772 is crescent or moon shaped. The cross-sectional opening of the second lumen 3772 may extend angularly about a central longitudinal axis of the pusher 3770 for about 30 degrees, about 45 degrees, about 60 degrees, about 90 degrees, from about 30 degrees to about 90 degrees, from about 30 degrees to about 60 degrees, or other amounts or ranges. During implant delivery, an obturator (e.g. a solid plastic tube) is placed

within the first lumen 3774 to stiffen the lumen 3774. The tether 3772 that attaches to the implant is in the second lumen 3772.

[0559] Following deployment of the implant, the clinician may remove the obturator and insert an intracardiac echo (ICE) catheter through the lumen 3772. This provides the clinician with direct access to the left atrium to visualize the implant 3000. This design is advantageous to allow the clinician to visualize the implant 3000 without the use of transesophageal echocardiography (TEE). TEE requires the use of general anesthesia. Administering general anesthesia increases risks to the patient and complicates the scheduling of the procedure.

[0560] Without the two shaft lumen, inserting an ICE catheter to visualize the implant would require a second transseptal puncture to access the left atrium. This is technically challenging and may increase the risk of leaving a residual iatrogenic atrial septal defect due to the extra catheter manipulation required with two sheaths crossing the atrial septum simultaneously. The second puncture also carries the inherent risk of cardiac perforation arising due to the use of sharp needles in the heart.

[0561] In various embodiments the shapes of the lumens and wall may vary. For example, FIG. 106B shows an embodiment of a pusher 3800 having semi-circular openings of approximately equal size. Other sizes and shapes of the lumens may be used in the pusher. The first lumen 3810 is divided from the second lumen 3812 by a wall 3820. In some embodiments the two sides could be the same size, or different sizes, the shapes could be a 'D' shape or other shapes. During implant delivery, an obturator (solid plastic tube) is placed within the first lumen 3810 to stiffen it. The tether 3772 that attaches to the implant is in the second lumen 3812.

[0562] FIG. 106C depicts the proximal end of an embodiment of a delivery catheter pusher 3800. Similar features may be implemented with the pusher 3700. The pusher 3800 has a bifurcation at the proximal end. At the bifurcation, the obturator containing lumen, or first lumen 3810, goes straight and the tether containing lumen, or second lumen is set at 45 degrees. After the bifurcation point 3822, the first lumen 3810 extends into a bifurcated first lumen 3814, and the second lumen 3812 extends into a bifurcated second lumen 3816. Delivery catheter pusher 3770 may be similarly bifurcated.

[0563] Various modifications to the implementations described in this disclosure will be readily apparent to those skilled in the art, and the generic principles defined herein can be applied to other implementations without departing from the spirit or scope of this disclosure. Thus, the disclosure is not intended to be limited to the implementations shown herein, but is to be accorded the widest scope consistent with the claims, the principles and the novel features disclosed herein. The word "example" is used exclusively herein to mean "serving as an example, instance, or illustration." Any implementation described herein as "example" is not necessarily to be construed as preferred or advantageous over other implementations, unless otherwise stated.

[0564] Certain features that are described in this specification in the context of separate implementations also can be implemented in combination in a single implementation. Conversely, various features that are described in the context of a single implementation also can be implemented in

multiple implementations separately or in any suitable sub-combination. Moreover, although features can be described above as acting in certain combinations and even initially claimed as such, one or more features from a claimed combination can in some cases be excised from the combination, and the claimed combination can be directed to a sub-combination or variation of a sub-combination.

[0565] Similarly, while operations are depicted in the drawings in a particular order, this should not be understood as requiring that such operations be performed in the particular order shown or in sequential order, or that all illustrated operations be performed, to achieve desirable results. Additionally, other implementations are within the scope of the following claims. In some cases, the actions recited in the claims can be performed in a different order and still achieve desirable results.

[0566] It will be understood by those within the art that, in general, terms used herein are generally intended as "open" terms (e.g., the term "including" should be interpreted as "including but not limited to," the term "having" should be interpreted as "having at least," the term "includes" should be interpreted as "includes but is not limited to," etc.). It will be further understood by those within the art that if a specific number of an introduced claim recitation is intended, such an intent will be explicitly recited in the claim, and in the absence of such recitation no such intent is present. For example, as an aid to understanding, the following appended claims may contain usage of the introductory phrases "at least one" and "one or more" to introduce claim recitations. However, the use of such phrases should not be construed to imply that the introduction of a claim recitation by the indefinite articles "a" or "an" limits any particular claim containing such introduced claim recitation to embodiments containing only one such recitation, even when the same claim includes the introductory phrases "one or more" or "at least one" and indefinite articles such as "a" or "an" (e.g., "a" and/or "an" should typically be interpreted to mean "at least one" or "one or more"); the same holds true for the use of definite articles used to introduce claim recitations. In addition, even if a specific number of an introduced claim recitation is explicitly recited, those skilled in the art will recognize that such recitation should typically be interpreted to mean at least the recited number (e.g., the bare recitation of "two recitations," without other modifiers, typically means at least two recitations, or two or more recitations). Furthermore, in those instances where a convention analogous to "at least one of A, B, and C, etc." is used, in general such a construction is intended in the sense one having skill in the art would understand the convention (e.g., "a system having at least one of A, B, and C" would include but not be limited to systems that have A alone, B alone, C alone, A and B together, A and C together, B and C together, and/or A, B, and C together, etc.). In those instances where a convention analogous to "at least one of A, B, or C, etc." is used, in general such a construction is intended in the sense one having skill in the art would understand the convention (e.g., "a system having at least one of A, B, or C" would include but not be limited to systems that have A alone, B alone, C alone, A and B together, A and C together, B and C together, and/or A, B, and C together, etc.). It will be further understood by those within the art that virtually any disjunctive word and/or phrase presenting two or more alternative terms, whether in the description, claims, or drawings, should be understood to contemplate the possibilities of

including one of the terms, either of the terms, or both terms. For example, the phrase “A or B” will be understood to include the possibilities of “A” or “B” or “A and B.”

What is claimed is:

1. A conformable left atrial appendage occlusion device, comprising:

an expandable tubular body having a compressible open cell foam sidewall, a proximal, occlusive end for facing a left atrium following implantation of the device in a left atrial appendage, a distal end for facing into the left atrial appendage following implantation of the device in the left atrial appendage, and a longitudinal axis extending therethrough, the tubular foam body having a mean diameter in an unconstrained expansion; and

a self-expandable support carried within the expandable tubular body such that the foam sidewall provides a cushion between the support and the wall of the left atrial appendage following implantation, the support comprising a plurality of struts forming a plurality of apexes;

wherein compression of the device from a diameter of about 25 mm to a diameter of about 15 mm along a minor axis transverse to the longitudinal axis causes no more than about a 5 mm reduction in the mean diameter.

2. The conformable left atrial appendage occlusion device of claim 1, wherein compression of the device from a diameter of about 25 mm to a diameter of about 15 mm along a minor axis transverse to the longitudinal axis causes no more than about a 2 mm reduction in the mean diameter.

3. The conformable left atrial appendage occlusion device of claim 1, wherein the support comprises a plurality of distally facing apexes, and the tubular foam body extends distally beyond the distal apexes to provide an atraumatic distal bumper.

4. The conformable left atrial appendage occlusion device of claim 1, wherein the expandable body can be compressed within a delivery catheter having an inside diameter of no more than about 20 F and can self-expand to a diameter of at least about 25 mm when released from the delivery catheter.

5. The conformable left atrial appendage occlusion device of claim 1, wherein application of 0.10 lbs compressive force along a minor axis transverse to the longitudinal axis produces a compression of at least about 0.10 inches along the minor axis.

6. The conformable left atrial appendage occlusion device of claim 1, wherein application of 0.20 lbs compressive

force along the minor axis produces a compression of at least about 0.15 inches along the minor axis.

7. The conformable left atrial appendage occlusion device of claim 1, further comprising at least one anchor coupled with the support and extending at least partially into the tubular foam body.

8. The conformable left atrial appendage occlusion device of claim 1, wherein the side wall has an uncompressed thickness of at least about 0.5 mm.

9. The conformable left atrial appendage occlusion device of claim 1, wherein the side wall extends in a distal direction beyond a distal end of the support by at least about 2 mm in an unconstrained, expanded state.

10. The conformable left atrial appendage occlusion device of claim 1, wherein the side wall comprises a foam having a plurality of interconnected reticulations and voids, and further comprising a PTFE coating on at least some of the interconnected reticulations.

11. The conformable left atrial appendage occlusion device of claim 1, wherein the occlusive end further comprises a cover.

12. The conformable left atrial appendage occlusion device of claim 11, wherein the cover comprises ePTFE.

13. The conformable left atrial appendage occlusion device of claim 1, wherein the expandable support is within a central cavity enclosed by the foam side wall.

14. The conformable left atrial appendage occlusion device of claim 1, wherein the support further comprises at least three recapture struts inclining radially inwardly in the proximal direction to a hub.

15. The conformable left atrial appendage occlusion device of claim 14, comprising at least six proximally facing apexes and at least six distally facing apexes.

16. The conformable left atrial appendage occlusion device of claim 15, wherein each recapture strut is joined to a unique proximally facing apex on the support.

17. The conformable left atrial appendage occlusion device of claim 14, wherein the recapture struts are integrally formed with the support.

18. The conformable left atrial appendage occlusion device of claim 1, wherein the foam sidewall comprises a reticulated, cross linked matrix having at least about 90% void content, an average pore size within the range of from about 250-500 microns, a wall thickness of at least about 2 mm and a compressive strength of at least about 1 psi.

19. The conformable left atrial appendage occlusion device of claim 1, wherein the compressive strength is within a range of from about 1 psi to about 2 psi.

* * * * *