



# Endoscopy

**Boston  
Scientific**

Advancing science for life™

## 2020 Reference Guide





# We're all in.

Because you're all in on delivering optimal patient care, we've made it our specialty to support yours. From clinical research and education to devices for gastrointestinal and pulmonary conditions that are changing the standard of care, we work with you to help solve the challenges that matter most to you and your patients.


Visit [bostonscientific.com/gastro](http://bostonscientific.com/gastro) to learn more about:

- Products
- Education & Training
- Ordering Information
- Solutions
- ACCESS Magazine Online



<sup>1</sup>Product with this symbol may be used in Magnetic Resonance environment according to the conditions described in Directions for Use.

# Resection & Retrieval

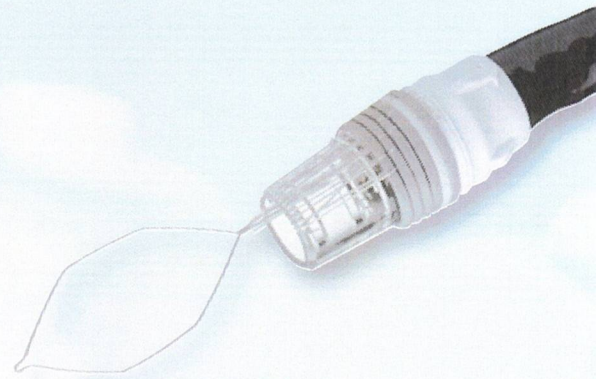

## Resection Devices

### EMR for Upper GI

- ▶ Captivator™ EMR Device ..... 75

### Stiff Snares

- ▶ Captivator COLD Single-Use Snares ..... 75
- ▶ Captivator II Single-Use Snares ..... 76
- ▶ Captivator Single-Use Snares ..... 76

### Specialty Snares

- ▶ Profile™ Single-Use Snares ..... 77
- ▶ Single-Use Rotatable Snares ..... 77

### Snares

- ▶ Captiflex™ Single-Use Snares ..... 78
- ▶ Sensation™ Single-Use Short Throw Snares ..... 78

### Active Cords

- ▶ Active Cords ..... 79

### Submucosal Lifting

- ▶ ORISE™ Gel ..... 79

## Retrieval Devices

### Retrieval Device

- ▶ RescueNet™ Retrieval Device ..... 80

### Retrieval Grasping Forceps


- ▶ Rescue™ Rat Tooth Grasping Forceps ..... 80
- ▶ Rescue Rat Tooth Grasping Forceps - Pediatric ..... 80
- ▶ Rescue Alligator Grasping Forceps, Long ..... 80
- ▶ Rescue Alligator Grasping Forceps ..... 80
- ▶ Rescue Rat Tooth / Alligator Grasping Forceps ..... 80

### Polyp Traps

- ▶ TrapEase™ Single Chamber Polyp Trap ..... 80
- ▶ TrapEase Quad Chamber Polyp Trap ..... 80

# Retrieval Devices

## Retrieval Device

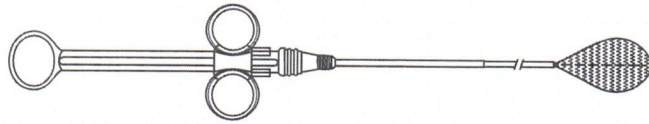


### RescueNet™ Retrieval Device



Order Number	GTIN	Description	Net Size (mm)	Sheath O.D. (mm)	Minimum Working Channel (mm)	Working Length (cm)	Packaging
DGN-538-5	10840253107425	RescueNet Retrieval Device	30	2.5	2.8	230	Box 5

## Retrieval Grasping Forceps

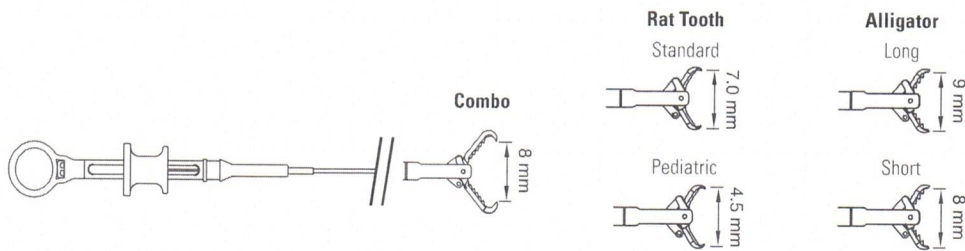

### Rescue™ Retrieval Single-Use Grasping Forceps



Order Number	GTIN	Description	Jaw Opening Width (mm)	Sheath O.D. (mm)	Minimum Working Channel (mm)	Working Length (cm)	Packaging
M00527651	26948318968637	Rescue Rat Tooth Grasping Forceps	7	2.4	2.8	230	Box 5
M00527751	26948318968644	Rescue Rat Tooth Grasping Forceps - Pediatric	4.5	1.8	2.0	180	Box 5
M00527551	26948318968620	Rescue Alligator Grasping Forceps, Long	9	2.4	2.8	230	Box 5
M00527451	26948318968613	Rescue Alligator Grasping Forceps	8	2.4	2.8	230	Box 5
M00527351	26948318968606	Rescue Rat Tooth / Alligator Grasping Forceps	8	2.4	2.8	230	Box 5

## Polyp Traps



### TrapEase™ Polyp Traps

Order Number	GTIN	Description	Packaging
STE-297-50	00816849010182	TrapEase Single Chamber Polyp Trap	Box 50
STE-298-25	00816849010199	TrapEase Quad Chamber Polyp Trap	Box 25



Section Table of Contents

Prev Page ◀ 80 ▶ Next Page

Main Table of Contents



For pricing information contact your Boston Scientific Sales Representative or Customer Service at 1.888.272.1001

# Certain Terms and Conditions

## Ordering Information

All orders should be placed directly with Boston Scientific Endoscopy Customer Service by mail, telephone, fax or Electronic Data Interchange (EDI).

Boston Scientific Endoscopy  
500 Commander Shea Blvd.  
Quincy, MA 02171  
(888) 272-1001 Phone  
(888) 272-9444 Fax  
(877) 272-3340 EDI

Please contact EDI if interested in ordering your endoscopy products via the internet.  
Please note that the above address is our mailing address only.

Customer Service is available between the hours of 8:30 am and 9:30 pm (Eastern Standard Time) weekdays excluding national holidays. Our toll-free fax number, (888) 272-9444, is available at all times. In addition, technical and emergency service is available 24 hours a day, 7 days a week, call (888) 272-1001 for further instructions.

### Standing Orders

Boston Scientific Endoscopy accepts standing orders on all products. This convenience provides you with scheduled shipments using a single purchase order. Contact the Customer Service Database Department at (888) 325-1060 for details.

### Terms

Terms are Net 30 Days. All shipments are F.O.B. Quincy, Massachusetts. Prices are subject to change without notice.

### Returned Goods

Permission to return merchandise is required for all returns and, except as provided herein, may be withheld in the sole discretion of Boston Scientific Endoscopy. This authorization must be requested by calling or writing:

Customer Service  
Boston Scientific Endoscopy  
500 Commander Shea Blvd.  
Quincy, MA 02171  
(800) 862-1284

#### The request for authorization must include:

- Reason for the return – "Ordered in Error," "Shipped in Error," etc.
- Catalog number, size, quantity, lot number
- Purchase order number, Boston Scientific Endoscopy invoice number and date of invoice

All merchandise returned to Boston Scientific Endoscopy must be accompanied by a copy of the packing slip or invoice enclosed with the original shipment. The Returned Goods Authorization (RGA) number must be clearly marked on the shipping container. Merchandise returned without an RGA number will not be accepted or considered as returned product.

#### Merchandise that will not be accepted for return:

- Expired product or products with less than 6 months shelf life
- Merchandise manufactured as SPECIALS or CUSTOM
- Merchandise in unsaleable condition (opened, damaged, tampered, etc.)
- Merchandise not listed in this Price List or any Supplement
- Merchandise sterilized or used by customer
- Merchandise that is not packaged properly for shipping when returned
- Incomplete kits or boxes (unless defective)
- Unauthorized returns



# Certain Terms and Conditions

## Returned Goods (continued)

### Allowance Schedule for Authorized Returns:

#### Allowance Schedule for Capital Equipment:

- Capital Equipment processed in error by Boston Scientific Endoscopy will receive full credit if returned in saleable condition
- Capital Equipment cannot be returned once the customer has taken title of the equipment

#### Allowance Schedule for Metal and Polyflex™ Stents and Alair™ Bronchial Thermoplasty Products:

- Merchandise processed in error by Boston Scientific Endoscopy will receive full credit if returned in saleable condition
- Merchandise returned within 30 days of invoice date in saleable condition will receive 100% credit
- Merchandise returned from 31 days to 90 days in saleable condition will receive full credit less a 30% restocking charge
- Merchandise returned from 91 days to 150 days in saleable condition will receive full credit less a 50% restocking fee
- Merchandise returned past 150 days will not receive any credit

#### Allowance Schedule for All Other Products:

- Merchandise processed in error by Boston Scientific Endoscopy will receive full credit if returned in saleable condition
- Other merchandise returned within 30 days of invoice date in saleable condition will receive full credit less a 15% restocking charge
- Merchandise returned past 31 days in saleable condition will receive full credit less a 40% restocking charge provided there is at least 6 months left on the expiration date

## Pricing and Specification Changes

As we are continually introducing products and improving our existing products, this Price List does not purport to be complete, and the equipment supplied may not agree in all details with the description and specifications shown in the catalog and / or price list. All product offerings, prices and specifications are subject to change without notice.

## Notice

Indications, contraindications and instructions for use, as well as product warranty information, if applicable, can be found in the product labeling supplied with each device. Caution: Federal law restricts this device to sale by or on the order of a physician.

## Warning Re: Single-Use Devices

Products marked as "single-use" are for single use only. Do not reuse, reprocess or resterilize single-use products. Reuse, reprocessing or resterilization may compromise the structural integrity of the device and / or lead to device failure which in turn may result in patient injury, illness or death. Reuse, reprocessing or resterilization may also create a risk of contamination of the device and / or cause patient infection or cross-infection, including, but not limited to, the transmission of infectious disease(s) from one patient to another. Contamination of the device may lead to injury, illness or death of the patient. **BSC assumes no liability with respect to single-use devices reused, reprocessed or resterilized and makes no warranties, express or implied, including, but not limited to, any implied warranties of merchantability or fitness for a particular purpose, with respect to any such instrument.**

©2020 Boston Scientific Corporation or its Affiliates. All rights reserved.

### INDICATIONS FOR USE

The WallFlex™ Biliary RX Fully Covered Stent System RMV is indicated for use in the palliative treatment of biliary strictures produced by malignant neoplasms, relief of malignant biliary obstruction prior to surgery and for indwell up to 12 months in the treatment of benign biliary strictures secondary to chronic pancreatitis.

### LIMITATIONS

The sale, distribution, and use of the device are restricted to prescription use in accordance with 21 CFR §801.109.

### Contraindications:

- The WallFlex Biliary RX Fully Covered Stent System RMV should not be placed in strictures that cannot be dilated enough to pass the delivery system, in a perforated duct, or in very small intrahepatic ducts.
- The WallFlex Biliary RX Fully Covered Stent System RMV should not be used in patients for whom endoscopic techniques are contraindicated.

### Warnings:

- The safety and effectiveness of the stent for benign stricture treatment has not been established for indwell periods exceeding 12 months.
- The WallFlex Biliary RX Fully Covered Stent System RMV is for single-use only.
- The safety and effectiveness of the WallFlex Biliary RX Fully Covered Stent System RMV for use in the vascular system has not been established.
- Clinical Study was not able to demonstrate that the use of this device is safe and effective in the treatment of benign biliary post liver transplantation anastomotic strictures and of benign biliary post abdominal surgery strictures.
- Testing of overlapped stents has not been conducted.
- The stent contains nickel, which may cause an allergic reaction in individuals with nickel sensitivity.

**PLEASE REFER TO THE LABELING FOR A MORE COMPLETE LIST OF WARNINGS, PRECAUTIONS AND CONTRAINDICATIONS.**



Section Table of Contents

Prev Page ◀ 114 ▶ Next Page

Main Table of Contents



For pricing information contact your Boston Scientific Sales Representative or Customer Service at 1.888.272.1001

## Customer Ordering Information

### Universal Product Number

#### Radial Jaw™ 4 Single-Use Jumbo Biopsy Forceps

Order Number	GTIN	Description
M00513343	08714729761891	Radial Jaw 4 Jumbo Forceps
M00513353	08714729761907	Radial Jaw 4 Jumbo Forceps
M00513363	08714729761914	Radial Jaw 4 Jumbo Forceps
M00513373	08714729761938	Radial Jaw 4 Jumbo Forceps
M00513361	08714729648871	Radial Jaw 4 Jumbo Forceps
M00513371	08714729648895	Radial Jaw 4 Jumbo Forceps
<b>M00513362</b>	08714729648888	Radial Jaw 4 Jumbo Forceps

**Order Number**  
is old order number

For customer convenience, the Boston Scientific Endoscopy ordering system accepts the UPN (Universal Product Number) e.g., **M00513362** found on product labeling as well as Boston Scientific's old 4 digit order numbers e.g., **1336**.

Please use either one of these numbers when placing an order via phone, fax, internet, or Electronic Data Interchange (EDI).

For those customers who scan product today, Boston Scientific is moving to the GS1 GTIN barcode and labeling standards as part of our ongoing commitment to improve supply chain efficiency. For more information go to the website: [www.bostonscientific.com/GS1](http://www.bostonscientific.com/GS1).

Boston Scientific Endoscopy Customer Service Representatives will be happy to help you with any questions. We are eager to make the ordering procedure as simple and efficient as possible.



Section Table of Contents

Prev Page ◀

▶ Next Page

Main Table of Contents



The paper used for  
this product catalog  
has been produced in  
accordance with:



<sup>1</sup>Product with this symbol may be used in Magnetic Resonance environment according to the conditions described in Directions for Use.

All trademarks are the property of their respective owners.

**Boston  
Scientific**  
Advancing science for life™

Boston Scientific Corporation  
300 Boston Scientific Way  
Marlborough, MA 01752-1234  
[www.bostonscientific.com](http://www.bostonscientific.com)

**Ordering Information**  
**1.888.272.1001**

©2020 Boston Scientific Corporation  
or its affiliates. All rights reserved.

ENDO-736702-AA P