

Essential Medical™
Closure Evolved



MANTA™
Vascular Closure Device

18F



(01)00856279007017(17)200422(10)SAMPLE

REF

2115NE

(Catalog Number)



2020-04-22

(Use By)

CE
0086

LOT

SAMPLE

(Lot Number)



(Do Not Re-Sterilize)



(Do Not Re-Use)

STERILE R

(Sterilized using Irradition)



(Consult Instructions for use)



(Keep Away from Sunlight)



(Keep Dry)



(MR Conditional)



(Do Not Use if Package is Damaged)

15°C 49°C
(Store Product Between 15°C - 49°C)

Essential Medical, Inc
260 Sierra Dr., Suite 120
Exton, PA 19341 USA

EC REP

MedPass SAS
95b Boulevard Pereire
75017 - Paris
France


Contents: 5

P/N: 2180-3 Rev. D



MANTA™
Vascular Closure Device

Essential Medical
Closure Evolved

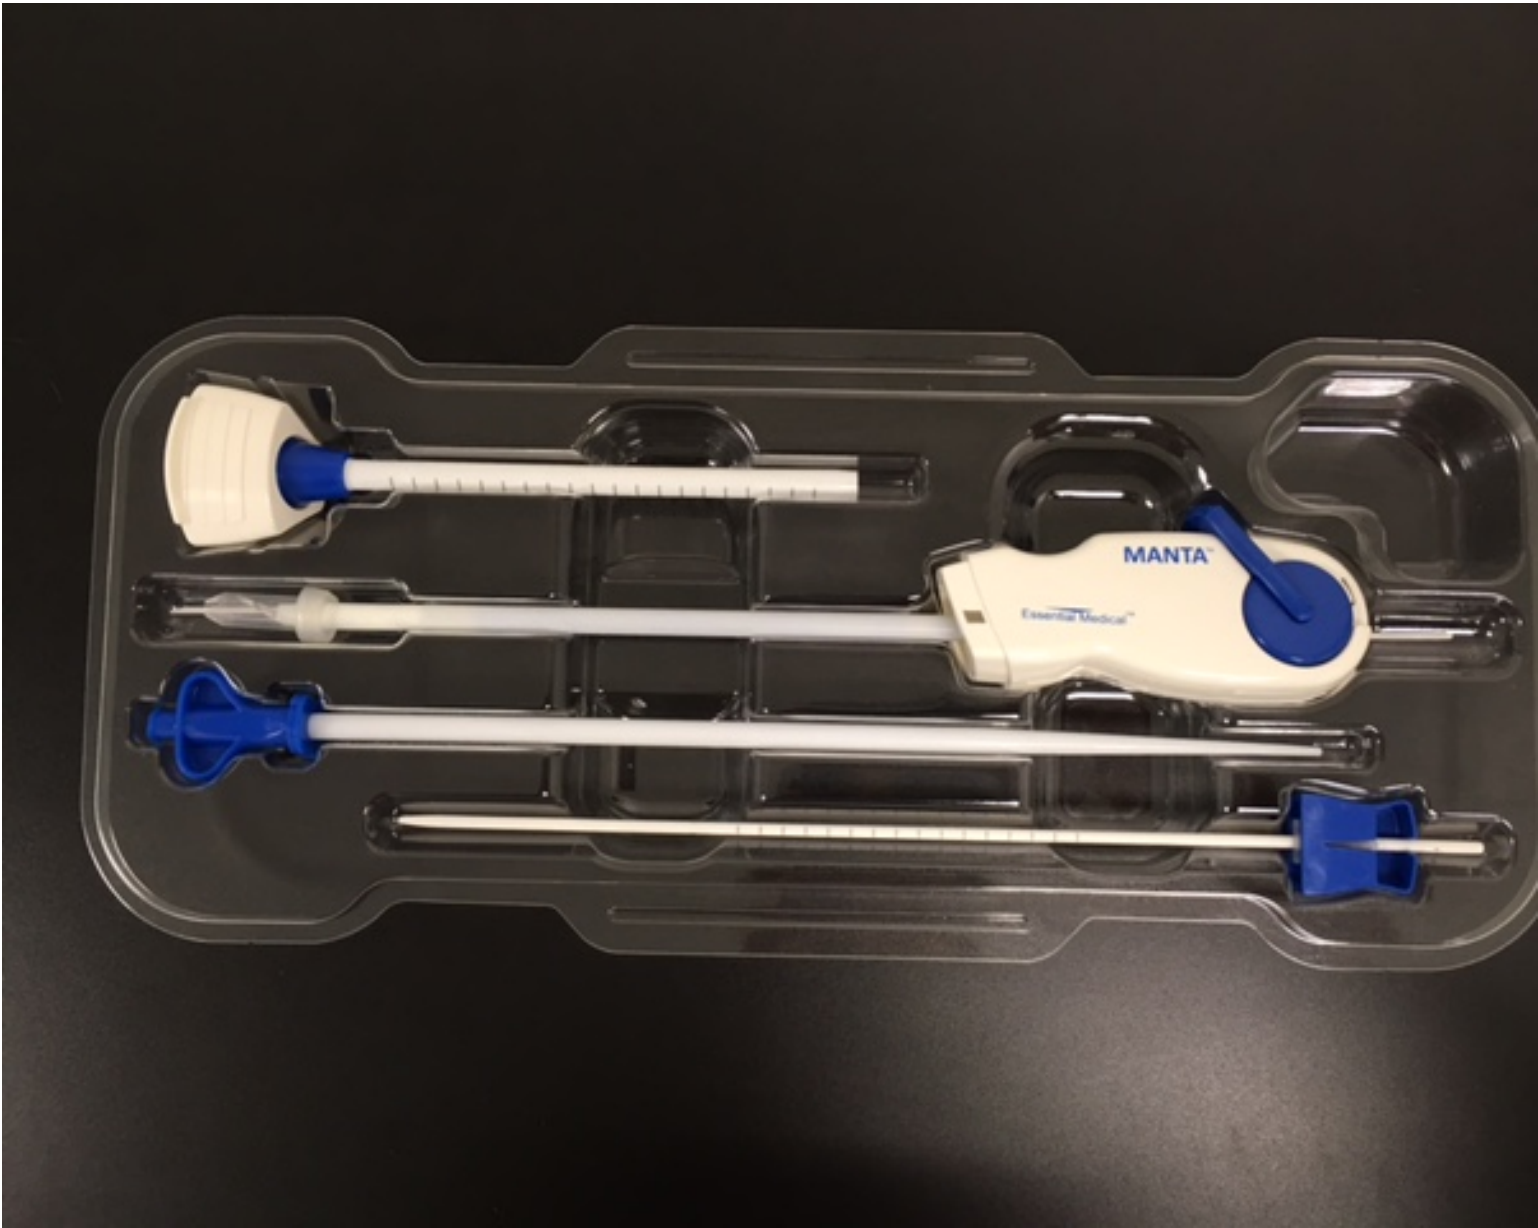

Essential Medical™
Closure Evolved



MANTA™
Vascular Closure Device

18F



(01)00856279007017(17)200422(10)SAMPLE

REF 2115NE
(Catalog Number)

2020-04-22
(Use By)

CE
0086

LOT SAMPLE
(Lot Number)

2
(Do Not Re-Sterilize)

2
(Do Not Re-Use)

STERILE R
(Sterilized using Irradition)

i
(Consult Instructions for use)

15°C - 49°C
(Store Product Between 15°C - 49°C)

☀
(Keep Away from Sunlight)

☂
(Keep Dry)

MR
(MR Conditional)

⊗
(Do Not Use if Package is Damaged)

Essential Medical, Inc
260 Sierra Dr., Suite 120
Exton, PA 19341 USA

EC REP MedPass SAS
95b Boulevard Pereire
75017 - Paris
France

Contents: 5

P/N: 2180-3 Rev. D



MANTA™
Vascular Closure Device

Essential Medical
Closure Evolved